

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
 Data File : VV037420.D
 Acq On : 20 Sep 2024 10:11
 Operator : SY/MD
 Sample : P3994-05DL 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B21DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV037420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	84	rVB	92930	94571	4.17%	0.839%
2	1.529	145	152	166	rVB	122712	138374	6.10%	1.227%
3	2.053	306	315	336	rVB2	207187	316033	13.93%	2.803%
4	2.445	426	437	450	rBV3	14332	26831	1.18%	0.238%
5	3.809	844	861	903	rBV4	155852	586790	25.87%	5.205%
6	4.240	978	995	1020	rBV	174522	467651	20.62%	4.148%
7	4.950	1199	1216	1250	rBV3	387184	1013790	44.70%	8.992%
8	5.529	1385	1396	1422	rBV	343125	746793	32.93%	6.624%
9	5.825	1474	1488	1526	rBV	1108364	2268055	100.00%	20.118%
10	5.982	1526	1537	1559	rVV	229714	486553	21.45%	4.316%
11	6.915	1815	1827	1854	rBV2	72500	163202	7.20%	1.448%
12	7.239	1916	1928	1957	rBV	404156	771621	34.02%	6.844%
13	7.558	2018	2027	2051	rBV2	38819	90622	4.00%	0.804%
14	7.905	2125	2135	2149	rVB3	18211	34431	1.52%	0.305%
15	8.024	2162	2172	2211	rBV	486534	1101414	48.56%	9.770%
16	8.780	2397	2407	2442	rBV	558888	977412	43.09%	8.670%
17	10.149	2820	2833	2859	rBV	195782	331748	14.63%	2.943%
18	11.181	3143	3154	3179	rBV	533230	900703	39.71%	7.989%
19	11.554	3259	3270	3293	rBV	450315	757189	33.38%	6.716%




Sum of corrected areas: 11273783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037420.D
Acq On : 20 Sep 2024 10:11
Operator : SY/MD
Sample : P3994-05DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

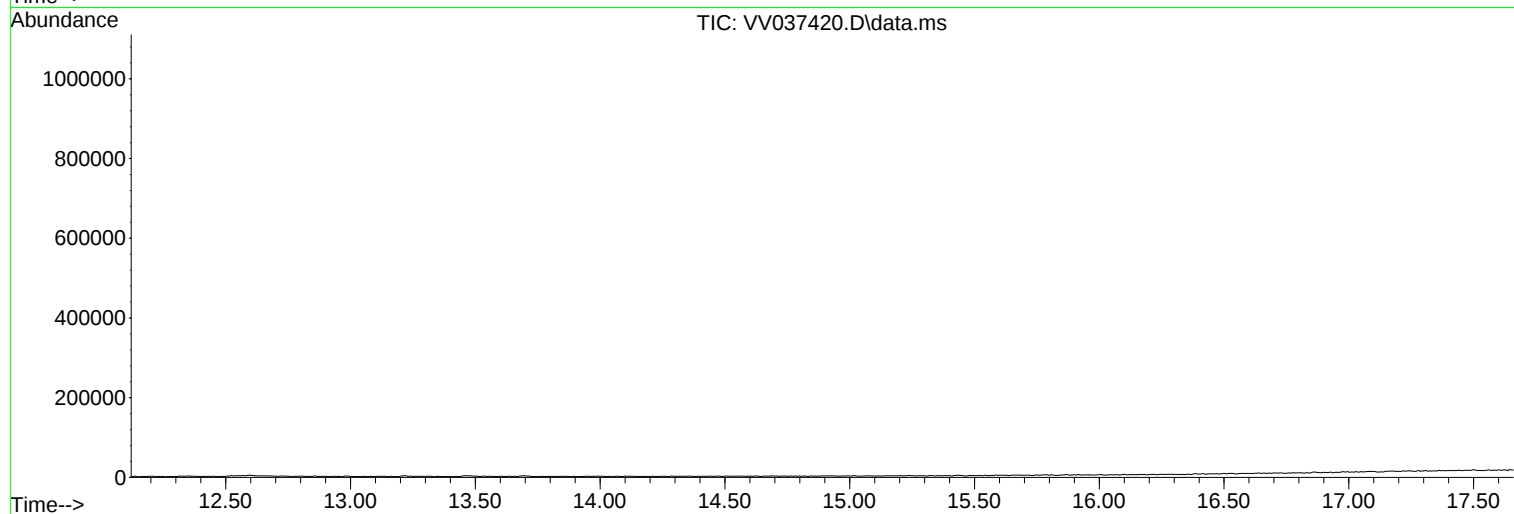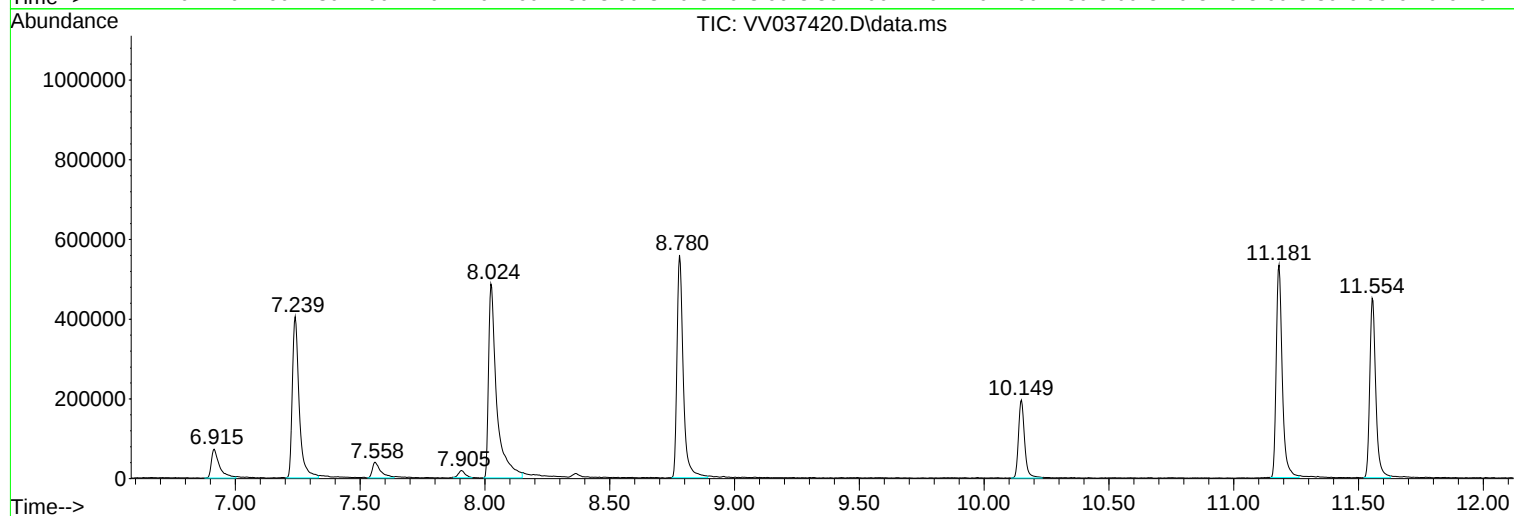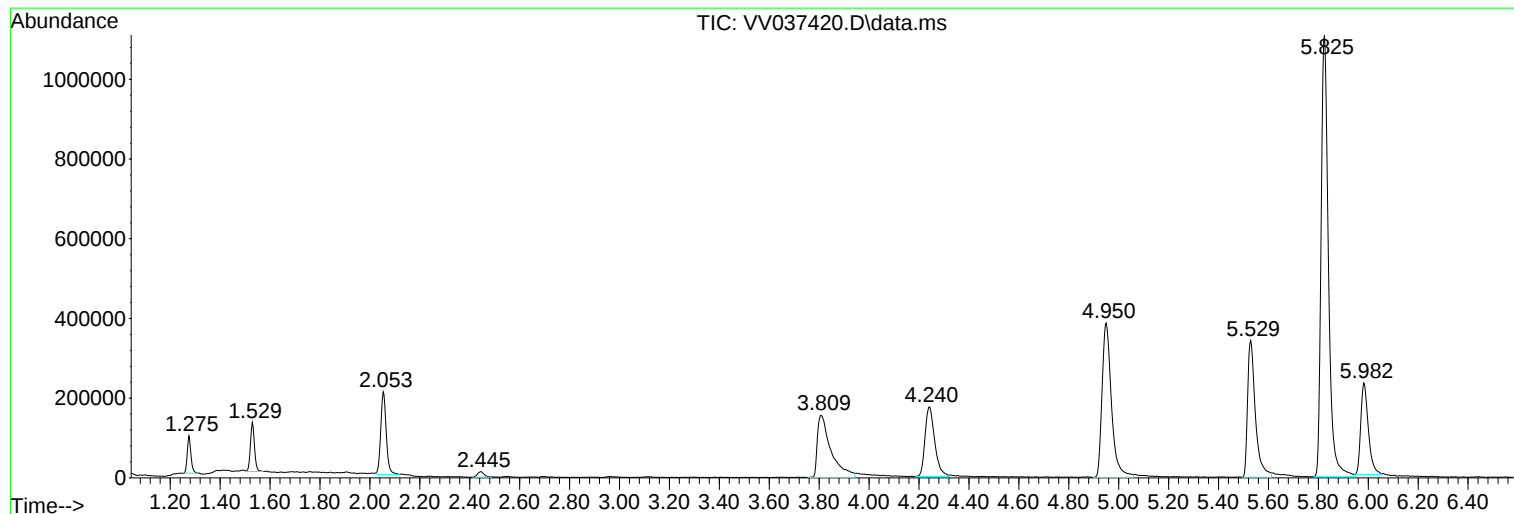

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037420.D
Acq On : 20 Sep 2024 10:11
Operator : SY/MD
Sample : P3994-05DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037420.D
Acq On : 20 Sep 2024 10:11
Operator : SY/MD
Sample : P3994-05DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc