

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
 Data File : VV037423.D
 Acq On : 20 Sep 2024 11:23
 Operator : SY/MD
 Sample : P3988-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV037423.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	46	54	62	rBV2	12237	18746	1.68%	0.219%
2	1.275	66	73	88	rVV	133018	146117	13.11%	1.705%
3	1.529	145	152	167	rVB	121896	146517	13.14%	1.709%
4	2.053	305	315	335	rVB	238260	357976	32.12%	4.176%
5	2.442	427	436	453	rVB3	10186	20825	1.87%	0.243%
6	3.834	858	869	894	rBV2	70411	304586	27.33%	3.553%
7	4.243	980	996	1020	rBV	162449	434428	38.98%	5.068%
8	4.953	1203	1217	1249	rBV2	378399	988983	88.73%	11.537%
9	5.532	1381	1397	1429	rBV	307429	689660	61.87%	8.045%
10	5.847	1481	1495	1499	rBV	8220	12734	1.14%	0.149%
11	5.985	1526	1538	1565	rBV	215173	479374	43.01%	5.592%
12	6.915	1818	1827	1851	rBV	79844	175295	15.73%	2.045%
13	7.239	1917	1928	1966	rBV	421833	809899	72.66%	9.448%
14	7.561	2020	2028	2043	rBV2	42816	89151	8.00%	1.040%
15	7.866	2116	2123	2136	rVB4	6476	13215	1.19%	0.154%
16	8.027	2163	2173	2231	rBV	452503	1114626	100.00%	13.003%
17	8.783	2397	2408	2435	rBV	502371	884991	79.40%	10.324%
18	10.149	2822	2833	2852	rBV	185160	311910	27.98%	3.639%
19	10.320	2877	2886	2901	rVB4	10217	17481	1.57%	0.204%
20	11.181	3142	3154	3179	rBV	489111	821085	73.66%	9.579%
21	11.554	3259	3270	3295	rBV	433443	734450	65.89%	8.568%




Sum of corrected areas: 8572049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037423.D
Acq On : 20 Sep 2024 11:23
Operator : SY/MD
Sample : P3988-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

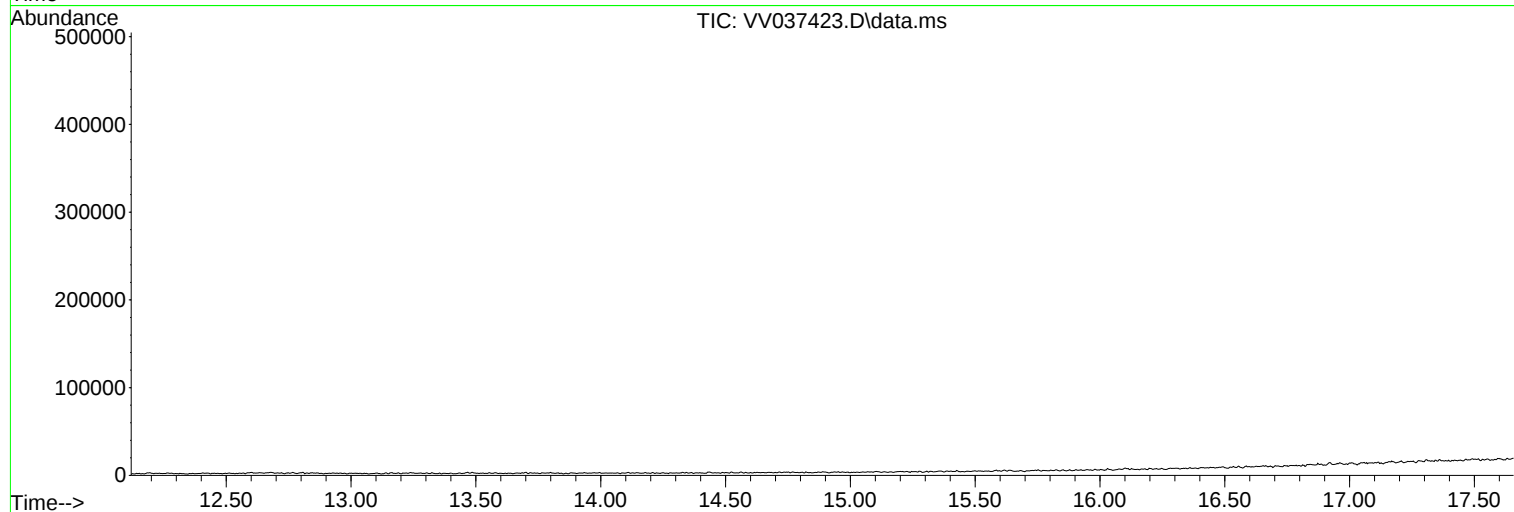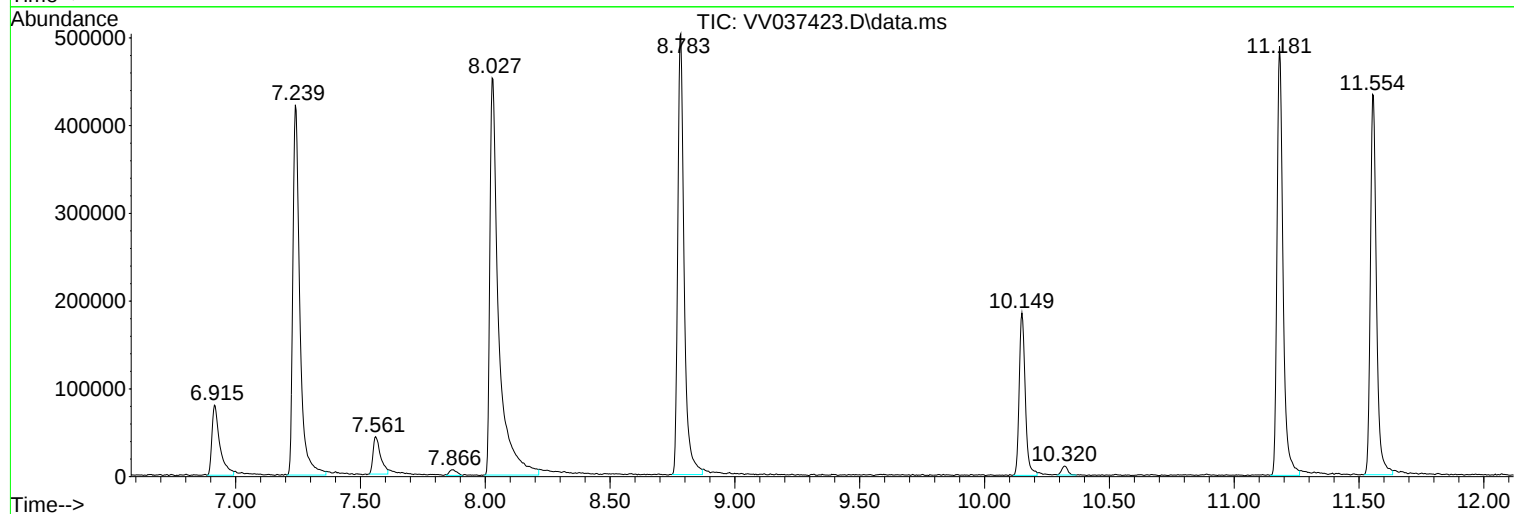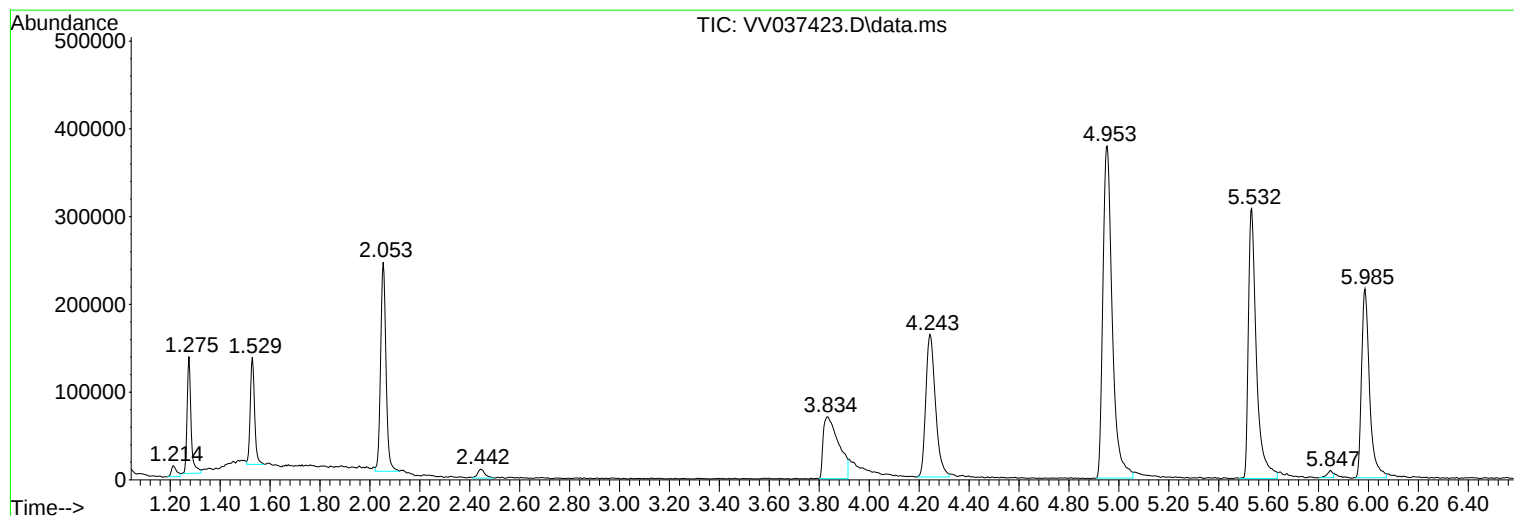

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037423.D
Acq On : 20 Sep 2024 11:23
Operator : SY/MD
Sample : P3988-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037423.D
Acq On : 20 Sep 2024 11:23
Operator : SY/MD
Sample : P3988-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc