

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
 Data File : VV037427.D
 Acq On : 20 Sep 2024 13:00
 Operator : SY/MD
 Sample : P3994-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B44

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV037427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.211	41	53	56	rBV3	13577	26409	2.29%	0.300%
2	1.275	66	73	87	rVB	91818	101659	8.80%	1.156%
3	1.381	94	106	116	rBV3	17798	49434	4.28%	0.562%
4	1.529	145	152	168	rVB	118240	139853	12.11%	1.591%
5	2.053	305	315	331	rVB	201728	294545	25.50%	3.350%
6	3.805	850	860	903	rBV	127073	439168	38.02%	4.995%
7	4.243	978	996	1027	rBV3	170793	457580	39.62%	5.204%
8	4.953	1199	1217	1253	rBV2	376794	1006892	87.18%	11.452%
9	5.529	1387	1396	1424	rBV	312438	689267	59.68%	7.839%
10	5.844	1484	1494	1514	rVB	7992	20815	1.80%	0.237%
11	5.985	1525	1538	1563	rBV	233110	503941	43.63%	5.732%
12	6.918	1818	1828	1853	rBV2	69142	156206	13.52%	1.777%
13	7.239	1918	1928	1967	rBV	395573	763352	66.09%	8.682%
14	7.561	2020	2028	2048	rBV2	37561	82082	7.11%	0.934%
15	8.024	2163	2172	2211	rBV	503125	1154966	100.00%	13.136%
16	8.783	2395	2408	2440	rBV	512225	917682	79.46%	10.437%
17	10.149	2823	2833	2858	rBV	207319	345770	29.94%	3.933%
18	11.181	3143	3154	3179	rBV	500892	843677	73.05%	9.596%
19	11.500	3243	3253	3260	rBV4	16070	31502	2.73%	0.358%
20	11.558	3261	3271	3297	rVB	451073	767441	66.45%	8.729%




Sum of corrected areas: 8792241

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037427.D
Acq On : 20 Sep 2024 13:00
Operator : SY/MD
Sample : P3994-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

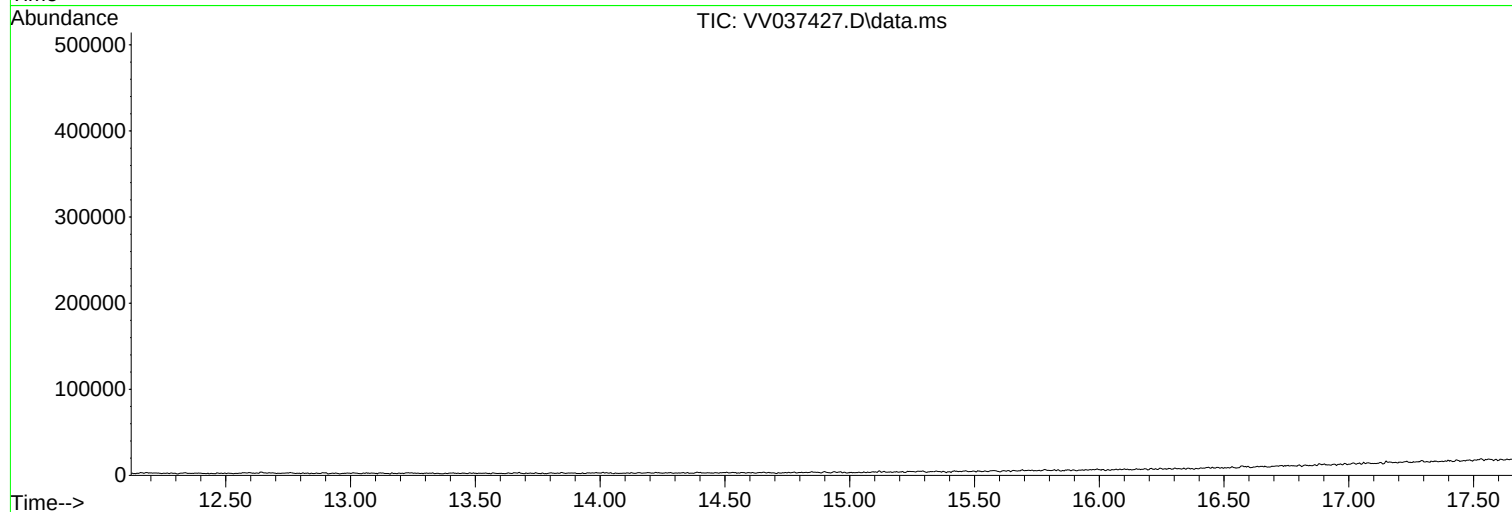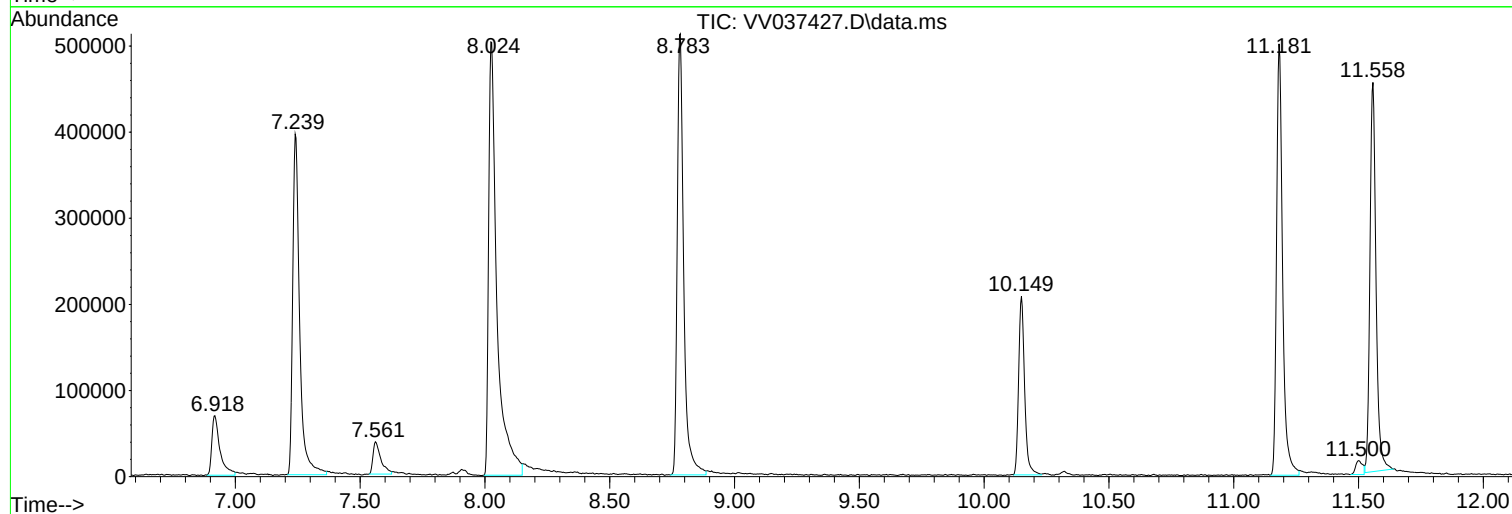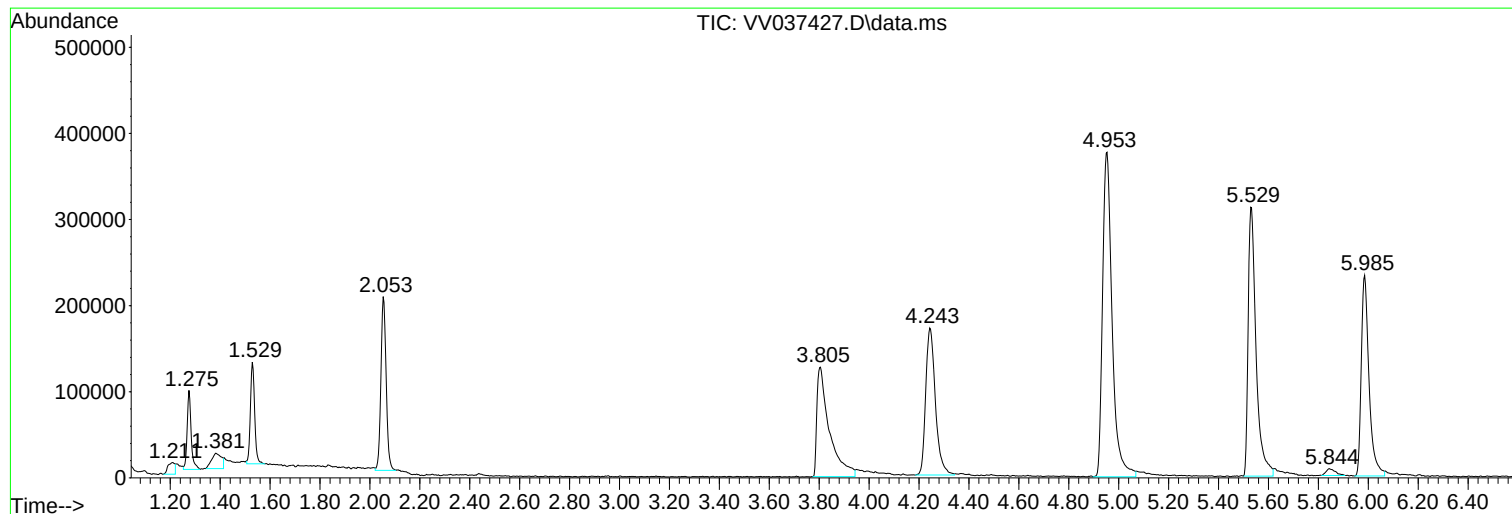

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037427.D
Acq On : 20 Sep 2024 13:00
Operator : SY/MD
Sample : P3994-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037427.D
Acq On : 20 Sep 2024 13:00
Operator : SY/MD
Sample : P3994-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc