

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
 Data File : VV037450.D
 Acq On : 20 Sep 2024 23:18
 Operator : SY/MD
 Sample : P4107-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B23

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV037450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	83	rVB	83469	83948	7.48%	0.846%
2	1.529	145	152	165	rVB	105110	123064	10.96%	1.240%
3	2.056	306	316	332	rVB3	204459	327132	29.15%	3.296%
4	3.805	848	860	897	rBV2	143706	508096	45.27%	5.119%
5	4.246	982	997	1031	rBV2	175465	530180	47.24%	5.341%
6	4.728	1131	1147	1172	rBV	93038	236306	21.05%	2.381%
7	4.950	1199	1216	1250	rBV2	354108	933140	83.14%	9.400%
8	5.532	1387	1397	1425	rBV	301916	670102	59.70%	6.751%
9	5.828	1477	1489	1520	rBV	433195	916876	81.69%	9.237%
10	5.985	1526	1538	1562	rBV	212627	454927	40.53%	4.583%
11	6.918	1815	1828	1846	rBV2	69565	147290	13.12%	1.484%
12	7.239	1914	1928	1951	rBV	363561	695782	61.99%	7.009%
13	7.561	2020	2028	2049	rBV2	35765	83334	7.42%	0.840%
14	7.902	2118	2134	2160	rBV2	189313	344830	30.72%	3.474%
15	8.024	2163	2172	2220	rBV	488617	1122374	100.00%	11.307%
16	8.779	2397	2407	2435	rBV	495142	871608	77.66%	8.781%
17	10.149	2819	2833	2853	rBV	202614	336641	29.99%	3.391%
18	11.181	3143	3154	3186	rBV	489976	810127	72.18%	8.161%
19	11.557	3252	3271	3299	rBV	416097	730785	65.11%	7.362%




Sum of corrected areas: 9926542

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037450.D
Acq On : 20 Sep 2024 23:18
Operator : SY/MD
Sample : P4107-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

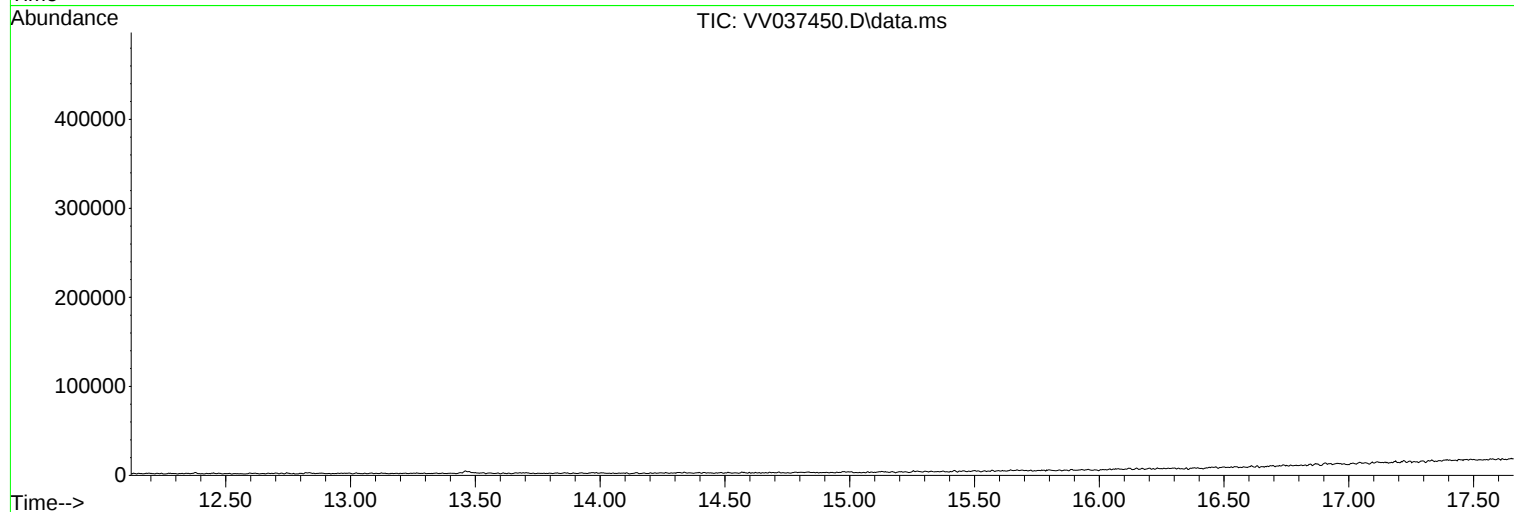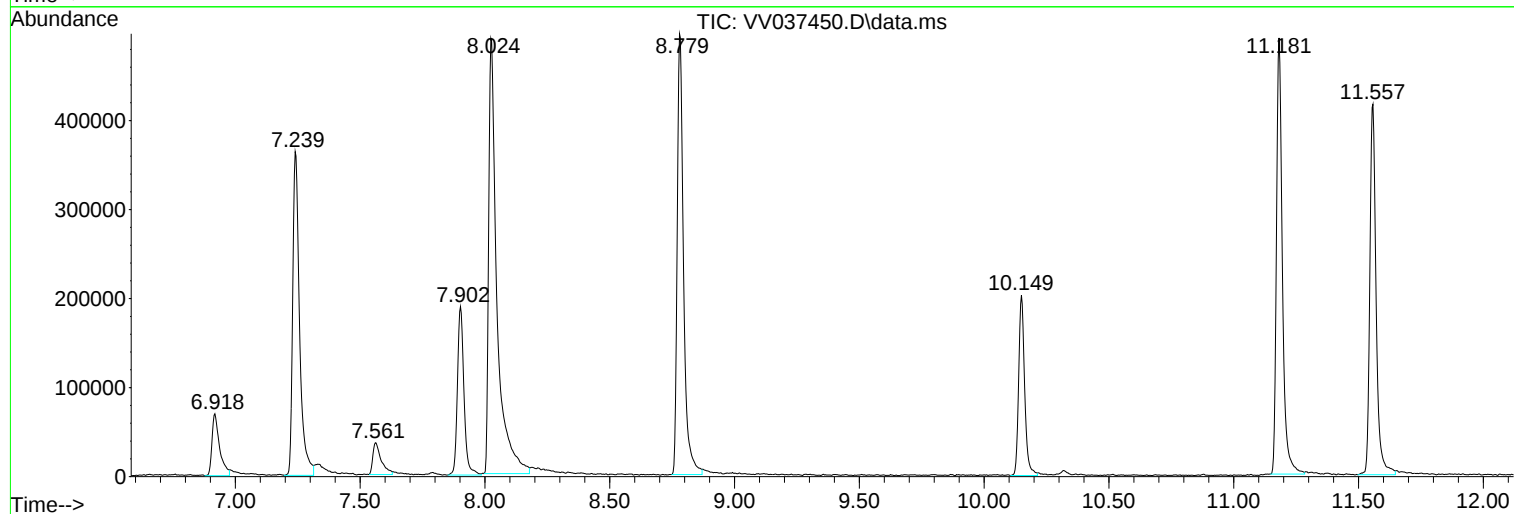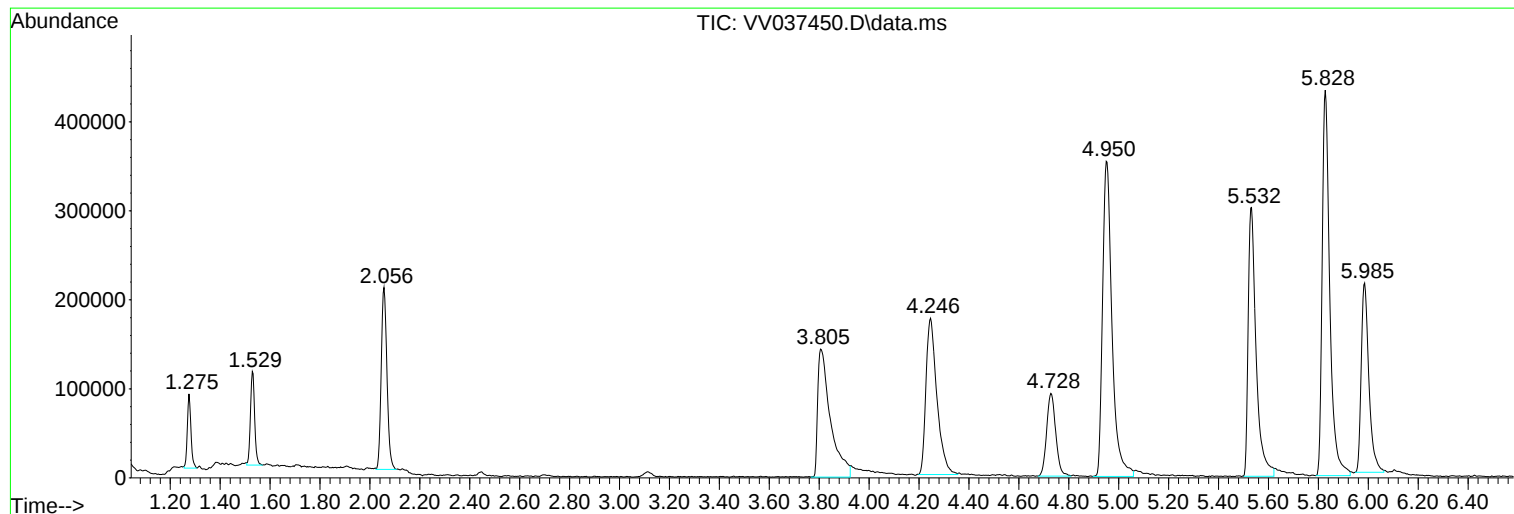

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037450.D
Acq On : 20 Sep 2024 23:18
Operator : SY/MD
Sample : P4107-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037450.D
Acq On : 20 Sep 2024 23:18
Operator : SY/MD
Sample : P4107-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc