

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
 Data File : VV037455.D
 Acq On : 21 Sep 2024 01:19
 Operator : SY/MD
 Sample : P4107-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B43

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV037455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.211	42	53	57	rBV3	8115	14299	1.27%	0.155%
2	1.275	67	73	90	rVB	80715	89437	7.96%	0.971%
3	1.529	145	152	166	rVB	108125	124986	11.12%	1.357%
4	2.056	306	316	333	rVB	182922	276045	24.57%	2.996%
5	3.805	849	860	909	rBV	132021	484778	43.14%	5.262%
6	4.243	980	996	1028	rBV2	159421	427303	38.03%	4.638%
7	4.950	1203	1216	1260	rBV2	348829	933973	83.12%	10.137%
8	5.529	1385	1396	1433	rBV	309363	694047	61.77%	7.533%
9	5.834	1478	1491	1523	rBV2	133236	300082	26.71%	3.257%
10	5.985	1523	1538	1564	rBV	212627	466971	41.56%	5.068%
11	6.918	1817	1828	1850	rBV2	65461	145357	12.94%	1.578%
12	7.239	1916	1928	1954	rBV	359255	690738	61.47%	7.497%
13	7.564	2018	2029	2047	rBV2	35213	79102	7.04%	0.859%
14	7.902	2121	2134	2155	rBV2	308550	550243	48.97%	5.972%
15	8.024	2163	2172	2213	rBV	494701	1123644	100.00%	12.196%
16	8.783	2397	2408	2443	rBV	509197	912020	81.17%	9.899%
17	10.149	2822	2833	2860	rBV	198498	333781	29.71%	3.623%
18	11.181	3144	3154	3175	rBV	517477	849649	75.62%	9.222%
19	11.557	3260	3271	3299	rBV	422834	716843	63.80%	7.781%




Sum of corrected areas: 9213298

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037455.D
Acq On : 21 Sep 2024 01:19
Operator : SY/MD
Sample : P4107-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

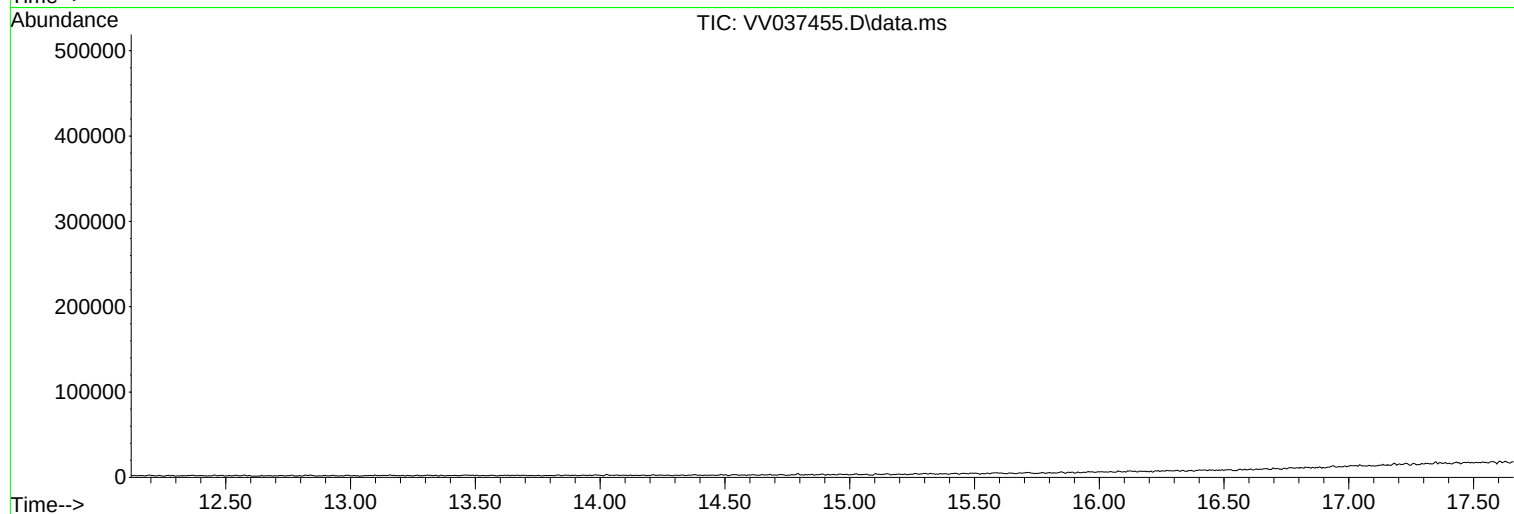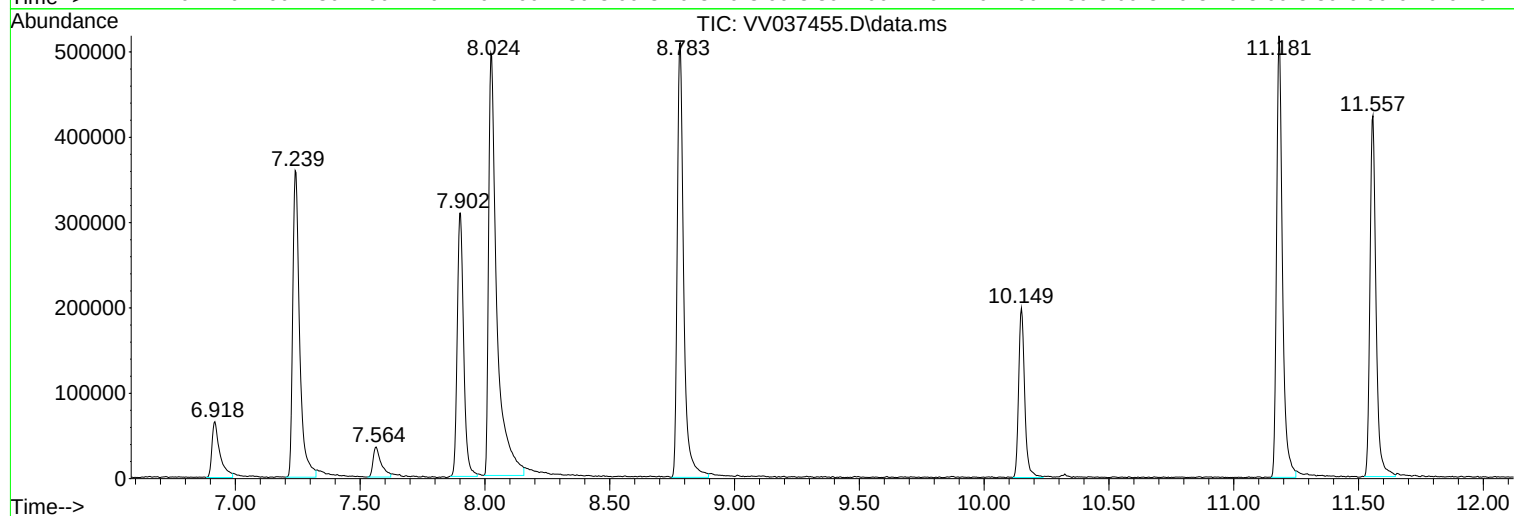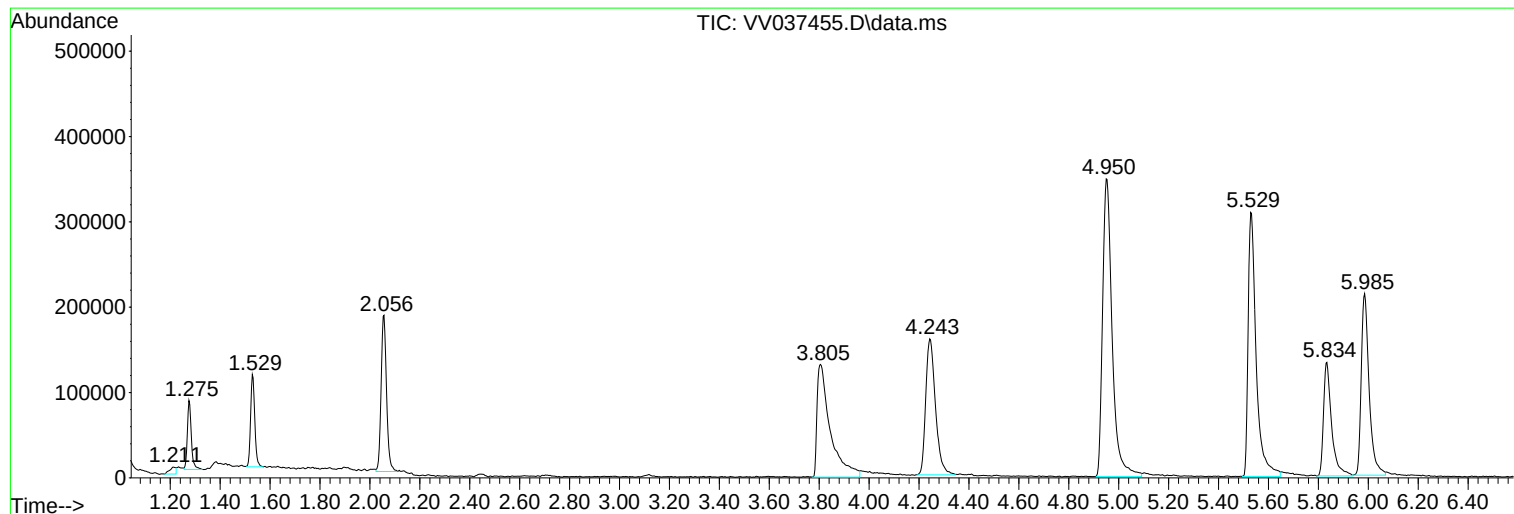

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037455.D
Acq On : 21 Sep 2024 01:19
Operator : SY/MD
Sample : P4107-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037455.D
Acq On : 21 Sep 2024 01:19
Operator : SY/MD
Sample : P4107-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc