


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037417.D
Acq On : 20 Sep 2024 08:21
Operator : SY/MD
Sample : BFB277
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB277

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Sep 21 01:15:22 2024

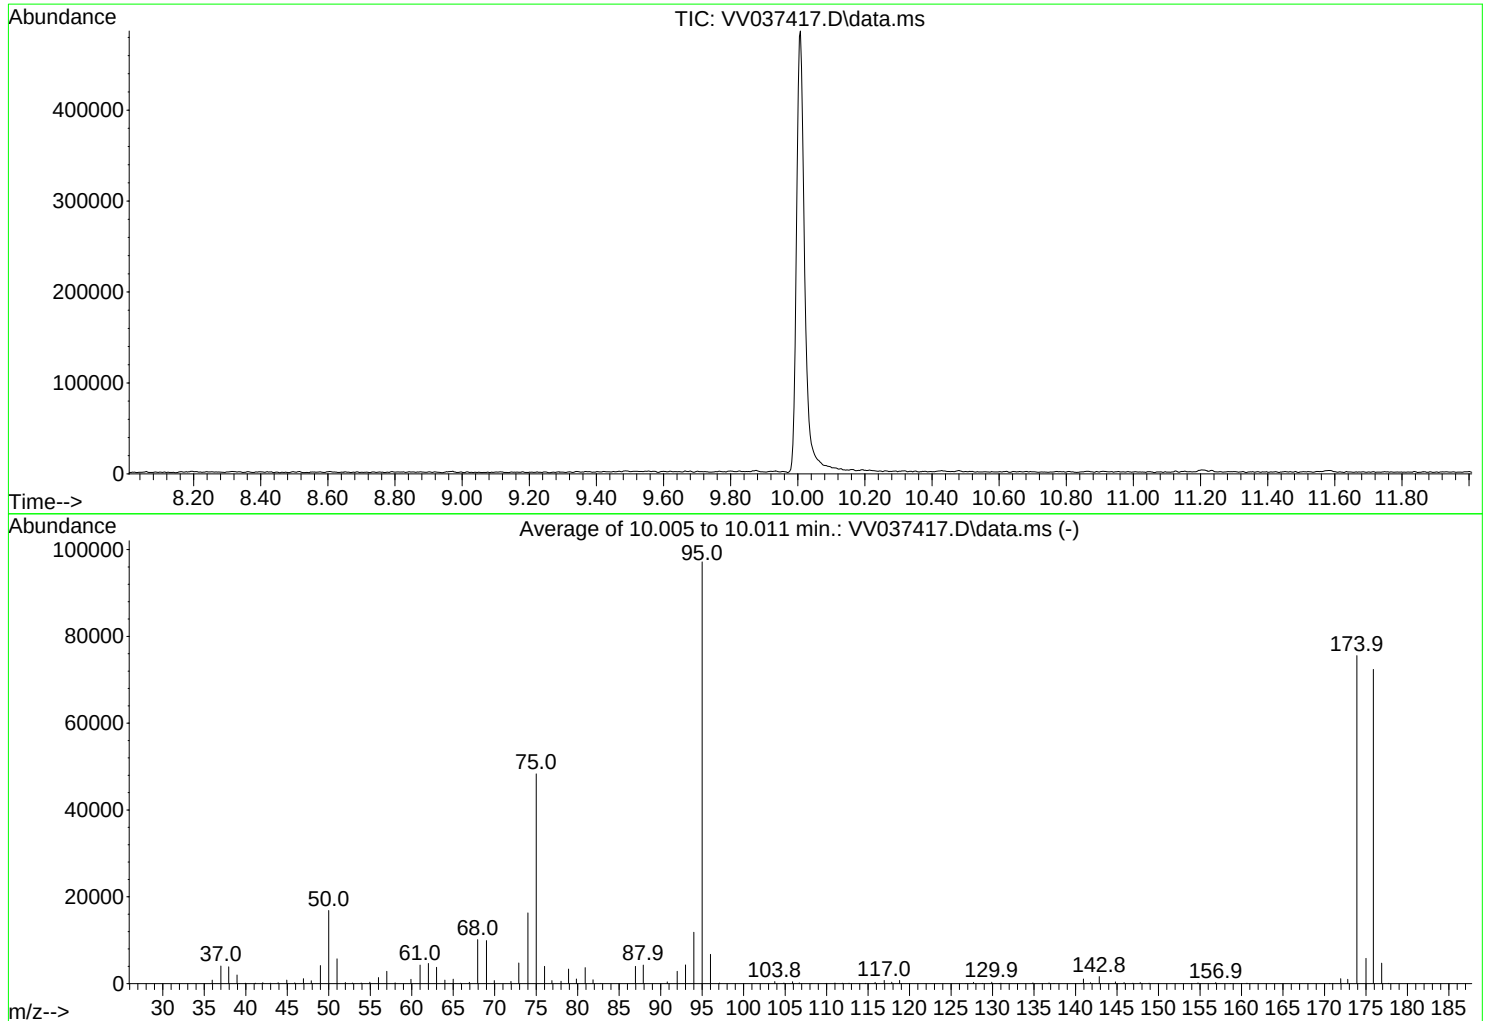

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	16836	PASS
75	95	30	80	49.7	48347	PASS
95	95	100	100	100.0	97181	PASS
96	95	5	9	6.9	6736	PASS
173	174	0.00	2	1.3	1006	PASS
174	95	50	120	77.8	75568	PASS
175	174	5	9	7.7	5826	PASS
176	174	95	105	95.8	72392	PASS
177	176	5	10	6.5	4723	PASS

m/z	Abundance
37.90	105.0
40.00	271.0
40.90	127.0
41.80	149.0
42.90	111.0
43.90	859.0
49.40	105.0
59.90	235.0
79.00	107.0
206.90	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277

m/z	Abundance
36.00	852.0
37.00	4249.0
38.00	4017.0
38.90	2063.0
40.10	333.0
40.90	134.0
42.00	240.0
43.00	247.0
43.90	1211.0
45.00	854.0
45.80	219.0
47.00	1045.0
47.90	744.0
49.00	4334.0
50.00	17256.0
51.00	5868.0
52.00	227.0
52.80	146.0
53.90	124.0
54.90	347.0
56.00	1429.0
57.00	2954.0
58.10	211.0
59.90	1181.0
61.00	4459.0
62.00	4878.0
63.00	4090.0
64.00	724.0
65.00	961.0
67.00	268.0
67.90	10598.0
69.00	10461.0
69.90	706.0
71.90	626.0
72.90	4777.0
74.00	16664.0
75.00	49336.0
76.00	4182.0
76.90	749.0
78.00	628.0
78.90	3700.0
79.80	1117.0
80.90	3759.0
81.90	878.0
87.00	4235.0
87.90	4620.0
90.80	459.0
92.00	2821.0
93.00	4240.0
94.00	12109.0
95.00	99432.0
96.00	6994.0
97.10	153.0
103.70	501.0
104.90	167.0
105.90	451.0
106.70	187.0
111.00	147.0
112.70	129.0
115.80	354.0
116.90	751.0
117.80	322.0
118.80	731.0
127.70	285.0
129.90	329.0
130.80	157.0
134.90	190.0
136.80	216.0
137.40	106.0
140.90	1025.0
141.80	193.0
142.80	1654.0
144.80	393.0
145.80	221.0
147.00	128.0
147.80	295.0
148.90	102.0
154.70	172.0
156.90	269.0
160.70	105.0
171.00	107.0
171.90	1077.0
172.80	1015.0
173.90	75896.0
175.00	6051.0
175.90	73496.0
176.90	4716.0
177.80	126.0
207.10	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277

m/z	Abundance
35.90	815.0
37.00	4179.0
38.00	4095.0
39.00	2081.0
39.90	381.0
41.10	142.0
42.10	250.0
43.00	219.0
43.90	1066.0
45.00	857.0
45.90	203.0
46.90	1155.0
47.90	647.0
49.00	4353.0
50.00	17312.0
51.00	5890.0
52.00	269.0
52.90	148.0
53.90	149.0
54.90	335.0
56.00	1446.0
57.00	2953.0
58.00	193.0
59.90	1286.0
61.00	4380.0
62.00	4757.0
63.00	3895.0
64.00	843.0
65.00	1079.0
65.90	123.0
66.90	293.0
68.00	10483.0
69.00	10217.0
70.00	691.0
71.90	553.0
72.90	4875.0
74.00	16912.0
75.00	49808.0
76.00	4084.0
76.90	700.0
78.00	588.0
78.90	3570.0
79.90	1103.0
80.90	3768.0
81.80	876.0
82.80	104.0
86.90	4007.0
87.90	4392.0
90.80	414.0
92.00	2887.0
93.00	4427.0
94.00	12194.0
95.00	100504.0
96.00	6958.0
97.10	139.0
103.80	491.0
104.90	145.0
105.90	458.0
106.70	206.0
109.90	113.0
111.00	164.0
111.90	156.0
112.70	139.0
114.70	138.0
115.90	310.0
117.00	790.0
117.80	323.0
118.80	760.0
126.80	107.0
127.70	298.0
128.80	118.0
129.90	345.0
131.00	158.0
134.80	193.0
136.80	209.0
140.90	1107.0
141.80	247.0
142.90	1695.0
144.80	434.0
145.90	250.0
146.90	134.0
147.80	271.0
148.90	128.0
154.80	172.0
156.90	258.0
158.70	149.0
160.60	120.0
171.90	1169.0
172.80	1055.0
173.90	78240.0
175.00	6049.0
175.90	74968.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277

176.90

4885.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277

m/z	Abundance
35.90	757.0
37.00	3793.0
38.00	3850.0
39.00	1872.0
39.90	399.0
41.20	166.0
42.10	207.0
43.10	157.0
44.00	977.0
44.90	769.0
46.00	177.0
46.90	1184.0
47.90	642.0
49.00	3791.0
50.00	15940.0
51.00	5357.0
52.00	319.0
52.90	141.0
53.90	147.0
55.00	327.0
56.00	1284.0
57.00	2629.0
57.90	151.0
59.90	1237.0
61.00	4007.0
62.00	4256.0
63.00	3325.0
64.00	860.0
65.00	1064.0
65.90	178.0
66.90	357.0
68.00	9330.0
69.00	9098.0
70.00	668.0
72.00	427.0
72.90	4667.0
74.00	15351.0
75.00	45896.0
76.00	3738.0
76.90	671.0
78.00	435.0
78.90	3072.0
79.90	1034.0
80.90	3551.0
81.80	885.0
82.80	116.0
86.90	3766.0
87.90	3813.0
90.80	352.0
92.00	2764.0
93.00	4268.0
94.00	11187.0
95.00	91608.0
96.00	6256.0
97.10	103.0
103.80	446.0
104.80	117.0
105.90	426.0
106.70	171.0
108.20	113.0
110.00	102.0
111.00	124.0
111.90	198.0
112.70	109.0
114.70	132.0
115.80	269.0
116.90	667.0
117.90	369.0
118.80	690.0
127.70	310.0
128.80	135.0
129.90	322.0
131.00	140.0
134.80	178.0
136.80	137.0
141.00	1093.0
141.80	248.0
142.90	1537.0
144.80	379.0
145.90	263.0
146.80	103.0
147.80	242.0
148.70	125.0
154.80	221.0
156.90	233.0
159.00	162.0
160.60	133.0
170.60	110.0
172.00	1192.0
172.80	948.0
173.90	72568.0
175.00	5379.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277

175.90	68712.0
176.90	4568.0
177.70	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277