

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028009.D
 Acq On : 21 Sep 2022 12:08
 Operator : SY/MD
 Sample : VV0921WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Quant Time: Sep 22 03:22:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 03:03:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	370548	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	353079	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	161380	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	140004	43.039	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	86.080%	
7) Chloroethane-d5	1.561	69	122746	47.235	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	94.460%	
11) 1,1-Dichloroethene-d2	2.098	63	202391	35.120	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	70.240%	
21) 2-Butanone-d5	3.873	46	216387	111.865	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	111.860%	
24) Chloroform-d	4.336	84	263529	48.252	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.500%	
26) 1,2-Dichloroethane-d4	5.021	65	178733	50.498	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.000%	
32) Benzene-d6	5.040	84	523986	51.489	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.980%	
36) 1,2-Dichloropropane-d6	6.059	67	169821	54.040	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	108.080%	
41) Toluene-d8	7.310	98	446494	47.911	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.820%	
43) trans-1,3-Dichloroprop...	7.616	79	76499	48.680	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	97.360%	
47) 2-Hexanone-d5	8.085	63	160001	103.932	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	103.930%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	230497	49.833	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	99.660%	
66) 1,2-Dichlorobenzene-d4	11.619	152	171721	54.815	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	109.620%	
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.101	101	2071	0.770	ug/L	# 27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028009.D
Acq On : 21 Sep 2022 12:08
Operator : SY/MD
Sample : VV0921WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266


Quant Time: Sep 22 03:22:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 22 03:03:58 2022
Response via : Initial Calibration

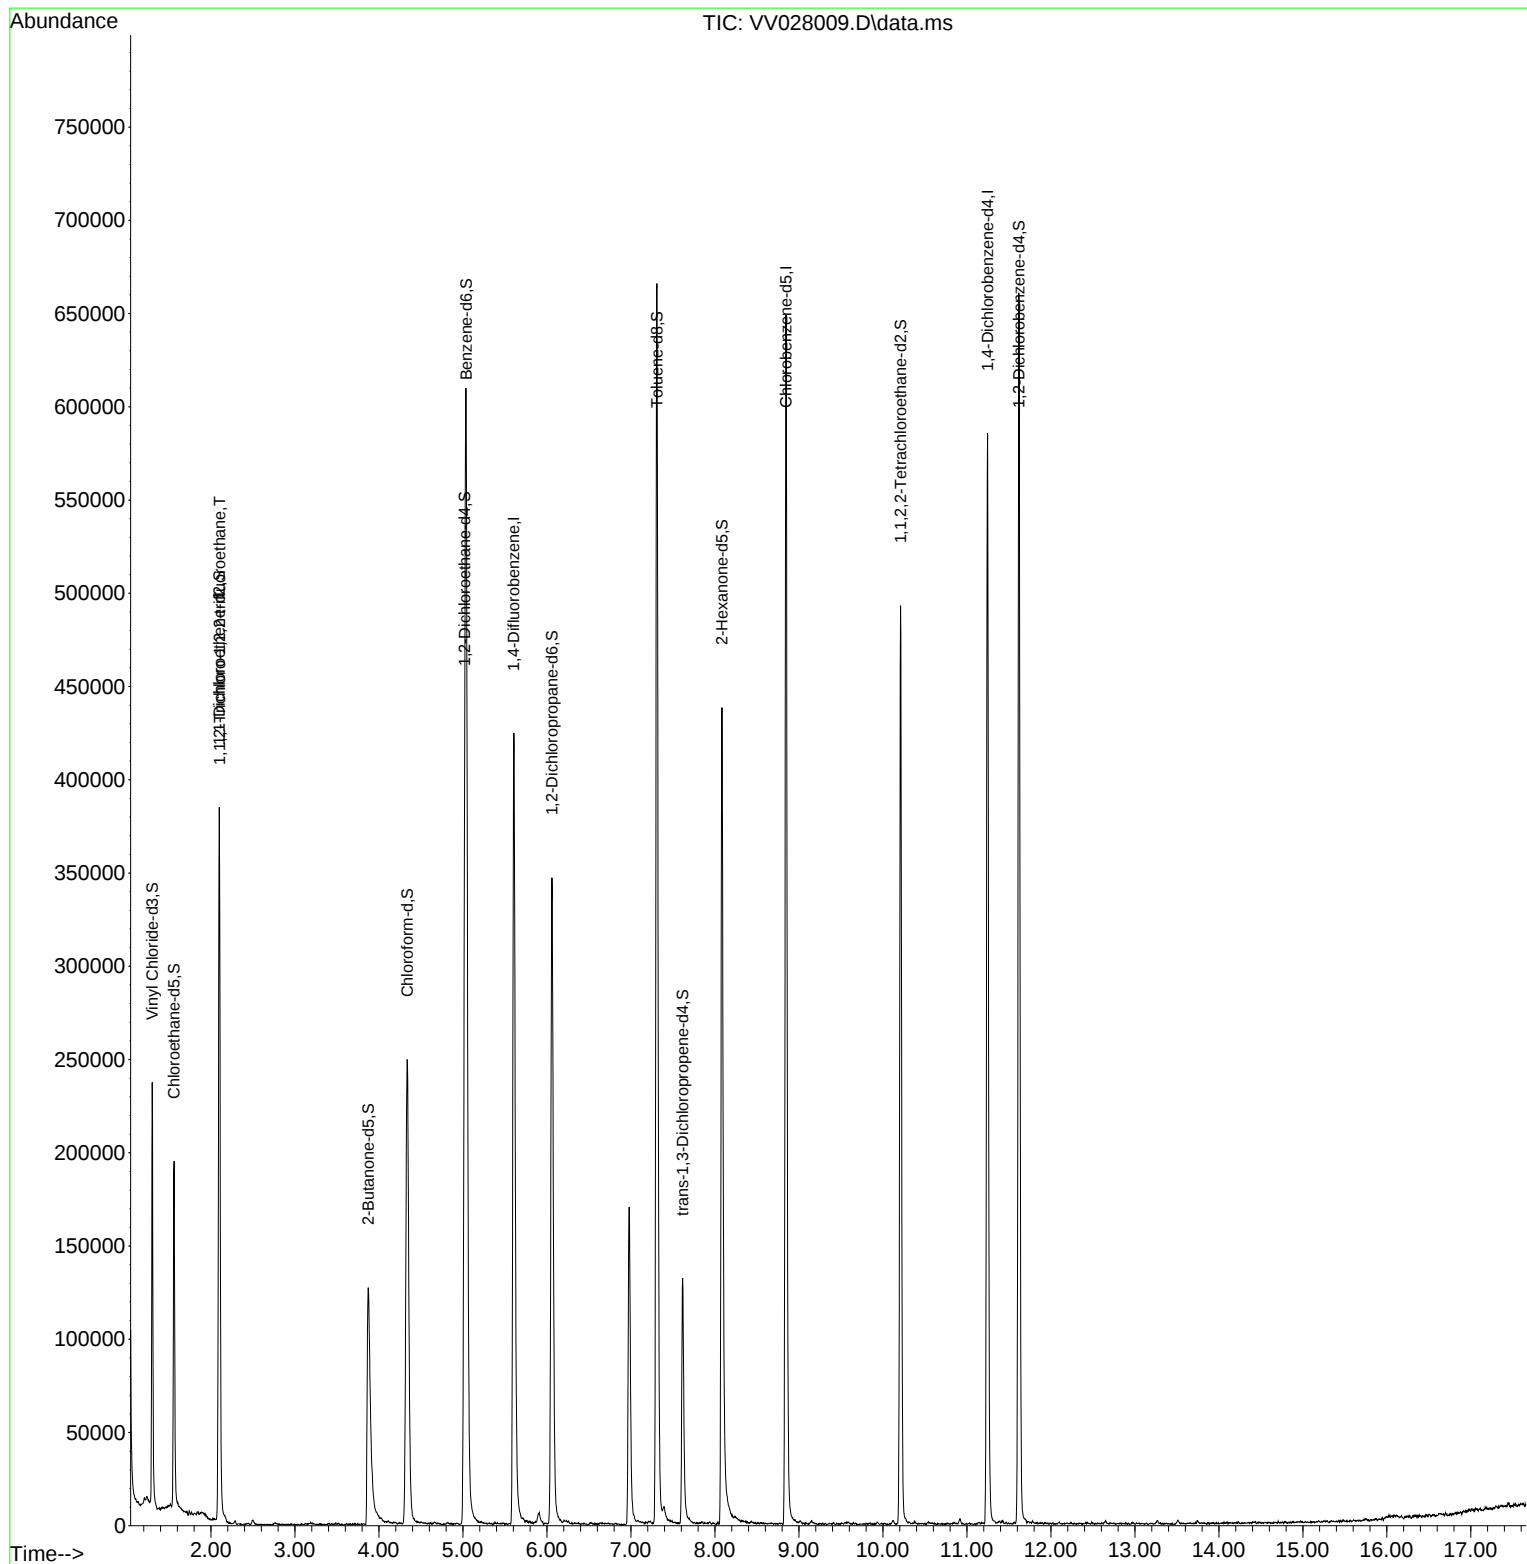

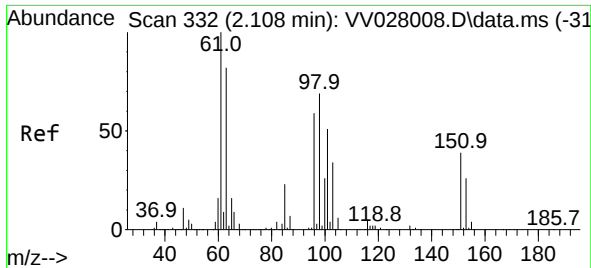

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.770 ug/L
 RT: 2.101 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV028009.D
 Acq: 21 Sep 2022 12:08

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

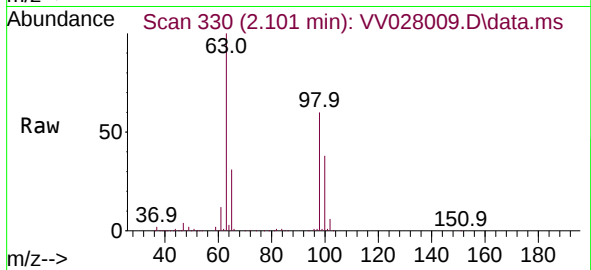

Tgt Ion:101 Resp: 2071
 Ion Ratio Lower Upper
 101 100
 85 3.1 35.6 53.4#
 151 10.2 62.2 93.4#

