

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW092122\
 Data File : VW028011.D
 Acq On : 21 Sep 2022 13:02
 Operator : SY/MD
 Sample : N4674-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC6

Quant Time: Sep 22 03:22:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 03:03:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	347356	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	336336	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	148810	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	120159	39.404	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.800%
7) Chloroethane-d5	1.558	69	105306	43.229	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.460%
11) 1,1-Dichloroethene-d2	2.101	63	172257	31.887	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.780%
21) 2-Butanone-d5	3.873	46	206431	113.843	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	113.840%
24) Chloroform-d	4.339	84	245310	47.915	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.820%
26) 1,2-Dichloroethane-d4	5.024	65	162960	49.116	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.240%
32) Benzene-d6	5.043	84	474692	48.967	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.940%
36) 1,2-Dichloropropane-d6	6.063	67	156111	52.150	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.300%
41) Toluene-d8	7.310	98	399815	45.037	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.080%
43) trans-1,3-Dichloroprop...	7.619	79	63852	42.655	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.300%
47) 2-Hexanone-d5	8.085	63	144901	98.809	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.810%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	221686	50.314	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.620%
66) 1,2-Dichlorobenzene-d4	11.622	152	152387	52.752	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.500%
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.246	75	15834	5.668	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028011.D
Acq On : 21 Sep 2022 13:02
Operator : SY/MD
Sample : N4674-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC6


Quant Time: Sep 22 03:22:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 22 03:03:58 2022
Response via : Initial Calibration

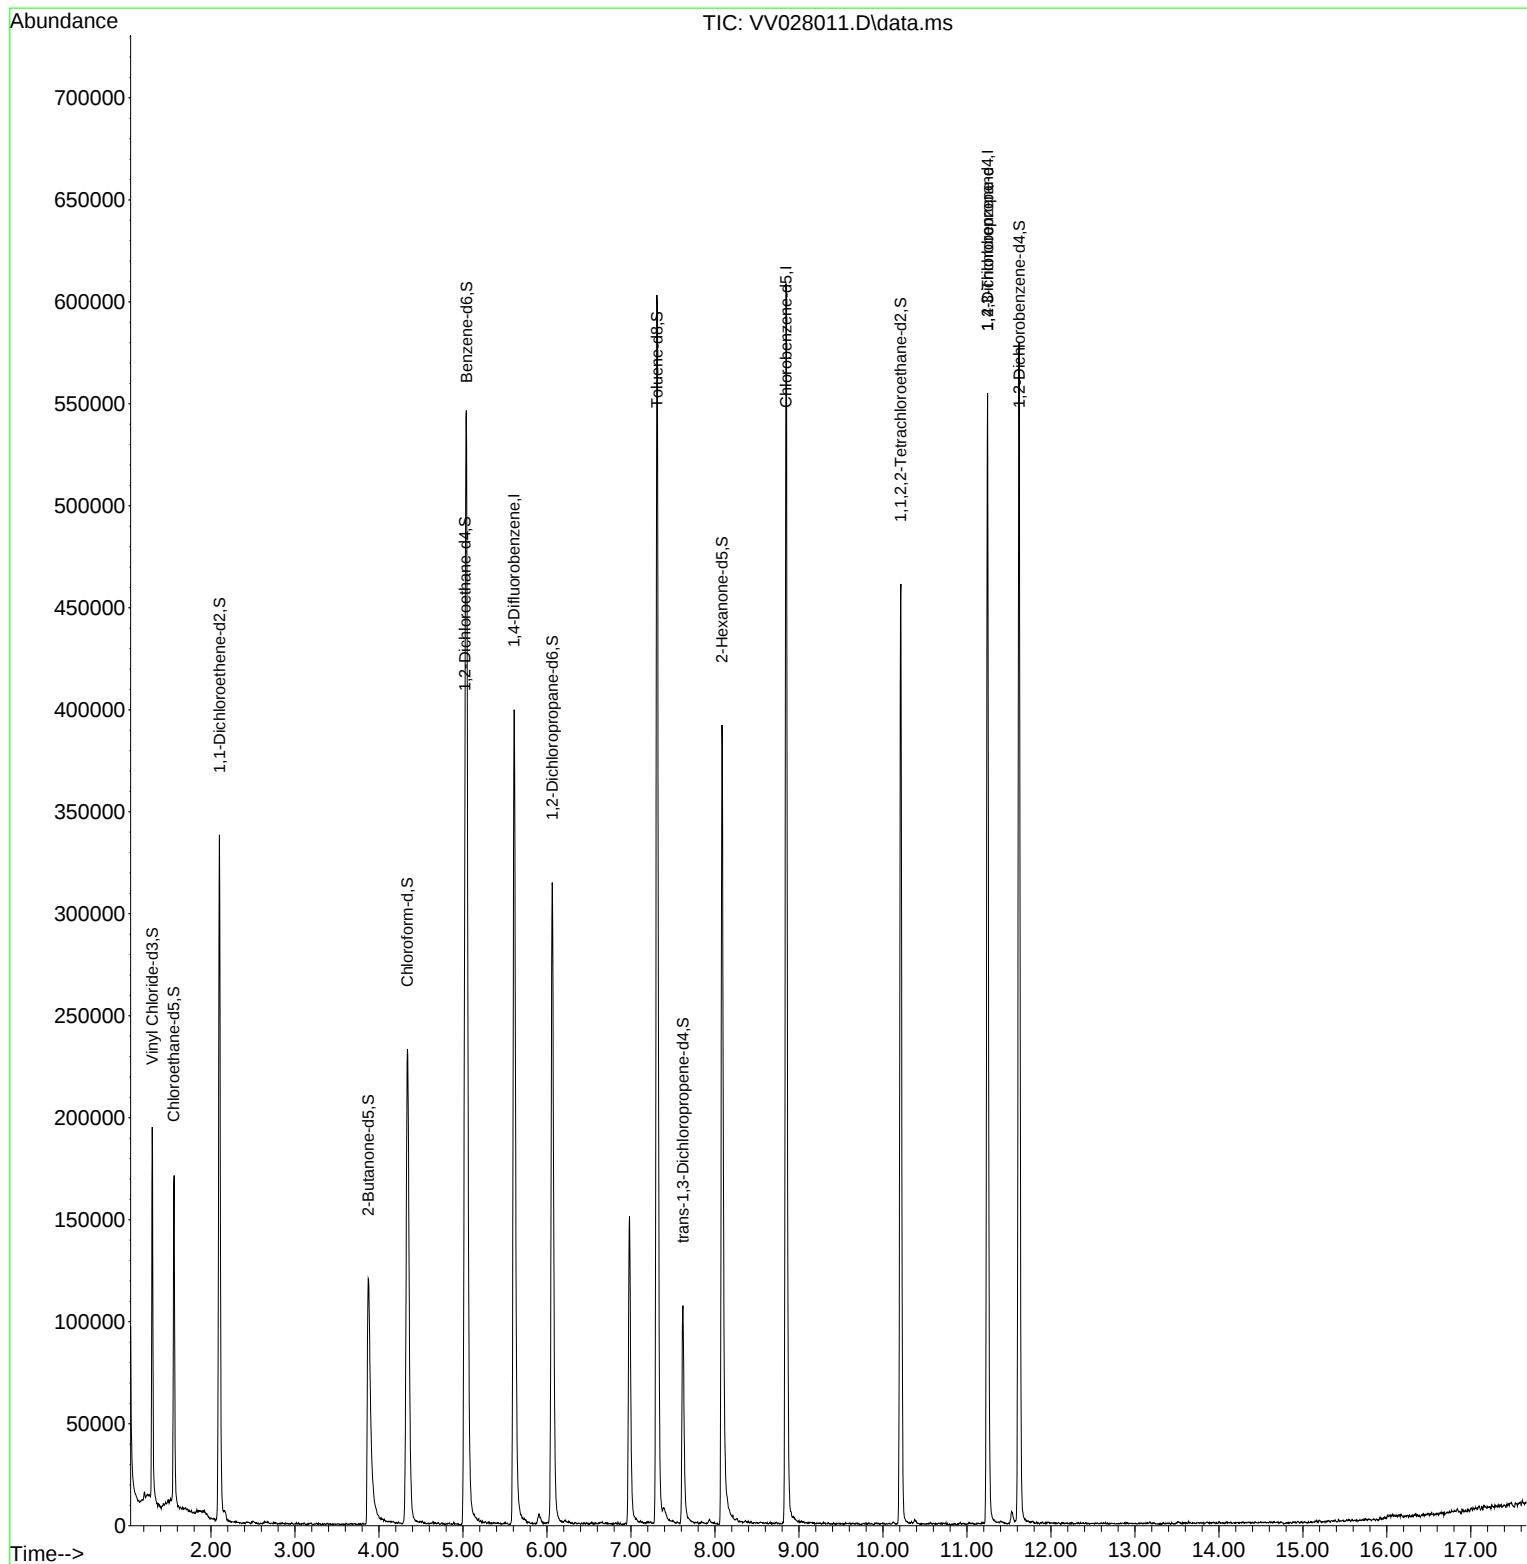

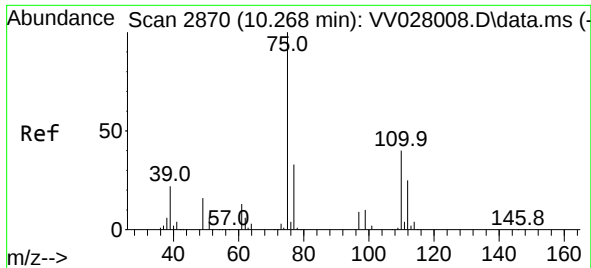

#61
 1,2,3-Trichloropropane
 Concen: 5.668 ug/L
 RT: 11.246 min Scan# 31
 Delta R.T. 0.978 min
 Lab File: VV028011.D
 Acq: 21 Sep 2022 13:02

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC6

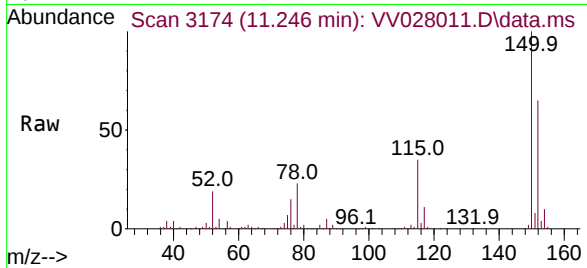

Tgt Ion: 75 Resp: 15834
 Ion Ratio Lower Upper
 75 100
 77 33.1 25.9 38.9
 110 2.1 31.1 46.7#

