

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028015.D
 Acq On : 21 Sep 2022 14:41
 Operator : SY/MD
 Sample : PB147776TB 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VLEB776

Quant Time: Sep 22 03:23:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 03:03:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	349563	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	344470	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	151537	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	115888	37.764	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.520%
7) Chloroethane-d5	1.558	69	104434	42.601	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.200%
11) 1,1-Dichloroethene-d2	2.098	63	164697	30.295	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.580%
21) 2-Butanone-d5	3.870	46	188783	103.453	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.450%
24) Chloroform-d	4.339	84	241861	46.943	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.880%
26) 1,2-Dichloroethane-d4	5.024	65	150267	45.004	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.000%
32) Benzene-d6	5.043	84	438615	44.177	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.360%
36) 1,2-Dichloropropane-d6	6.063	67	155808	50.820	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.640%
41) Toluene-d8	7.310	98	398466	43.826	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.660%
43) trans-1,3-Dichloroprop...	7.616	79	66899	43.635	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.280%
47) 2-Hexanone-d5	8.085	63	155006	103.203	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.200%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	218641	48.451	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.900%
66) 1,2-Dichlorobenzene-d4	11.622	152	153754	52.268	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.540%
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.098	101	1851	0.730	ug/L	# 19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028015.D
Acq On : 21 Sep 2022 14:41
Operator : SY/MD
Sample : PB147776TB 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VLEB776

Quant Time: Sep 22 03:23:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 22 03:03:58 2022
Response via : Initial Calibration

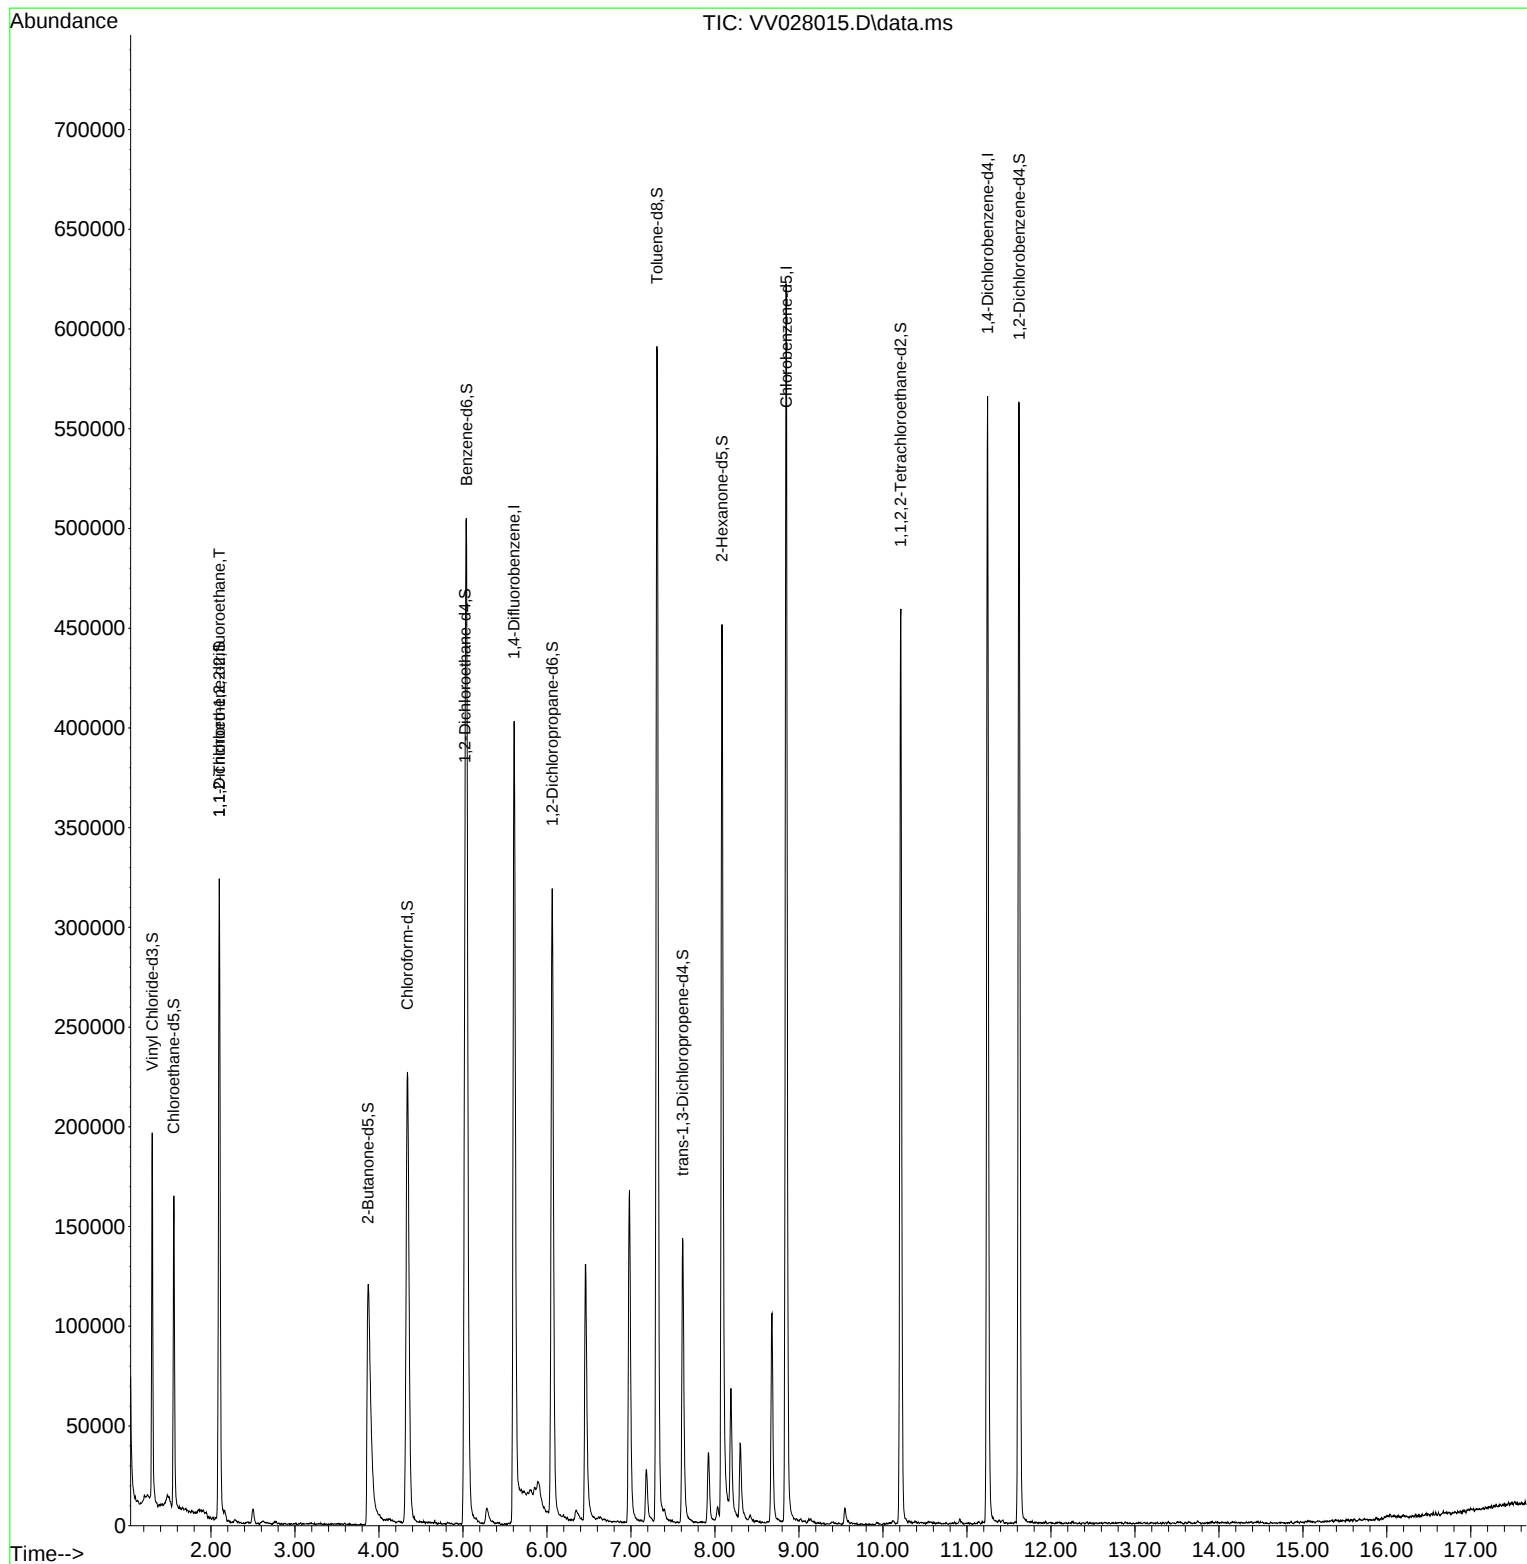

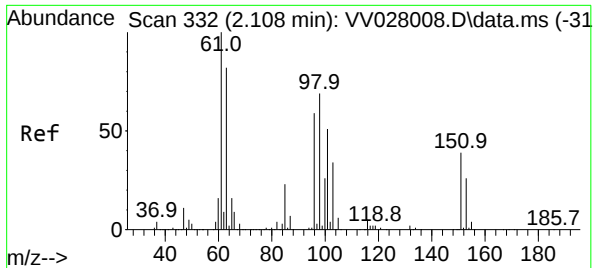

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.730 ug/L
 RT: 2.098 min Scan# 31
 Delta R.T. -0.009 min
 Lab File: VV028015.D
 Acq: 21 Sep 2022 14:41

Instrument :
 MSVOA_V
 ClientSampleId :
 VLEB776

Tgt Ion:	101	Resp:	1851
Ion	Ratio	Lower	Upper
101	100		
85	2.2	35.6	53.4#
151	0.0	62.2	93.4#

