

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW092122\
 Data File : VW028047.D
 Acq On : 22 Sep 2022 04:46
 Operator : SY/MD
 Sample : N4659-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC9

Quant Time: Sep 22 06:26:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 05:25:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	338070	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	326922	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	143125	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	147977	49.860	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 99.720%			
7) Chloroethane-d5	1.561	69	122632	51.725	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 103.440%			
11) 1,1-Dichloroethene-d2	2.098	63	206764	39.325	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 78.660%			
21) 2-Butanone-d5	3.883	46	206684	117.113	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 117.110%			
24) Chloroform-d	4.339	84	252163	50.606	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 101.220%			
26) 1,2-Dichloroethane-d4	5.024	65	170409	52.772	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.540%			
32) Benzene-d6	5.043	84	508578	53.973	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 107.940%			
36) 1,2-Dichloropropane-d6	6.063	67	169183	58.144	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 116.280%			
41) Toluene-d8	7.310	98	441479	51.163	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 102.320%			
43) trans-1,3-Dichloroprop...	7.619	79	69751	47.937	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 95.880%			
47) 2-Hexanone-d5	8.085	63	156075	109.493	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 109.490%			
56) 1,1,2,2-Tetrachloroeth...	10.214	84	232740	54.344	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 108.680%			
66) 1,2-Dichlorobenzene-d4	11.622	152	164573	59.234	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 118.460%			
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.101	101	2120	0.864	ug/L	# 20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028047.D
Acq On : 22 Sep 2022 04:46
Operator : SY/MD
Sample : N4659-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC9

Quant Time: Sep 22 06:26:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 22 05:25:17 2022
Response via : Initial Calibration

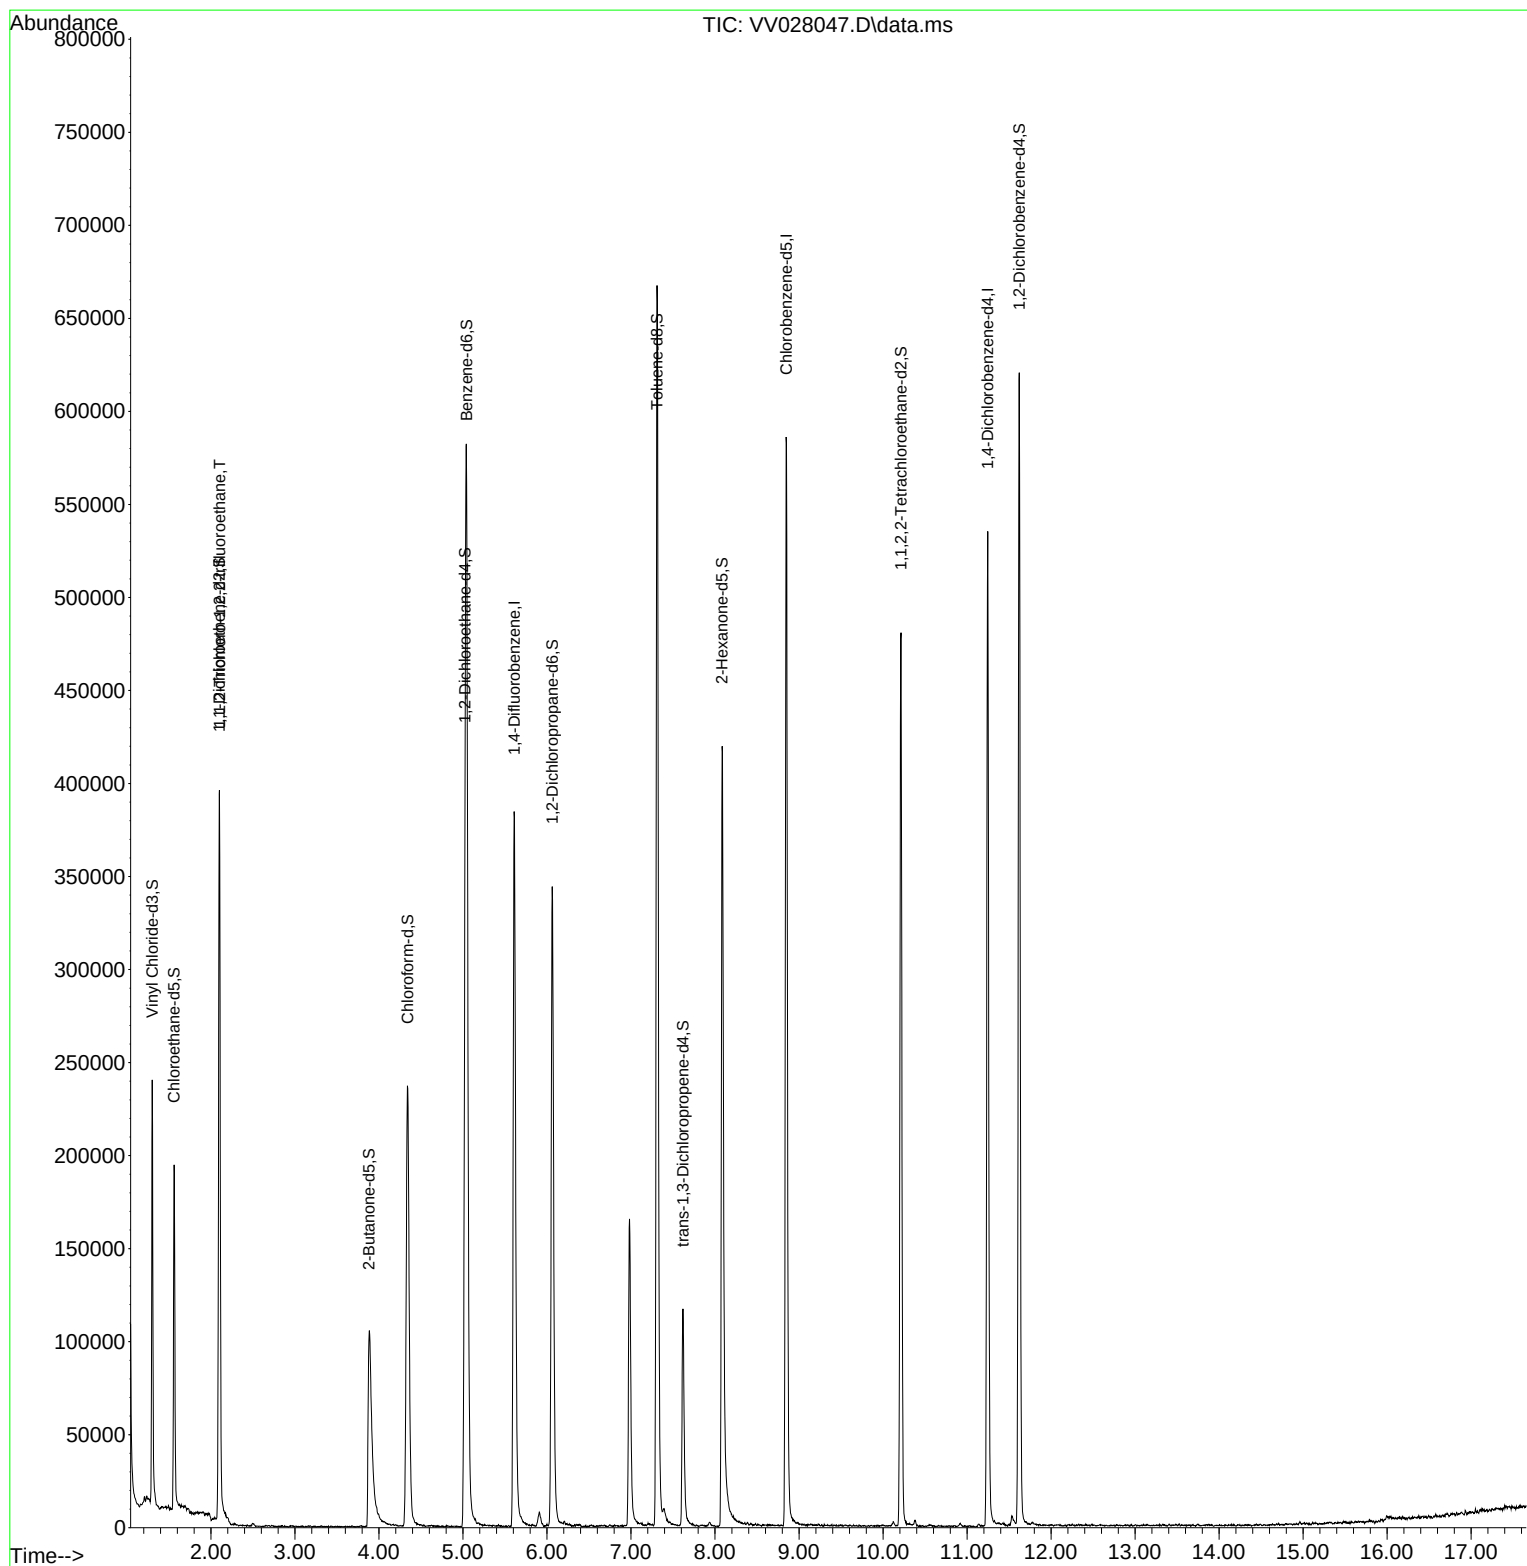

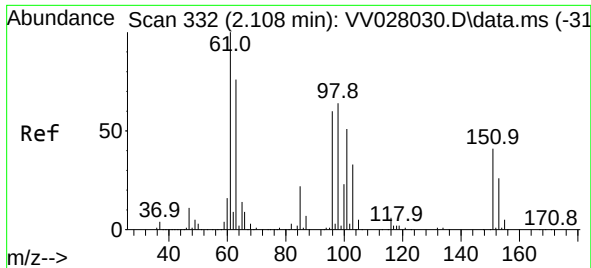

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.864 ug/L
 RT: 2.101 min Scan# 31
 Delta R.T. -0.007 min
 Lab File: VV028047.D
 Acq: 22 Sep 2022 04:46

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC9

Tgt Ion:101 Resp: 2120
 Ion Ratio Lower Upper
 101 100
 85 3.1 35.6 53.4#
 151 0.0 62.2 93.4#

