

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV092122\  
 Data File : VV028052.D  
 Acq On : 22 Sep 2022 09:21  
 Operator : SY/MD  
 Sample : VV0921WBL03  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 48 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 VBLK268


Quant Time: Sep 22 12:55:40 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM092022WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Sep 22 05:25:17 2022  
 Response via : Initial Calibration


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV092122\  
Data File : VV028052.D  
Acq On : 22 Sep 2022 09:21  
Operator : SY/MD  
Sample : VV0921WBL03  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 48 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK268

Quant Time: Sep 22 12:55:40 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM092022WMA.M  
Quant Title : VOC Analysis  
QLast Update : Thu Sep 22 05:25:17 2022  
Response via : Initial Calibration




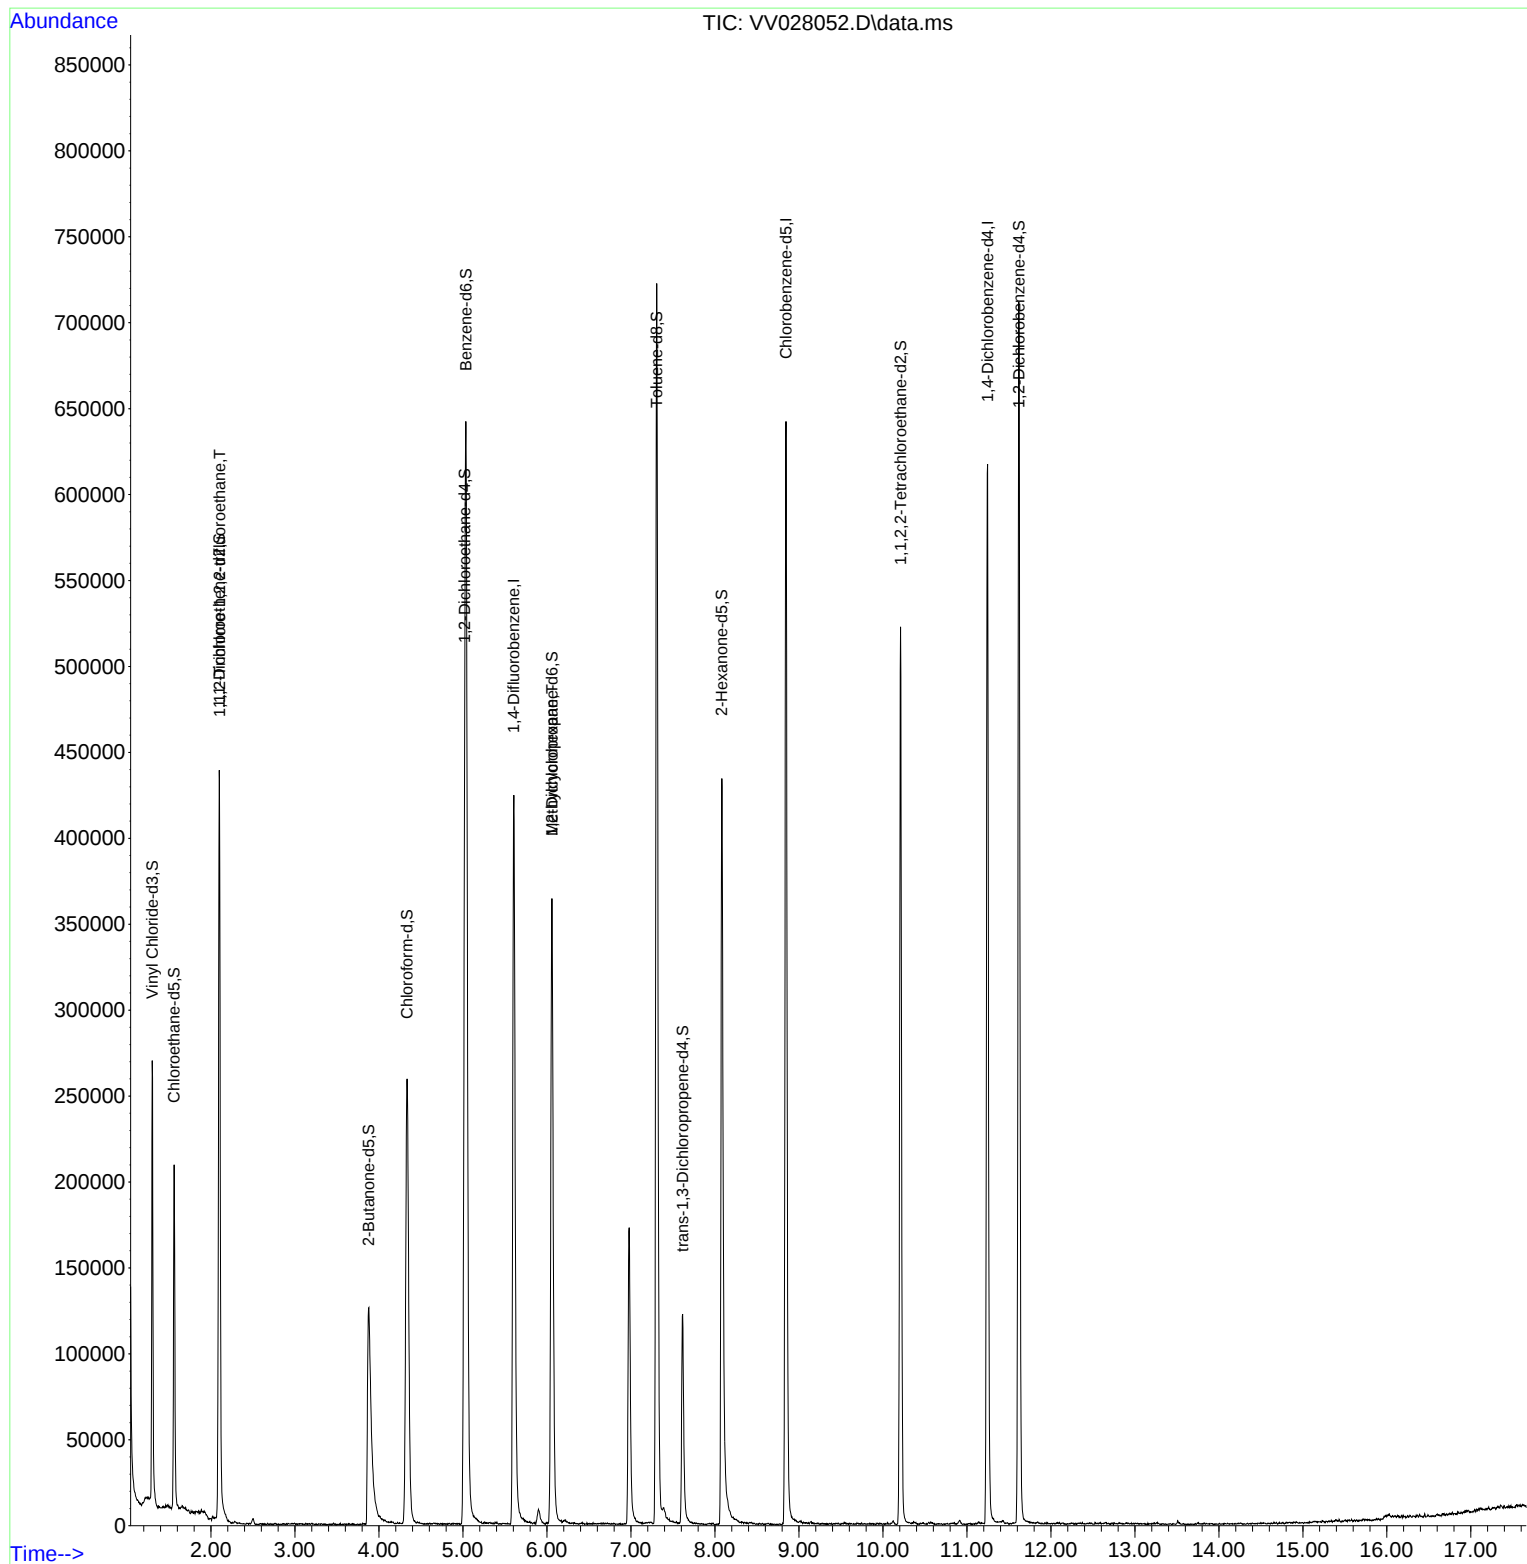


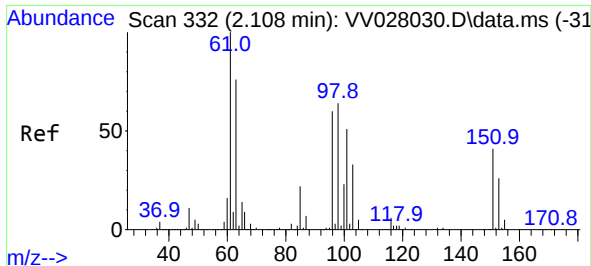

#10  
1,1,2-Trichloro-1,2,2-trifluoroethane  
Concen: 0.882 ug/L  
RT: 2.101 min Scan# 31  
Delta R.T. -0.007 min  
Lab File: VV028052.D  
Acq: 22 Sep 2022 09:21

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK268

Tgt Ion:101 Resp: 2380  
Ion Ratio Lower Upper  
101 100  
85 0.0 35.6 53.4#  
151 0.0 62.2 93.4#

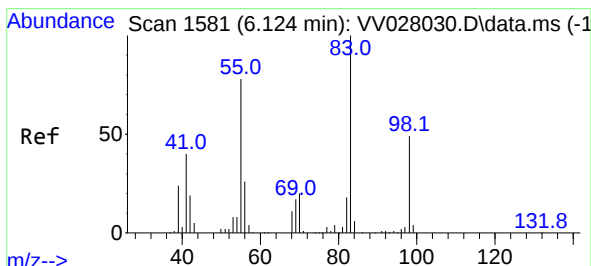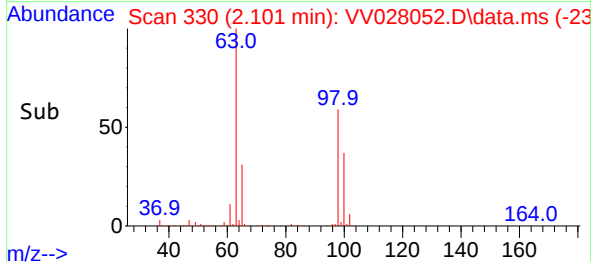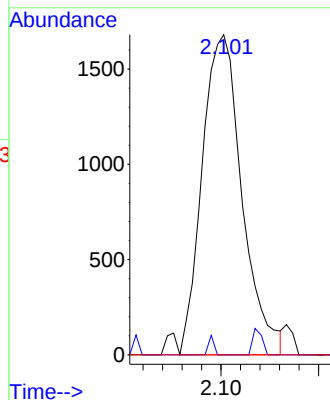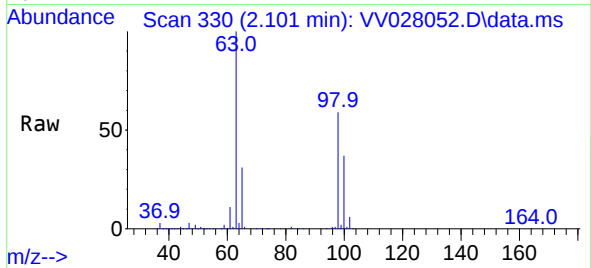

#35  
Methylcyclohexane  
Concen: 10.068 ug/L  
RT: 6.059 min Scan# 1561  
Delta R.T. -0.064 min  
Lab File: VV028052.D  
Acq: 22 Sep 2022 09:21

Tgt Ion: 83 Resp: 43741  
Ion Ratio Lower Upper  
83 100  
55 0.2 63.0 94.4#  
98 1.7 39.5 59.3#

