




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028010.D
 Acq On : 21 Sep 2022 12:37
 Operator : SY/MD
 Sample : N4674-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC5

Manual IntegrationsAPPROVED

Quant Time: Sep 22 03:22:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 03:03:58 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
 Supervised By :Mahesh Dadoda 09/22/2022

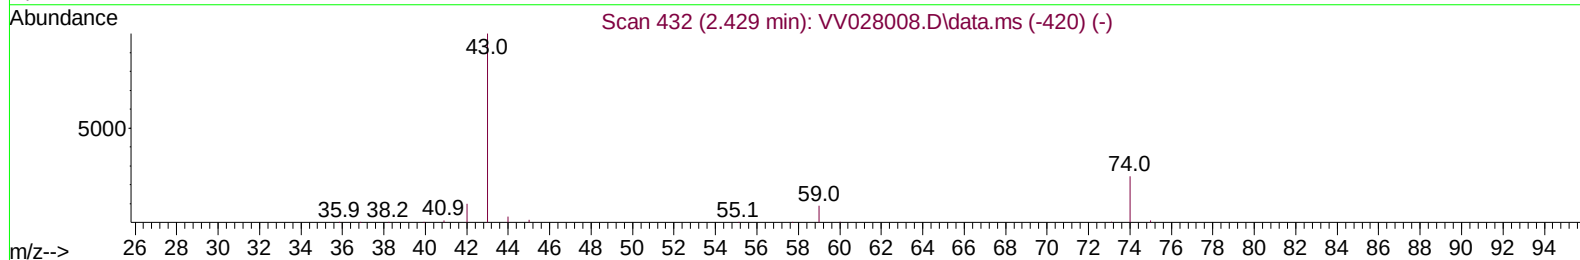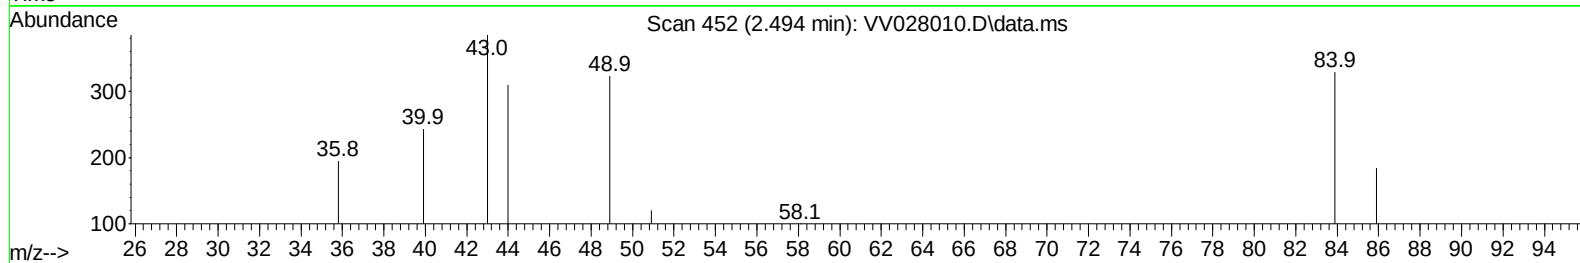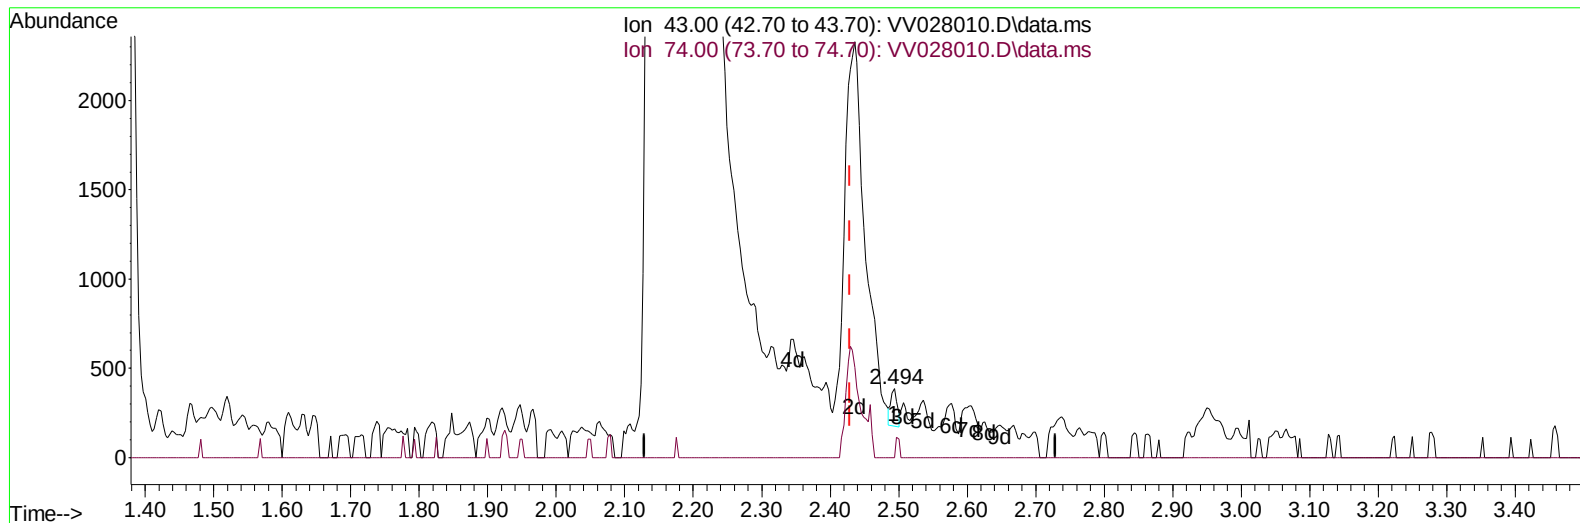

TIC: VV028010.D\data.ms

(15) Methyl Acetate (T)

2.494min (+ 0.064) 0.05 ug/L

response 138

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	26.10	30.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028010.D
 Acq On : 21 Sep 2022 12:37
 Operator : SY/MD
 Sample : N4674-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC5

Manual IntegrationsAPPROVED

Quant Time: Sep 22 03:22:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 03:03:58 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
 Supervised By :Mahesh Dadoda 09/22/2022

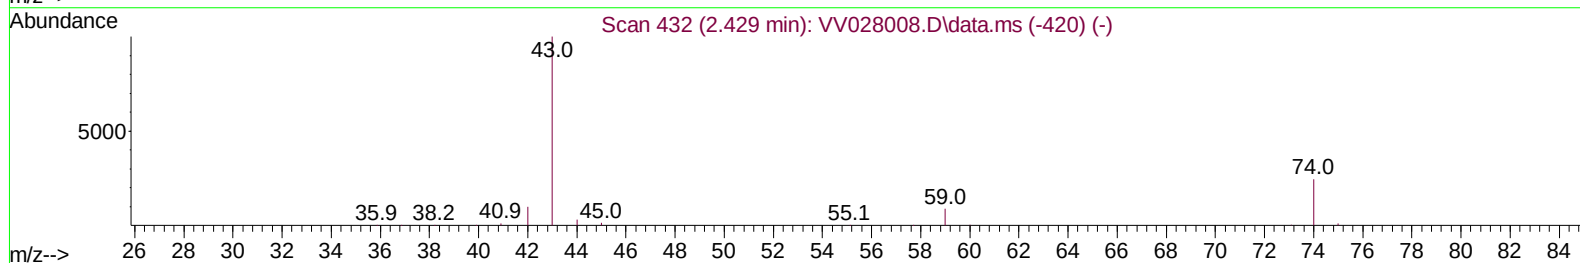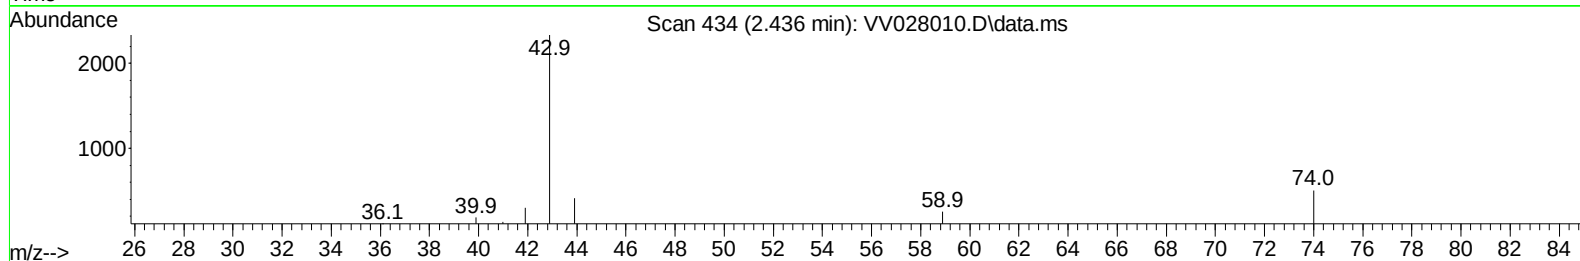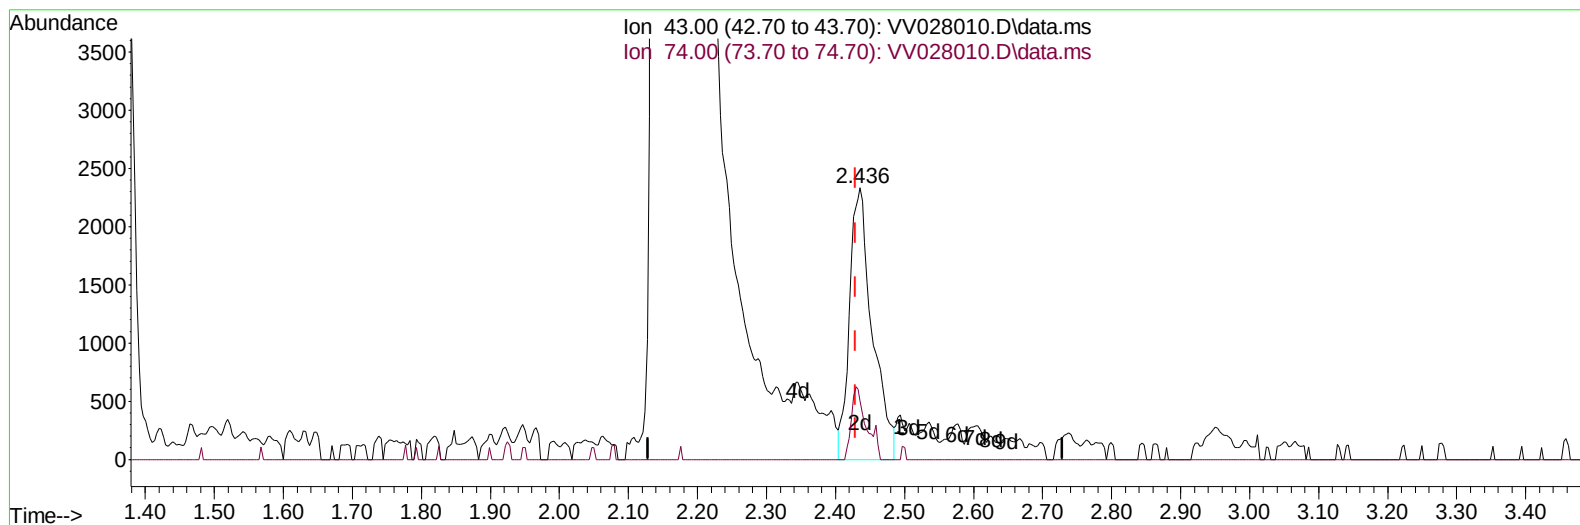

TIC: VV028010.D\data.ms

(15) Methyl Acetate (T)

2.436min (+ 0.007) 1.92 ug/L m

response 5342

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	26.10	0.79#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028010.D
 Acq On : 21 Sep 2022 12:37
 Operator : SY/MD
 Sample : N4674-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC5

Manual IntegrationsAPPROVED

Quant Time: Sep 22 03:22:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 03:03:58 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
 Supervised By :Mahesh Dadoda 09/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	346707	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	331842	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	156073	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	119973	39.417	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery =	78.840%		
7) Chloroethane-d5	1.558	69	107848	44.356	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery =	88.720%		
11) 1,1-Dichloroethene-d2	2.098	63	181723	33.702	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery =	67.400%		
21) 2-Butanone-d5	3.870	46	169103	93.432	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery =	93.430%		
24) Chloroform-d	4.336	84	230203	45.048	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	90.100%		
26) 1,2-Dichloroethane-d4	5.024	65	151632	45.787	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	91.580%		
32) Benzene-d6	5.040	84	447446	46.781	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	93.560%		
36) 1,2-Dichloropropane-d6	6.063	67	140401	47.537	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery =	95.080%		
41) Toluene-d8	7.310	98	390279	44.559	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	89.120%		
43) trans-1,3-Dichloroprop...	7.616	79	59791	40.483	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery =	80.960%		
47) 2-Hexanone-d5	8.085	63	129069	89.205	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery =	89.200%		
56) 1,1,2,2-Tetrachloroeth...	10.210	84	205349	47.237	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery =	94.480%		
66) 1,2-Dichlorobenzene-d4	11.619	152	160702	53.042	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	106.080%		
Target Compounds						
						Qvalue
13) Acetone	2.159	43	972323	602.813	ug/L	99
15) Methyl Acetate	2.436	43	5342m	1.917	ug/L	
34) Trichloroethene	5.915	95	7987	3.256	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028010.D
Acq On : 21 Sep 2022 12:37
Operator : SY/MD
Sample : N4674-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC5

Manual IntegrationsAPPROVED

Quant Time: Sep 22 03:22:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 22 03:03:58 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
Supervised By :Mahesh Dadoda 09/22/2022

