




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028029.D
 Acq On : 21 Sep 2022 20:53
 Operator : SY/MD
 Sample : N4677-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E94

Manual IntegrationsAPPROVED

Quant Time: Sep 22 03:26:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 03:03:58 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
 Supervised By :Mahesh Dadoda 09/22/2022

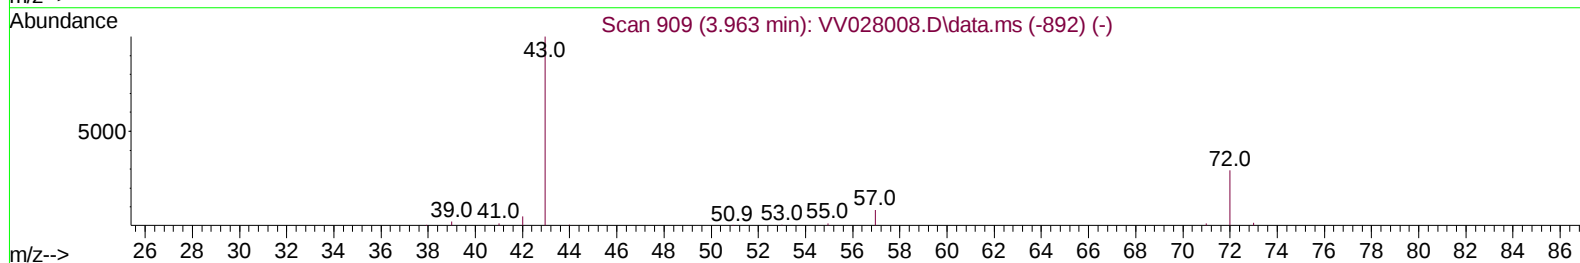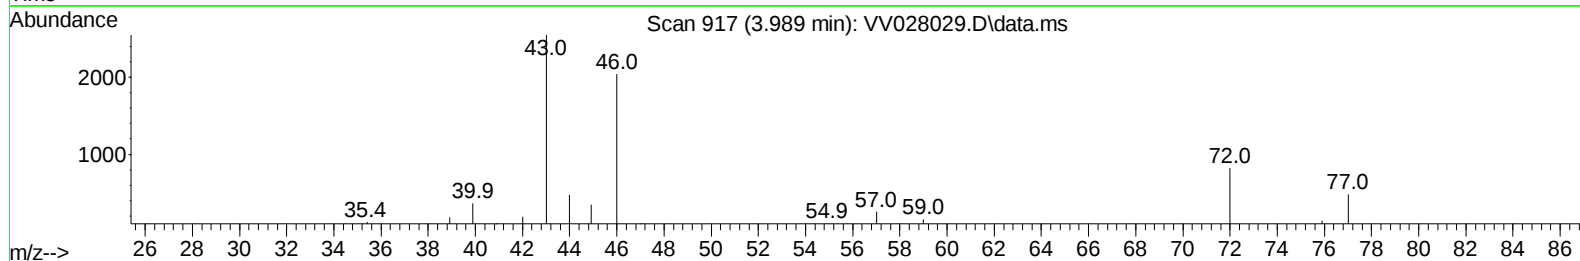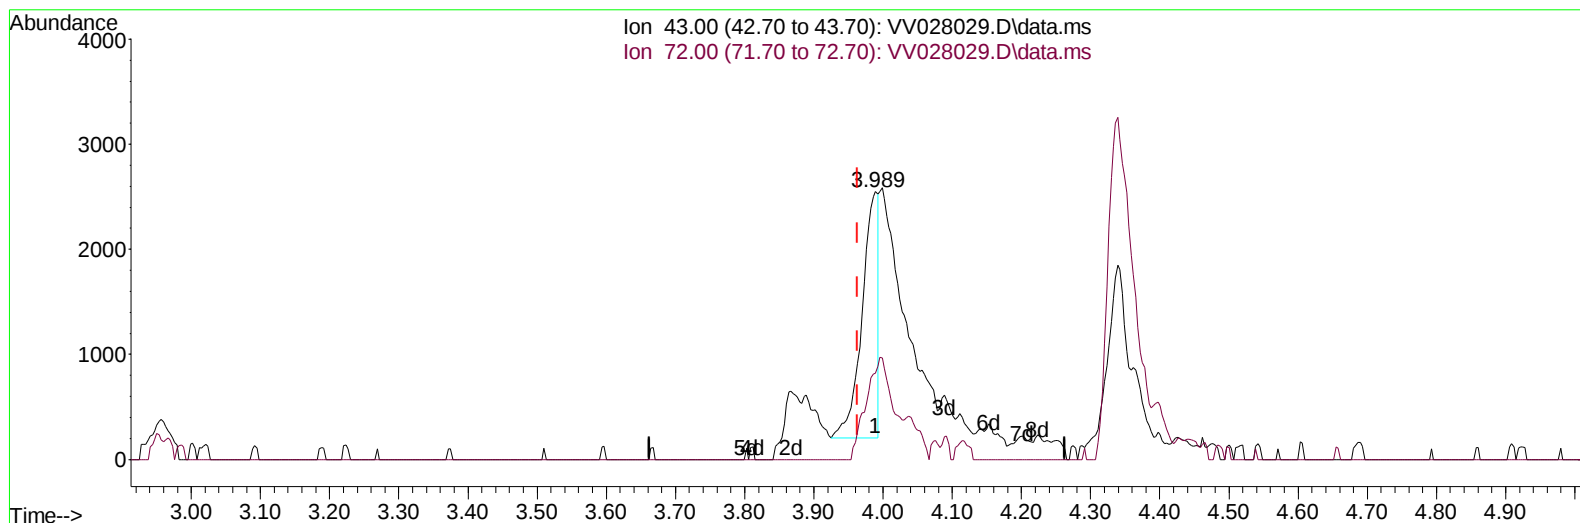

TIC: VV028029.D\data.ms

(22) 2-Butanone (T)

3.989min (+ 0.026) 2.07 ug/L

response 3748

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	26.90	68.09#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028029.D
 Acq On : 21 Sep 2022 20:53
 Operator : SY/MD
 Sample : N4677-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E94

Manual IntegrationsAPPROVED

Quant Time: Sep 22 03:26:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 03:03:58 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
 Supervised By :Mahesh Dadoda 09/22/2022

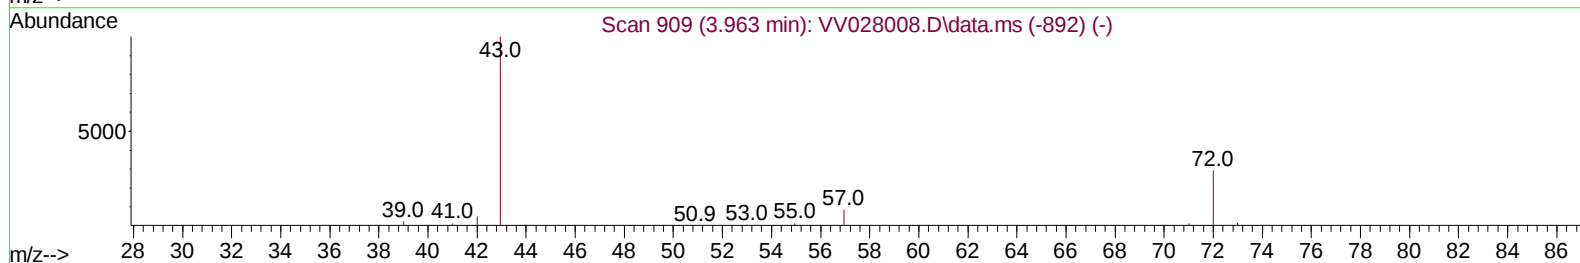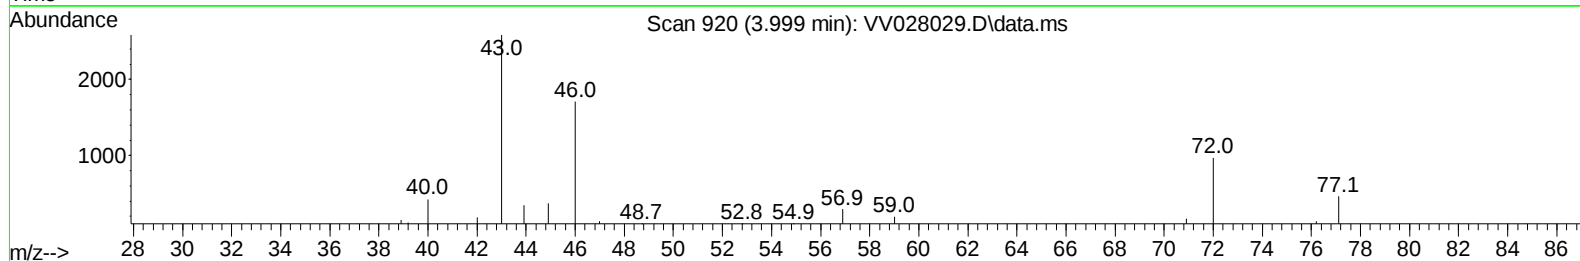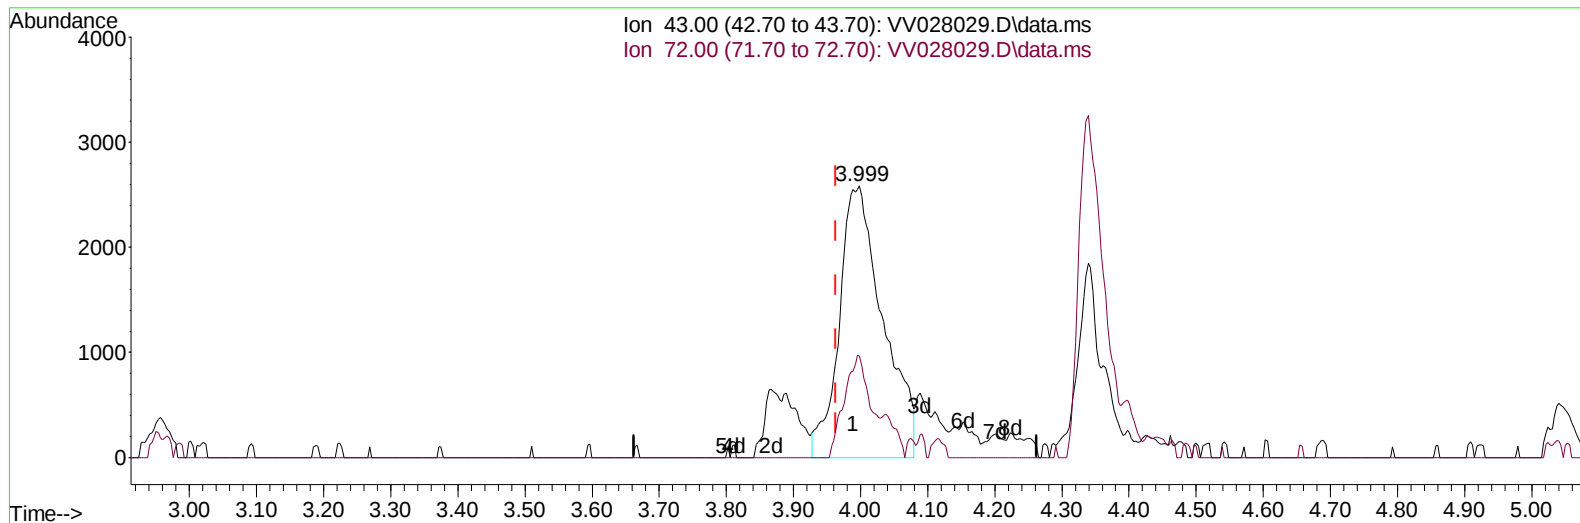

TIC: VV028029.D\data.ms

(22) 2-Butanone (T)

3.999min (+ 0.036) 6.43 ug/L m

response 11658

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	26.90	21.89
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028029.D
 Acq On : 21 Sep 2022 20:53
 Operator : SY/MD
 Sample : N4677-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E94

Manual IntegrationsAPPROVED

Quant Time: Sep 22 03:26:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 03:03:58 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
 Supervised By :Mahesh Dadoda 09/22/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.609	114		327231	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		325254	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152		143572	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		101451	35.315	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	70.640%	
7) Chloroethane-d5	1.558	69		93503	40.745	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	81.480%	
11) 1,1-Dichloroethene-d2	2.098	63		155163	30.489	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	60.980%	
21) 2-Butanone-d5	3.876	46		192869	112.905	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	112.910%	
24) Chloroform-d	4.339	84		215549	44.691	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	89.380%	
26) 1,2-Dichloroethane-d4	5.024	65		141450	45.255	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	90.500%	
32) Benzene-d6	5.044	84		399848	42.652	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	85.300%	
36) 1,2-Dichloropropane-d6	6.063	67		137695	47.565	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	95.140%	
41) Toluene-d8	7.310	98		348755	40.624	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	81.240%	
43) trans-1,3-Dichloroprop...	7.619	79		60256	41.624	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	83.240%	
47) 2-Hexanone-d5	8.085	63		151015	106.486	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	106.490%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		211613	49.664	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	99.320%	
66) 1,2-Dichlorobenzene-d4	11.622	152		139460	50.039	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	100.080%	
Target Compounds							
13) Acetone	2.169	43		16673	10.952	ug/L	98
22) 2-Butanone	3.999	43		11658m	6.433	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028029.D
Acq On : 21 Sep 2022 20:53
Operator : SY/MD
Sample : N4677-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E94

Manual IntegrationsAPPROVED

Quant Time: Sep 22 03:26:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 22 03:03:58 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
Supervised By :Mahesh Dadoda 09/22/2022

