




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028040.D
 Acq On : 22 Sep 2022 01:52
 Operator : SY/MD
 Sample : N4659-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E65

Manual IntegrationsAPPROVED

Quant Time: Sep 22 06:25:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 05:25:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
 Supervised By :Mahesh Dadoda 09/22/2022

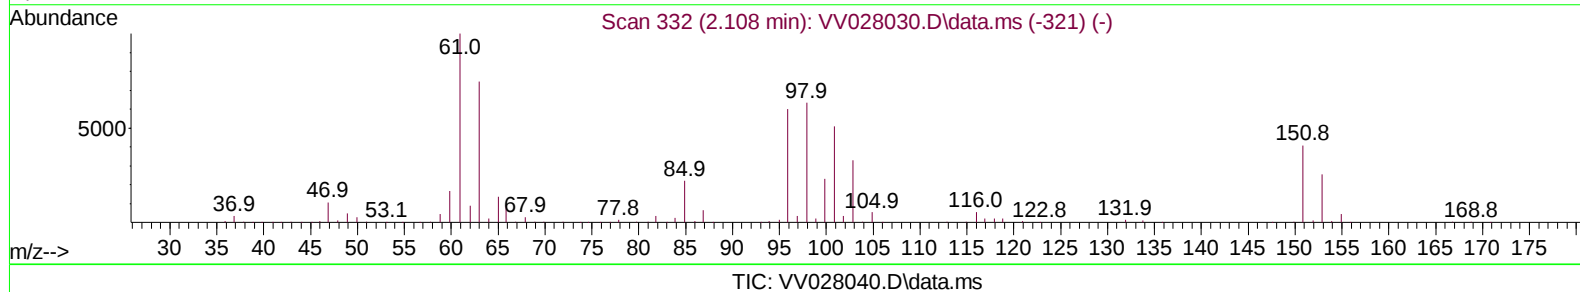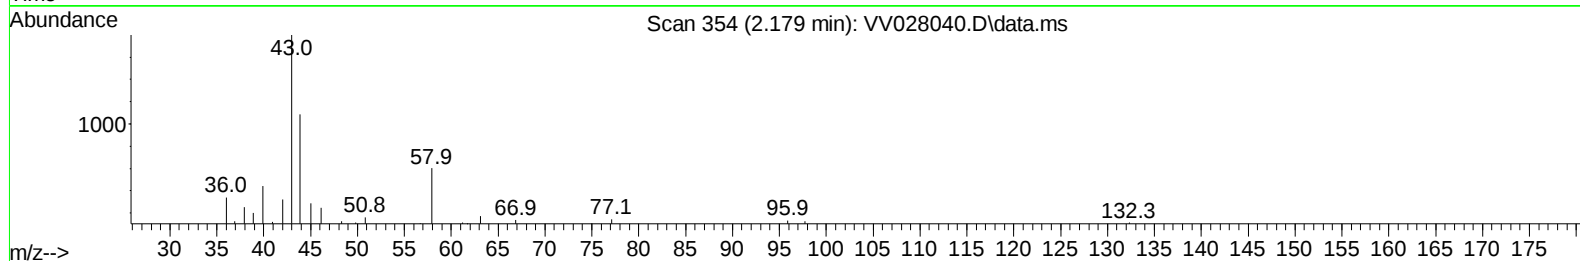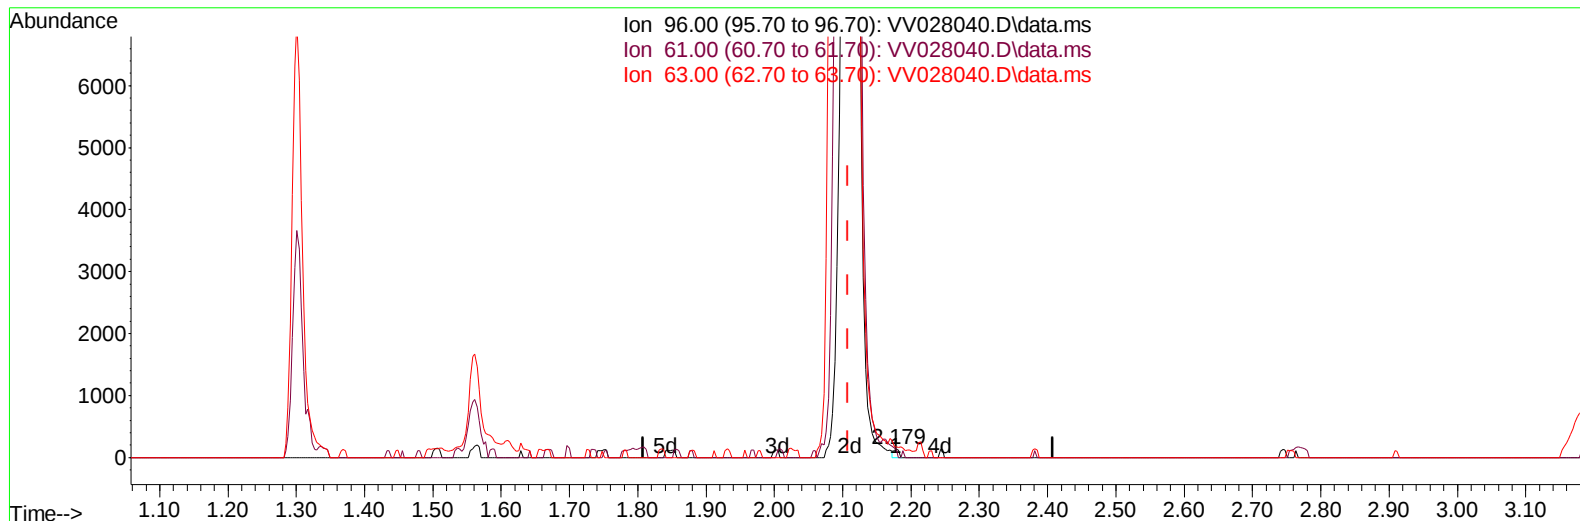

TIC: VV028040.D\data.ms

(12) 1,1-Dichloroethene (T)

2.179min (+ 0.071) 0.02 ug/L

response 69

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	176.70	166.67
63.00	155.10	132.58
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028040.D
 Acq On : 22 Sep 2022 01:52
 Operator : SY/MD
 Sample : N4659-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E65

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 09/22/2022
 Supervised By :Mahesh Dadoda 09/22/2022

Quant Time: Sep 22 06:25:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 05:25:17 2022
 Response via : Initial Calibration

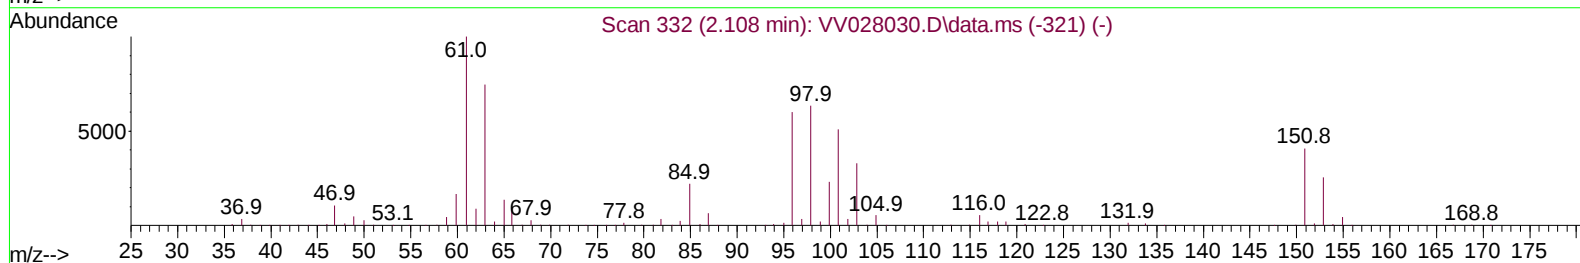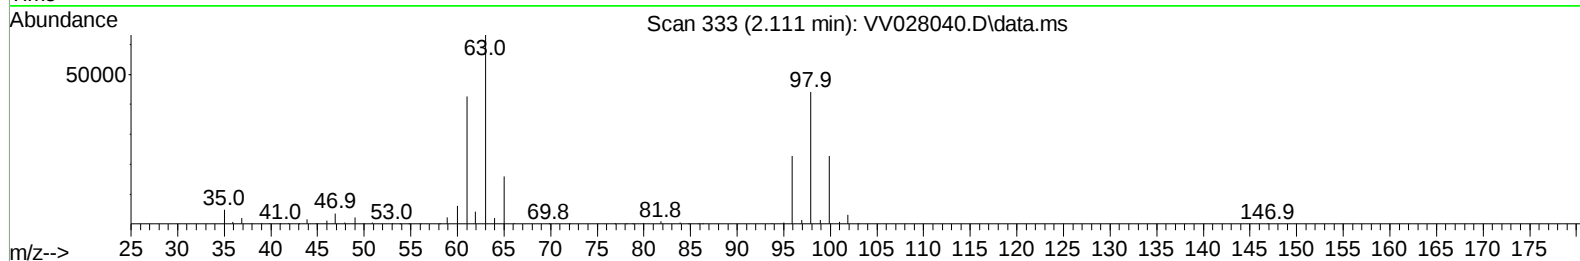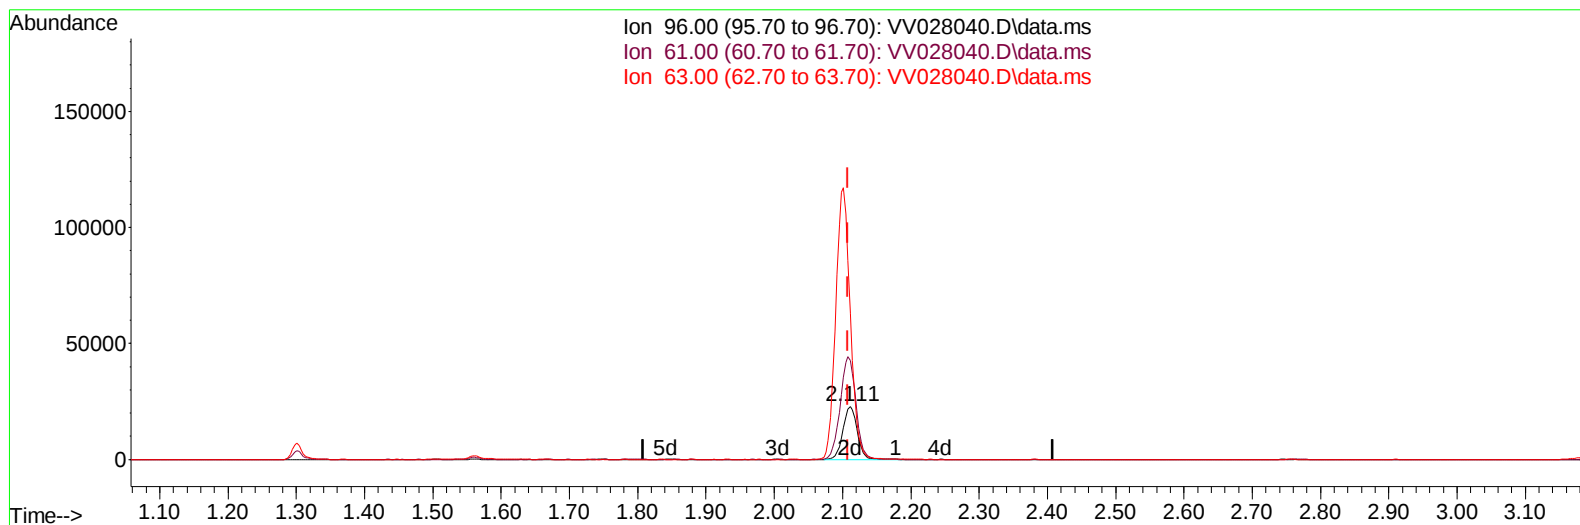

TIC: VV028040.D\data.ms

(12) 1,1-Dichloroethene (T)

2.111min (+ 0.003) 11.24 ug/L m

response 33173

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	176.70	186.57
63.00	155.10	276.93#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028040.D
 Acq On : 22 Sep 2022 01:52
 Operator : SY/MD
 Sample : N4659-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E65

Manual IntegrationsAPPROVED

Quant Time: Sep 22 06:25:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 05:25:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
 Supervised By :Mahesh Dadoda 09/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	406806	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	389199	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	167059	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	105984	29.677	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	59.360%#	
7) Chloroethane-d5	1.561	69	98225	34.430	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	68.860%#	
11) 1,1-Dichloroethene-d2	2.101	63	173858	27.480	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	54.960%#	
21) 2-Butanone-d5	3.880	46	196295	92.433	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	92.430%	
24) Chloroform-d	4.343	84	226693	37.808	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	75.620%	
26) 1,2-Dichloroethane-d4	5.024	65	156308	40.226	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	80.460%	
32) Benzene-d6	5.043	84	438806	39.117	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	78.240%	
36) 1,2-Dichloropropane-d6	6.063	67	140876	40.669	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	81.340%	
41) Toluene-d8	7.313	98	359399	34.986	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	69.980%#	
43) trans-1,3-Dichloroprop...	7.619	79	61690	35.613	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	71.220%	
47) 2-Hexanone-d5	8.085	63	148675	87.612	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	87.610%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	222718	43.682	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	87.360%	
66) 1,2-Dichlorobenzene-d4	11.622	152	144347	44.511	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	89.020%	
Target Compounds						
12) 1,1-Dichloroethene	2.111	96	33173m	11.239	ug/L	
20) cis-1,2-Dichloroethene	3.905	96	21214	6.771	ug/L	98
30) 1,1,1-Trichloroethane	4.603	97	30878	6.445	ug/L	98
34) Trichloroethene	5.905	95	464168	161.316	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028040.D
Acq On : 22 Sep 2022 01:52
Operator : SY/MD
Sample : N4659-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E65

Manual IntegrationsAPPROVED

Quant Time: Sep 22 06:25:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 22 05:25:17 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
Supervised By :Mahesh Dadoda 09/22/2022

