




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028050.D
 Acq On : 22 Sep 2022 06:00
 Operator : SY/MD
 Sample : N4659-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E62

Manual IntegrationsAPPROVED

Quant Time: Sep 22 08:42:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 05:25:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
 Supervised By :Mahesh Dadoda 09/22/2022

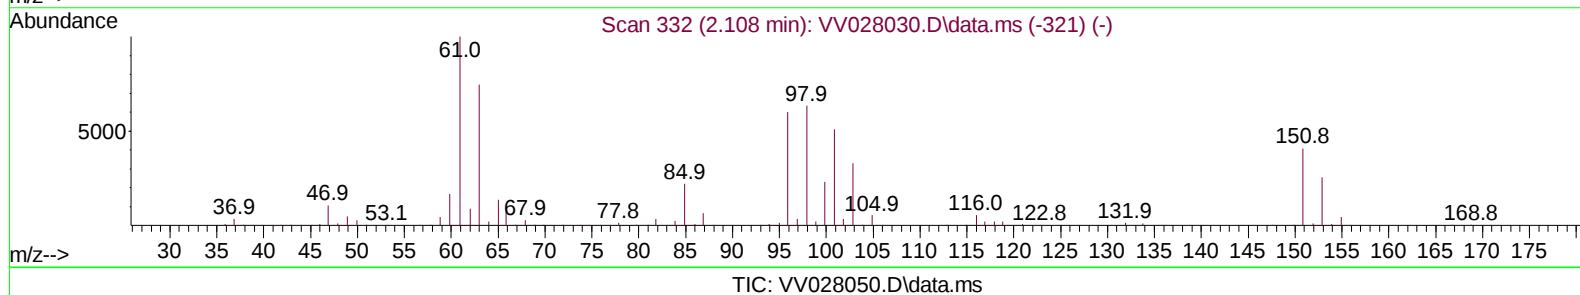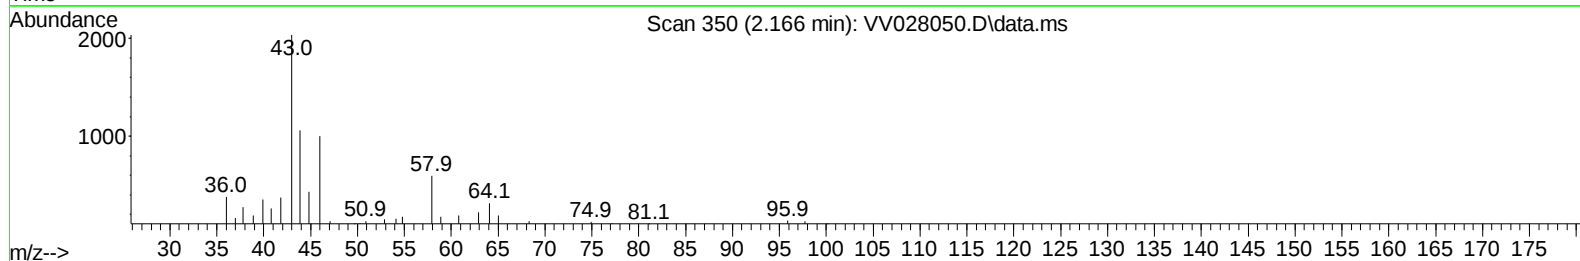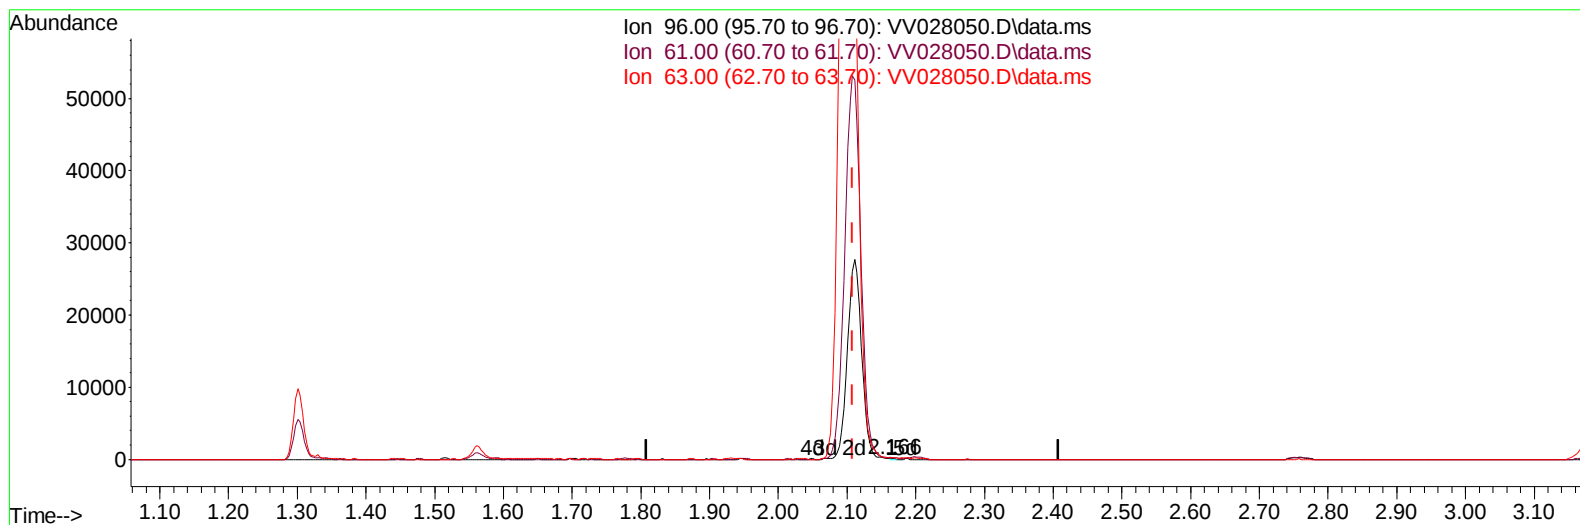

(12) 1,1-Dichloroethene (T)

2.166min (+ 0.058) 0.02 ug/L

response 48

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	176.70	142.11
63.00	155.10	166.17
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028050.D
Acq On : 22 Sep 2022 06:00
Operator : SY/MD
Sample : N4659-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E62

Manual IntegrationsAPPROVED

Quant Time: Sep 22 06:27:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 22 05:25:17 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
Supervised By :Mahesh Dadoda 09/22/2022

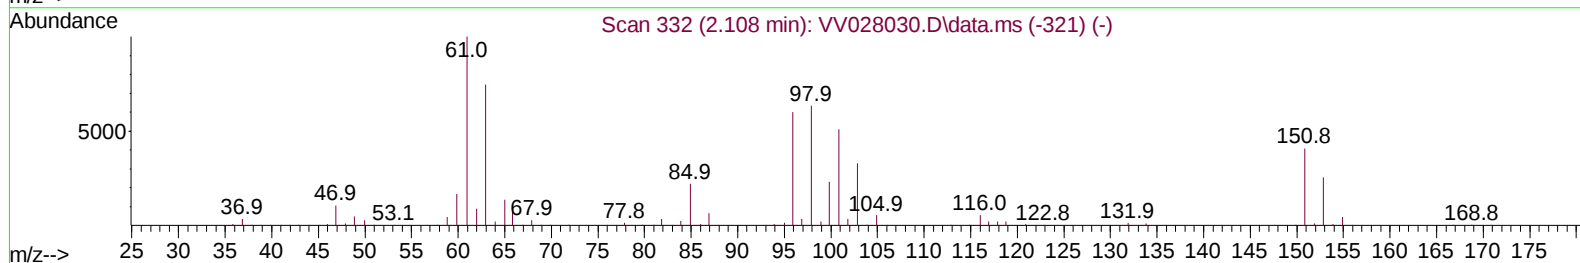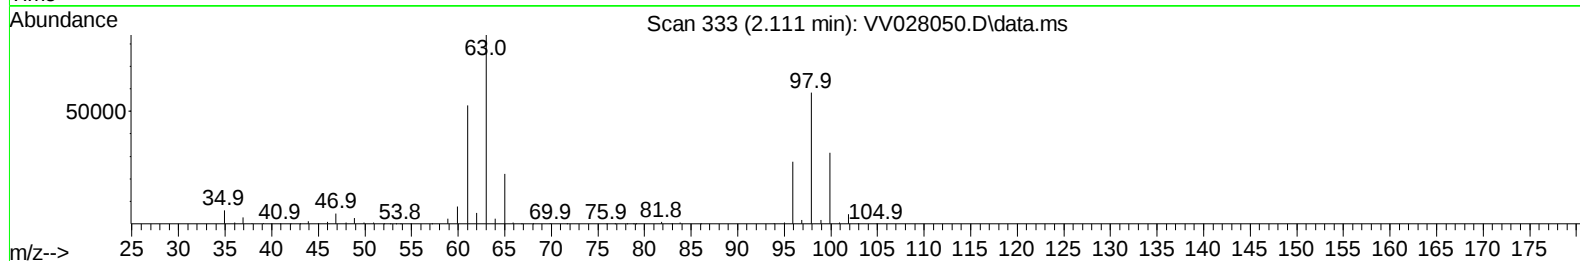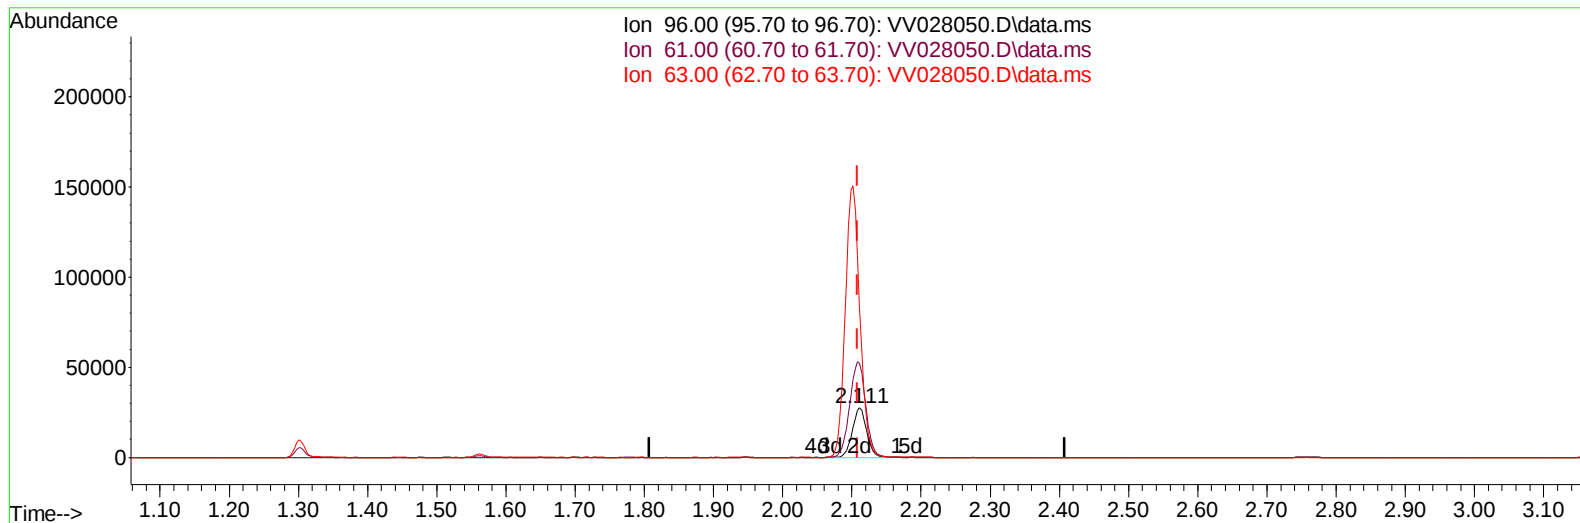

TIC: VV028050.D\data.ms

(12) 1,1-Dichloroethene (T)

2.111min (+ 0.003) 15.73 ug/L m

response 39879

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	176.70	189.71
63.00	155.10	302.80#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028050.D
 Acq On : 22 Sep 2022 06:00
 Operator : SY/MD
 Sample : N4659-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E62

Manual IntegrationsAPPROVED

Quant Time: Sep 22 06:27:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 05:25:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
 Supervised By :Mahesh Dadoda 09/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	349334	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	341587	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	153751	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	145128	47.323	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	94.640%	
7) Chloroethane-d5	1.561	69	119725	48.870	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	97.740%	
11) 1,1-Dichloroethene-d2	2.101	63	222226	40.903	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	81.800%	
21) 2-Butanone-d5	3.883	46	209650	114.963	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	114.960%	
24) Chloroform-d	4.339	84	252434	49.027	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	98.060%	
26) 1,2-Dichloroethane-d4	5.024	65	167767	50.279	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	100.560%	
32) Benzene-d6	5.043	84	509536	51.753	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	103.500%	
36) 1,2-Dichloropropane-d6	6.066	67	159005	52.300	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	104.600%	
41) Toluene-d8	7.310	98	439348	48.730	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	97.460%	
43) trans-1,3-Dichloroprop...	7.619	79	69198	45.516	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	91.040%	
47) 2-Hexanone-d5	8.085	63	152334	102.280	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	102.280%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	225200	50.326	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	100.660%	
66) 1,2-Dichlorobenzene-d4	11.622	152	172520	57.802	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	115.600%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.304	62	8535	2.720	ug/L	# 66
12) 1,1-Dichloroethene	2.111	96	39879m	15.734	ug/L	
13) Acetone	2.179	43	7710	4.744	ug/L	74
19) 1,1-Dichloroethane	3.182	63	7665	1.645	ug/L	96
20) cis-1,2-Dichloroethene	3.902	96	690908	256.799	ug/L	98
30) 1,1,1-Trichloroethane	4.603	97	42682	10.150	ug/L	100
34) Trichloroethene	5.912	95	28037	11.102	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028050.D
Acq On : 22 Sep 2022 06:00
Operator : SY/MD
Sample : N4659-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E62

Manual IntegrationsAPPROVED

Quant Time: Sep 22 06:27:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 22 05:25:17 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/22/2022
Supervised By :Mahesh Dadoda 09/22/2022

