

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW092122\
 Data File : VW028054.D
 Acq On : 22 Sep 2022 10:10
 Operator : SY/MD
 Sample : N4674-19DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC5DL

Quant Time: Sep 22 12:56:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 22 05:25:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	356753	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	339922	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	154992	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	152699	48.756	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	97.520%
7) Chloroethane-d5	1.561	69	124151	49.623	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.240%
11) 1,1-Dichloroethene-d2	2.098	63	210879	38.008	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.020%
21) 2-Butanone-d5	3.883	46	233478	125.367	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	125.370%
24) Chloroform-d	4.339	84	263837	50.176	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.360%
26) 1,2-Dichloroethane-d4	5.024	65	173236	50.838	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.680%
32) Benzene-d6	5.043	84	523639	53.446	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.900%
36) 1,2-Dichloropropane-d6	6.063	67	164452	54.357	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	108.720%
41) Toluene-d8	7.310	98	462069	51.501	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.000%
43) trans-1,3-Dichloroprop...	7.619	79	78364	51.797	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	103.600%
47) 2-Hexanone-d5	8.085	63	172408	116.326	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	116.330%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	229408	51.517	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.040%
66) 1,2-Dichlorobenzene-d4	11.622	152	172454	57.318	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	114.640%
Target Compounds						
13) Acetone	2.178	43	5875	3.540	ug/L	Qvalue 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028054.D
Acq On : 22 Sep 2022 10:10
Operator : SY/MD
Sample : N4674-19DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC5DL

Quant Time: Sep 22 12:56:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 22 05:25:17 2022
Response via : Initial Calibration

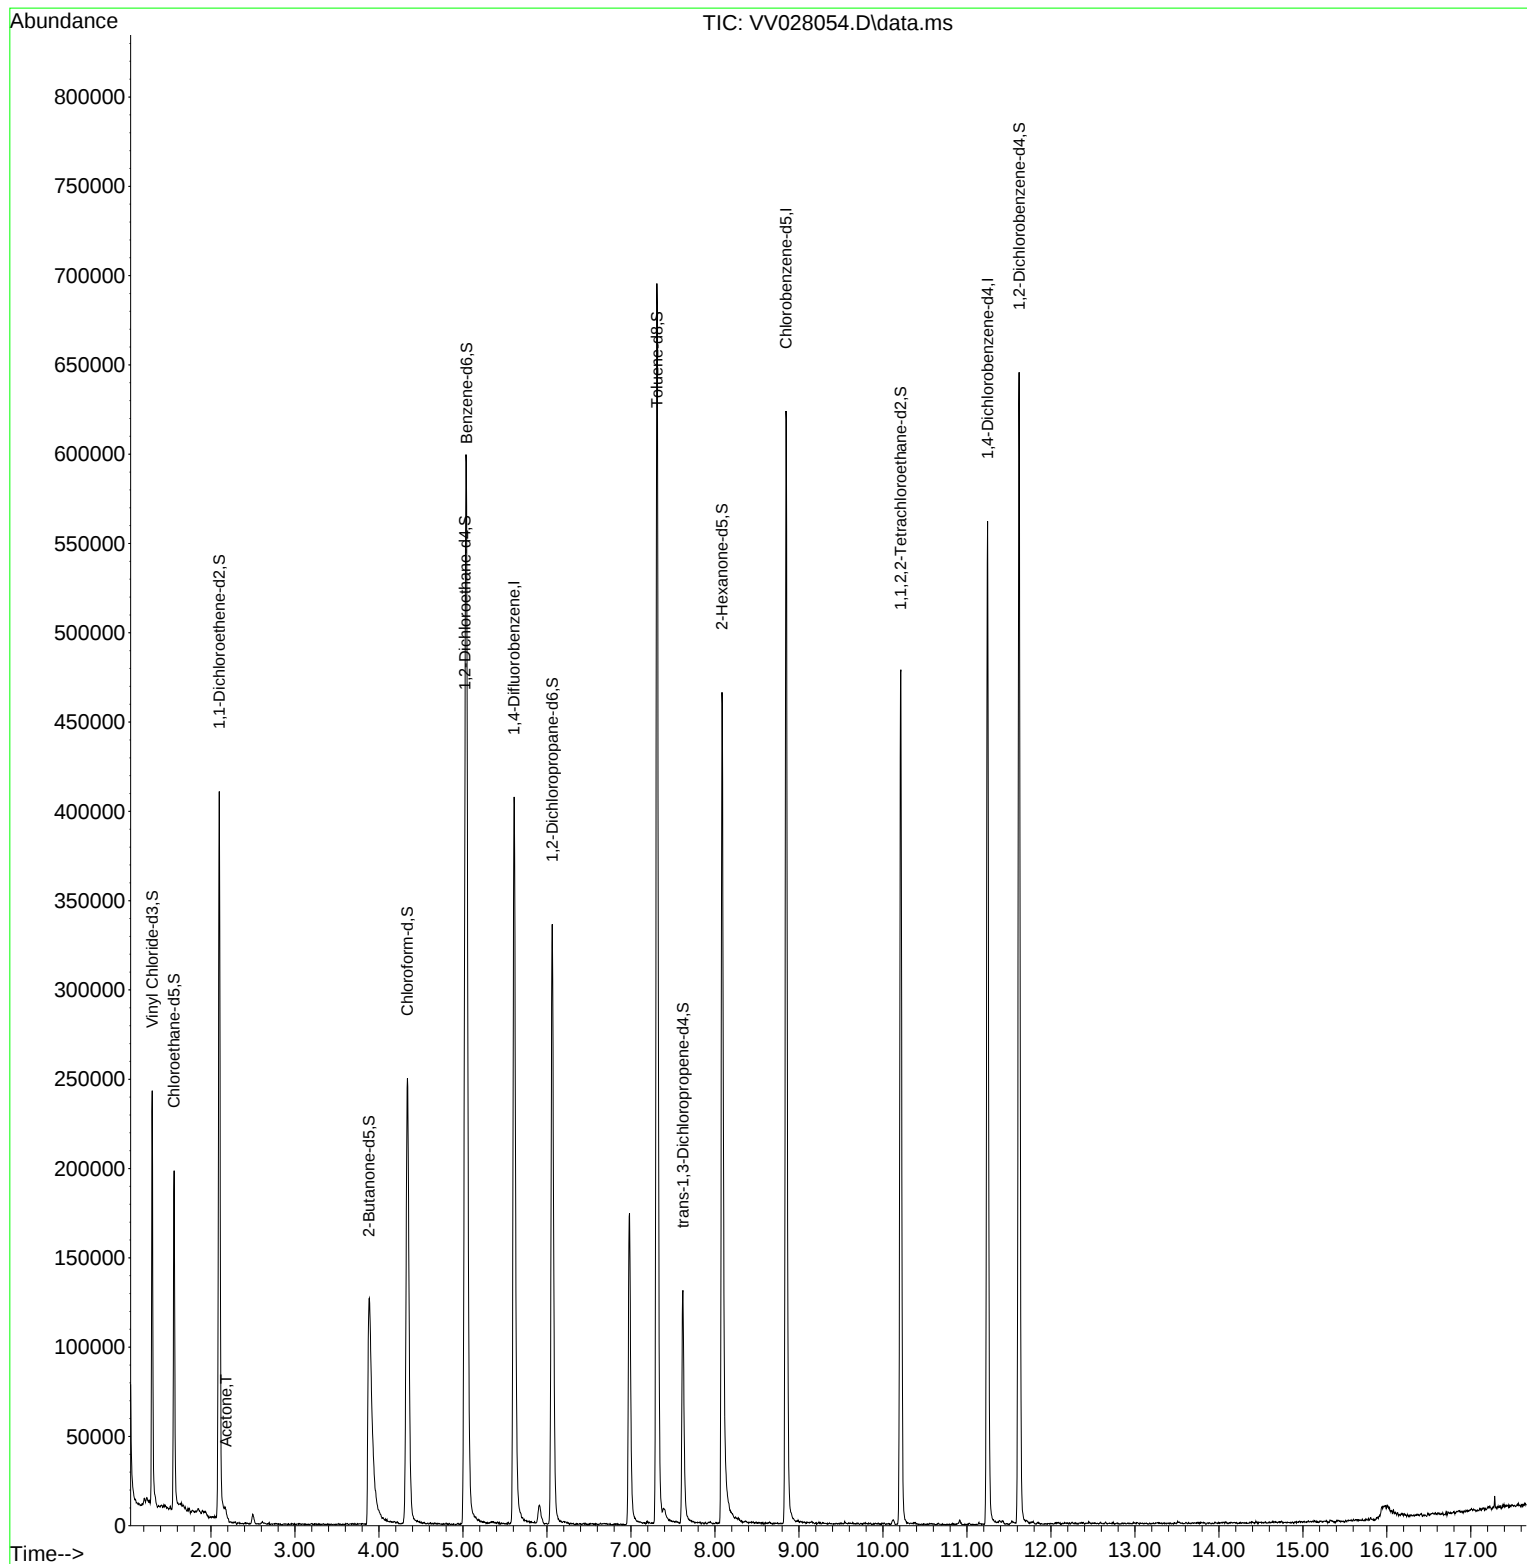

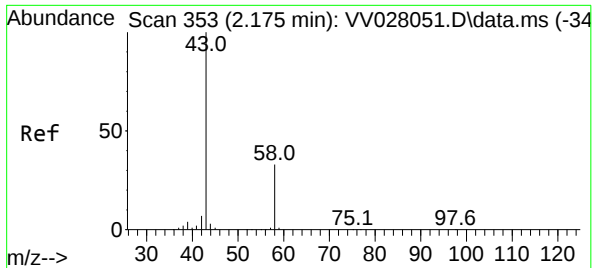

#13
 Acetone
 Concen: 3.540 ug/L
 RT: 2.178 min Scan# 31
 Delta R.T. 0.009 min
 Lab File: VV028054.D
 Acq: 22 Sep 2022 10:10

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC5DL

Tgt Ion: 43 Resp: 5875
 Ion Ratio Lower Upper
 43 100
 58 20.6 0.0 66.2

