

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028009.D
 Acq On : 21 Sep 2022 12:08
 Operator : SY/MD
 Sample : VV0921WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV028009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	228890	231719	14.92%	2.026%
2	1.561	155	162	175	rVB	183506	206198	13.28%	1.802%
3	2.098	320	329	358	rVB	383310	572068	36.83%	5.001%
4	2.494	447	452	453	rBV3	2120	1567	0.10%	0.014%
5	2.741	527	529	530	rBV3	538	223	0.01%	0.002%
6	2.902	575	579	582	rVB2	396	354	0.02%	0.003%
7	2.924	582	586	590	rBV3	369	268	0.02%	0.002%
8	2.950	592	594	597	rVV2	422	237	0.02%	0.002%
9	3.069	628	631	633	rBV	460	300	0.02%	0.003%
10	3.124	645	648	651	rBV3	633	414	0.03%	0.004%
11	3.291	697	700	703	rBV2	527	423	0.03%	0.004%
12	3.355	716	720	724	rBV4	380	295	0.02%	0.003%
13	3.474	754	757	758	rBV	566	301	0.02%	0.003%
14	3.484	758	760	763	rVB2	792	379	0.02%	0.003%
15	3.551	778	781	783	rBV	409	267	0.02%	0.002%
16	3.654	811	813	817	rVB2	589	412	0.03%	0.004%
17	3.715	828	832	835	rVB3	689	443	0.03%	0.004%
18	3.735	835	838	840	rBV	342	227	0.01%	0.002%
19	3.873	871	881	919	rBV	126858	367470	23.66%	3.212%
20	4.336	1010	1025	1048	rBV	248506	613926	39.52%	5.367%
21	4.606	1107	1109	1112	rBV3	697	434	0.03%	0.004%
22	4.783	1162	1164	1168	rBV2	357	235	0.02%	0.002%
23	4.812	1168	1173	1177	rBV5	1040	1159	0.07%	0.010%
24	4.857	1184	1187	1189	rBV2	543	352	0.02%	0.003%
25	4.895	1197	1199	1202	rVB2	522	322	0.02%	0.003%
26	4.963	1218	1220	1223	rBV2	392	332	0.02%	0.003%
27	5.034	1226	1242	1275	rVV2	608828	1553275	100.00%	13.578%
28	5.368	1342	1346	1348	rBV3	1149	869	0.06%	0.008%
29	5.384	1349	1351	1355	rVB4	1000	671	0.04%	0.006%
30	5.506	1386	1389	1390	rBV	497	344	0.02%	0.003%
31	5.545	1397	1401	1402	rBV2	701	493	0.03%	0.004%
32	5.606	1408	1420	1448	rBV	424290	859735	55.35%	7.515%
33	5.831	1487	1490	1492	rBV4	862	367	0.02%	0.003%
34	5.969	1531	1533	1535	rBV2	887	565	0.04%	0.005%
35	6.059	1547	1561	1591	rBV	346293	711245	45.79%	6.217%
36	6.297	1633	1635	1638	rVB2	968	465	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028009.D
 Acq On : 21 Sep 2022 12:08
 Operator : SY/MD
 Sample : VV0921WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.506	1695	1700	1701	rBV3	736	482	0.03%	0.004%
38	6.558	1713	1716	1718	rBV	416	248	0.02%	0.002%
39	6.606	1728	1731	1733	rBV2	732	380	0.02%	0.003%
40	6.638	1735	1741	1746	rBV7	957	1567	0.10%	0.014%
41	6.918	1823	1828	1832	rVB4	469	444	0.03%	0.004%
42	6.979	1833	1847	1864	rBV2	170557	315330	20.30%	2.756%
43	7.310	1936	1950	1969	rBV	665060	1161695	74.79%	10.155%
44	7.616	2035	2045	2068	rBV	131389	232441	14.96%	2.032%
45	7.873	2123	2125	2126	rBV2	728	241	0.02%	0.002%
46	8.030	2170	2174	2176	rBV4	1170	762	0.05%	0.007%
47	8.043	2176	2178	2180	rVB3	716	256	0.02%	0.002%
48	8.085	2180	2191	2224	rBV	437769	807943	52.02%	7.063%
49	8.715	2382	2387	2389	rBV3	679	675	0.04%	0.006%
50	8.847	2416	2428	2451	rBV	648841	1047904	67.46%	9.160%
51	9.079	2497	2500	2502	rBV3	1062	578	0.04%	0.005%
52	9.136	2510	2518	2519	rBV5	1166	1018	0.07%	0.009%
53	9.233	2545	2548	2550	rBV	470	290	0.02%	0.003%
54	9.246	2550	2552	2554	rBV	693	413	0.03%	0.004%
55	9.313	2569	2573	2577	rVB3	911	819	0.05%	0.007%
56	9.410	2599	2603	2605	rBV5	897	697	0.04%	0.006%
57	9.448	2611	2615	2616	rBV2	929	472	0.03%	0.004%
58	9.477	2622	2624	2627	rBV2	617	387	0.02%	0.003%
59	9.799	2721	2724	2728	rVB3	837	558	0.04%	0.005%
60	9.857	2740	2742	2746	rVB2	649	256	0.02%	0.002%
61	9.905	2754	2757	2760	rBV2	802	442	0.03%	0.004%
62	9.931	2760	2765	2766	rBV3	1207	844	0.05%	0.007%
63	10.021	2788	2793	2797	rBV3	624	780	0.05%	0.007%
64	10.079	2807	2811	2812	rBV2	635	387	0.02%	0.003%
65	10.117	2818	2823	2824	rBV4	1647	1157	0.07%	0.010%
66	10.210	2841	2852	2869	rBV	491995	761599	49.03%	6.658%
67	10.374	2901	2903	2905	rBV2	1245	627	0.04%	0.005%
68	10.493	2938	2940	2944	rVB3	557	341	0.02%	0.003%
69	10.542	2948	2955	2957	rBV4	1322	1375	0.09%	0.012%
70	10.654	2988	2990	2992	rBV2	626	284	0.02%	0.002%
71	10.725	3009	3012	3013	rBV2	369	229	0.01%	0.002%
72	10.754	3017	3021	3023	rBV2	637	460	0.03%	0.004%
73	10.834	3043	3046	3047	rBV2	865	467	0.03%	0.004%
74	10.918	3064	3072	3079	rVB7	2956	4246	0.27%	0.037%
75	10.995	3094	3096	3099	rVB3	550	317	0.02%	0.003%
76	11.120	3130	3135	3137	rBV2	580	399	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028009.D
 Acq On : 21 Sep 2022 12:08
 Operator : SY/MD
 Sample : VV0921WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.140	3137	3141	3144	rBV4	989	1117	0.07%	0.010%
78	11.172	3149	3151	3154	rBV3	760	421	0.03%	0.004%
79	11.246	3162	3174	3195	rBV	584851	912572	58.75%	7.977%
80	11.423	3223	3229	3231	rBV4	1251	1181	0.08%	0.010%
81	11.551	3265	3269	3270	rBV2	713	409	0.03%	0.004%
82	11.619	3278	3290	3311	rBV	659809	1033750	66.55%	9.037%
83	11.921	3381	3384	3385	rBV3	506	342	0.02%	0.003%
84	11.982	3401	3403	3405	rBV	522	286	0.02%	0.003%
85	12.033	3417	3419	3423	rVB2	647	293	0.02%	0.003%
86	12.535	3572	3575	3577	rBV2	516	246	0.02%	0.002%
87	12.606	3596	3597	3603	rVB6	785	454	0.03%	0.004%
88	12.651	3603	3611	3617	rBV8	1946	2745	0.18%	0.024%
89	12.702	3626	3627	3631	rBV3	582	372	0.02%	0.003%
90	12.844	3669	3671	3674	rBV2	702	412	0.03%	0.004%
91	12.921	3692	3695	3700	rVB3	755	591	0.04%	0.005%
92	12.966	3706	3709	3711	rBV3	1004	634	0.04%	0.006%
93	13.268	3795	3803	3809	rBV7	1856	2679	0.17%	0.023%
94	13.445	3856	3858	3860	rVB2	696	279	0.02%	0.002%
95	13.554	3890	3892	3896	rBV3	703	561	0.04%	0.005%
96	13.721	3942	3944	3947	rBV3	647	271	0.02%	0.002%
97	13.869	3985	3990	3991	rBV2	927	627	0.04%	0.005%
98	13.902	3997	4000	4003	rBV3	653	519	0.03%	0.005%
99	13.966	4018	4020	4023	rBV3	665	350	0.02%	0.003%
100	14.705	4248	4250	4253	rBV2	1023	436	0.03%	0.004%




Sum of corrected areas: 11439711

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028009.D
Acq On : 21 Sep 2022 12:08
Operator : SY/MD
Sample : VV0921WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

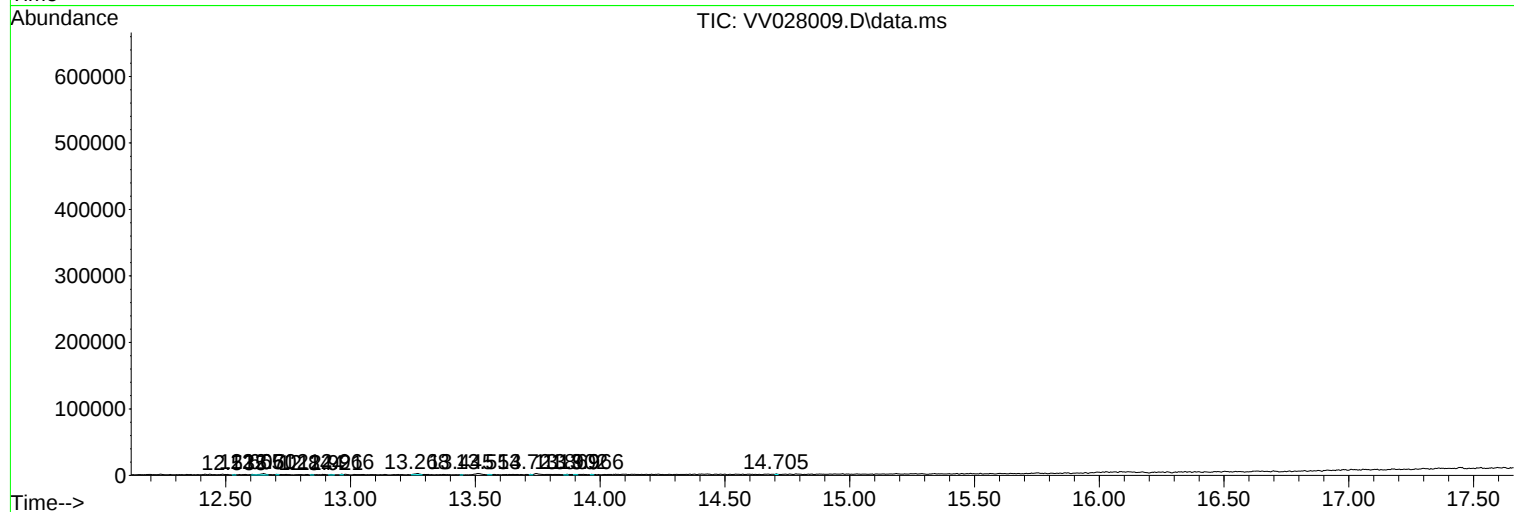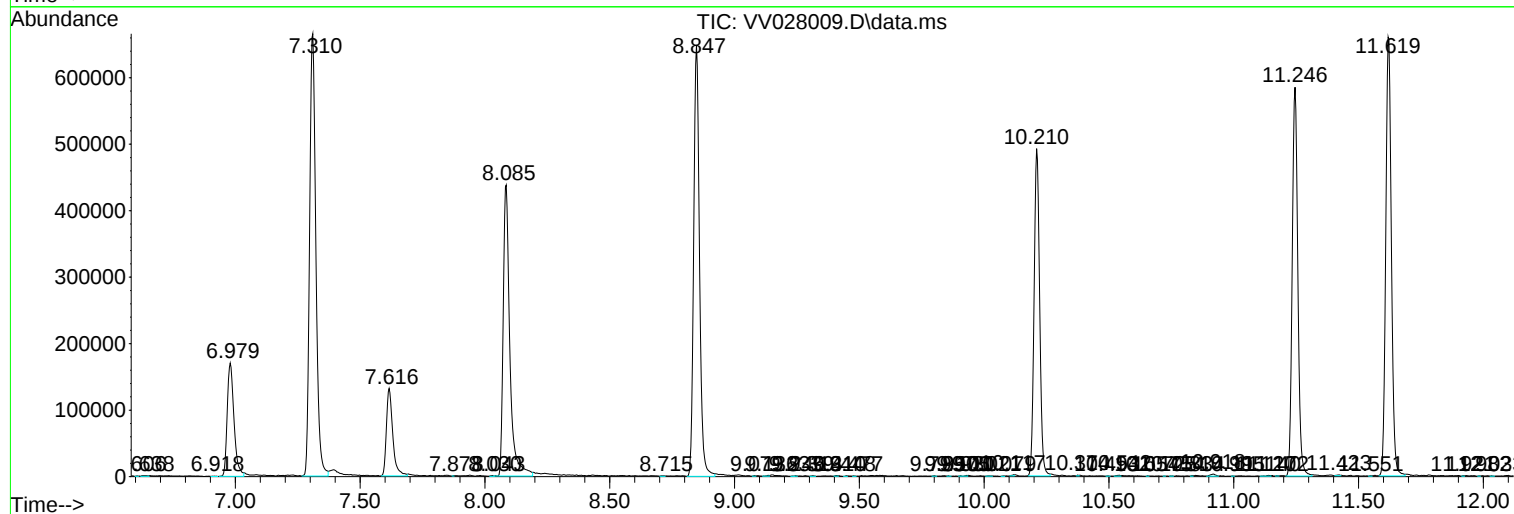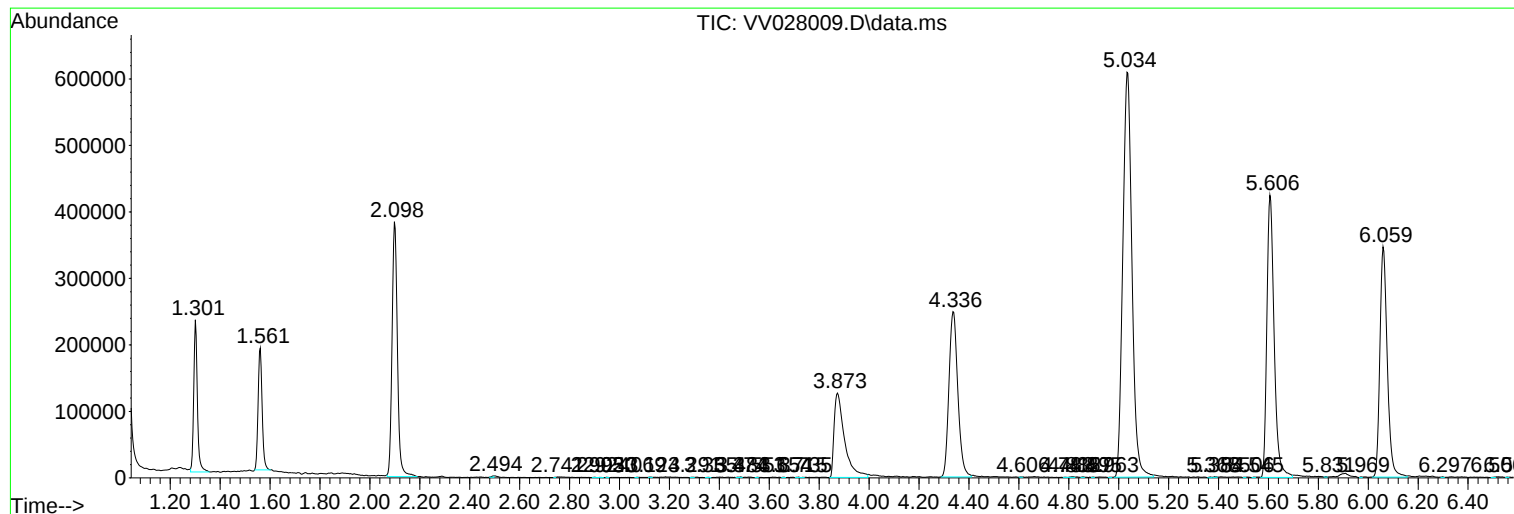

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028009.D
Acq On : 21 Sep 2022 12:08
Operator : SY/MD
Sample : VV0921WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028009.D
Acq On : 21 Sep 2022 12:08
Operator : SY/MD
Sample : VV0921WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc