

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028011.D
 Acq On : 21 Sep 2022 13:02
 Operator : SY/MD
 Sample : N4674-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	98	rVB	184421	190311	13.49%	1.824%
2	1.561	155	162	176	rVB	162372	187377	13.28%	1.796%
3	2.101	320	330	344	rBV	334693	483594	34.27%	4.635%
4	2.619	489	491	492	rBV	522	222	0.02%	0.002%
5	2.748	528	531	533	rBV2	1063	635	0.05%	0.006%
6	2.802	544	548	551	rBV4	416	271	0.02%	0.003%
7	2.822	551	554	556	rBV3	516	321	0.02%	0.003%
8	2.879	570	572	574	rBV2	552	295	0.02%	0.003%
9	3.011	610	613	614	rBV2	484	251	0.02%	0.002%
10	3.040	619	622	625	rVB2	815	537	0.04%	0.005%
11	3.108	641	643	649	rVB3	834	597	0.04%	0.006%
12	3.156	655	658	660	rBV2	701	438	0.03%	0.004%
13	3.233	678	682	683	rBV2	302	224	0.02%	0.002%
14	3.330	709	712	715	rVB2	590	306	0.02%	0.003%
15	3.352	715	719	721	rBV3	549	446	0.03%	0.004%
16	3.375	723	726	728	rBV3	494	314	0.02%	0.003%
17	3.461	750	753	754	rBV2	480	222	0.02%	0.002%
18	3.487	759	761	765	rBV2	374	221	0.02%	0.002%
19	3.519	769	771	776	rVB3	483	422	0.03%	0.004%
20	3.609	796	799	801	rBV3	682	368	0.03%	0.004%
21	3.658	812	814	816	rBV2	384	229	0.02%	0.002%
22	3.812	857	862	863	rBV3	672	476	0.03%	0.005%
23	3.873	872	881	926	rVV	120264	350844	24.87%	3.363%
24	4.339	1008	1026	1055	rBV	232606	579072	41.04%	5.550%
25	4.773	1159	1161	1165	rVB3	762	426	0.03%	0.004%
26	4.799	1165	1169	1171	rBV2	725	523	0.04%	0.005%
27	4.892	1191	1198	1200	rBV5	1230	816	0.06%	0.008%
28	4.953	1215	1217	1221	rVB	353	231	0.02%	0.002%
29	5.040	1227	1244	1273	rBV2	546180	1410968	100.00%	13.523%
30	5.609	1406	1421	1445	rBV	399455	818064	57.98%	7.841%
31	5.905	1504	1513	1517	rBV6	4661	7366	0.52%	0.071%
32	5.969	1531	1533	1536	rBV3	584	373	0.03%	0.004%
33	6.063	1548	1562	1593	rBV	314053	653228	46.30%	6.261%
34	6.413	1668	1671	1674	rBV4	854	631	0.04%	0.006%
35	6.432	1674	1677	1678	rBV	511	225	0.02%	0.002%
36	6.477	1686	1691	1695	rBV3	803	750	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028011.D
 Acq On : 21 Sep 2022 13:02
 Operator : SY/MD
 Sample : N4674-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.529	1699	1707	1710	rBV6	1013	1166	0.08%	0.011%
38	6.545	1710	1712	1714	rVV2	650	243	0.02%	0.002%
39	6.574	1717	1721	1724	rBV3	938	803	0.06%	0.008%
40	6.786	1785	1787	1789	rBV2	698	305	0.02%	0.003%
41	6.799	1789	1791	1794	rVV2	473	297	0.02%	0.003%
42	6.847	1802	1806	1808	rBV2	1024	525	0.04%	0.005%
43	6.873	1812	1814	1816	rBV2	753	345	0.02%	0.003%
44	6.905	1821	1824	1825	rBV2	374	221	0.02%	0.002%
45	6.928	1828	1831	1832	rBV2	681	402	0.03%	0.004%
46	6.982	1837	1848	1871	rBV	151000	276359	19.59%	2.649%
47	7.188	1909	1912	1914	rBV3	924	664	0.05%	0.006%
48	7.204	1914	1917	1920	rVV3	892	631	0.04%	0.006%
49	7.310	1938	1950	1970	rBV	602181	1047269	74.22%	10.037%
50	7.619	2035	2046	2075	rBV2	106939	197368	13.99%	1.892%
51	7.815	2105	2107	2109	rBV	613	327	0.02%	0.003%
52	7.902	2132	2134	2136	rBV	488	239	0.02%	0.002%
53	8.085	2181	2191	2226	rBV	391894	719904	51.02%	6.900%
54	8.808	2414	2416	2417	rBV	715	322	0.02%	0.003%
55	8.847	2417	2428	2451	rVV	607687	991278	70.26%	9.501%
56	9.114	2509	2511	2514	rBV2	502	237	0.02%	0.002%
57	9.201	2534	2538	2539	rBV2	400	277	0.02%	0.003%
58	9.284	2560	2564	2565	rBV2	600	413	0.03%	0.004%
59	9.294	2565	2567	2570	rVV2	734	351	0.02%	0.003%
60	9.390	2594	2597	2599	rBV3	462	271	0.02%	0.003%
61	9.445	2610	2614	2616	rBV2	636	398	0.03%	0.004%
62	9.464	2616	2620	2623	rBV3	500	382	0.03%	0.004%
63	9.554	2646	2648	2650	rVB2	730	321	0.02%	0.003%
64	9.702	2693	2694	2698	rVB2	572	294	0.02%	0.003%
65	9.767	2712	2714	2716	rBV2	416	290	0.02%	0.003%
66	9.796	2721	2723	2725	rVV2	694	380	0.03%	0.004%
67	9.831	2730	2734	2740	rVV5	736	868	0.06%	0.008%
68	9.860	2741	2743	2747	rVB	513	314	0.02%	0.003%
69	9.905	2755	2757	2760	rBV	764	434	0.03%	0.004%
70	10.040	2796	2799	2800	rBV2	513	243	0.02%	0.002%
71	10.120	2819	2824	2826	rBV5	982	887	0.06%	0.009%
72	10.169	2836	2839	2841	rBV2	530	363	0.03%	0.003%
73	10.214	2841	2853	2873	rVV	460798	727355	51.55%	6.971%
74	10.567	2961	2963	2968	rVB4	839	603	0.04%	0.006%
75	10.603	2972	2974	2980	rVB4	504	292	0.02%	0.003%
76	10.641	2983	2986	2989	rBV3	415	333	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028011.D
 Acq On : 21 Sep 2022 13:02
 Operator : SY/MD
 Sample : N4674-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.699	3002	3004	3006	rVB2	703	299	0.02%	0.003%
78	10.715	3006	3009	3012	rBV2	741	530	0.04%	0.005%
79	10.741	3015	3017	3019	rVV	684	341	0.02%	0.003%
80	10.763	3022	3024	3027	rVB	742	247	0.02%	0.002%
81	10.921	3067	3073	3077	rVB3	998	1136	0.08%	0.011%
82	11.024	3103	3105	3106	rBV2	715	332	0.02%	0.003%
83	11.246	3163	3174	3195	rBV	554146	844893	59.88%	8.098%
84	11.532	3255	3263	3265	rBV4	5971	6560	0.46%	0.063%
85	11.622	3280	3291	3311	rVB	576824	906930	64.28%	8.692%
86	11.831	3354	3356	3359	rVB2	894	430	0.03%	0.004%
87	11.950	3390	3393	3394	rBV3	694	390	0.03%	0.004%
88	12.127	3446	3448	3450	rBV2	872	501	0.04%	0.005%
89	12.467	3552	3554	3557	rBV2	314	230	0.02%	0.002%
90	12.535	3571	3575	3577	rBV3	612	409	0.03%	0.004%
91	12.673	3614	3618	3621	rVB3	715	446	0.03%	0.004%
92	13.146	3763	3765	3768	rBV3	574	281	0.02%	0.003%
93	13.329	3818	3822	3823	rBV2	524	274	0.02%	0.003%
94	13.439	3853	3856	3859	rBV2	1006	585	0.04%	0.006%
95	13.496	3868	3874	3876	rBV4	731	863	0.06%	0.008%
96	13.583	3897	3901	3902	rBV2	819	573	0.04%	0.005%
97	13.902	3997	4000	4003	rBV3	729	450	0.03%	0.004%
98	13.924	4003	4007	4009	rBV3	556	414	0.03%	0.004%
99	14.104	4061	4063	4065	rBV2	723	311	0.02%	0.003%
100	14.651	4230	4233	4236	rBV4	901	732	0.05%	0.007%




Sum of corrected areas: 10433725

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028011.D
Acq On : 21 Sep 2022 13:02
Operator : SY/MD
Sample : N4674-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

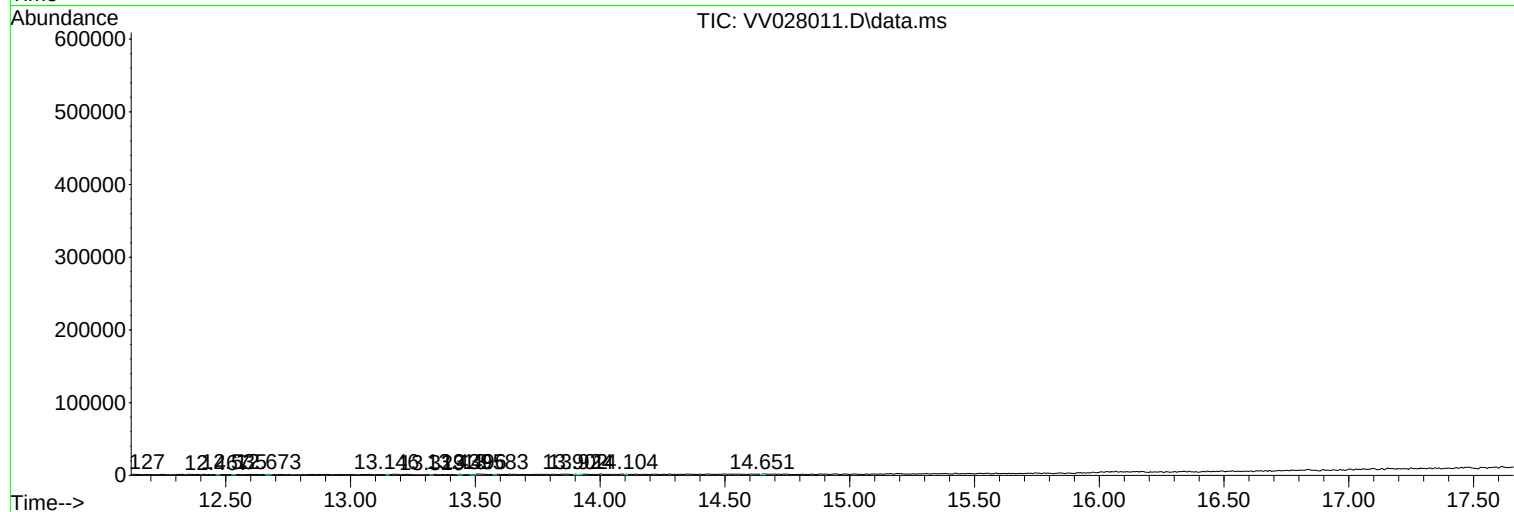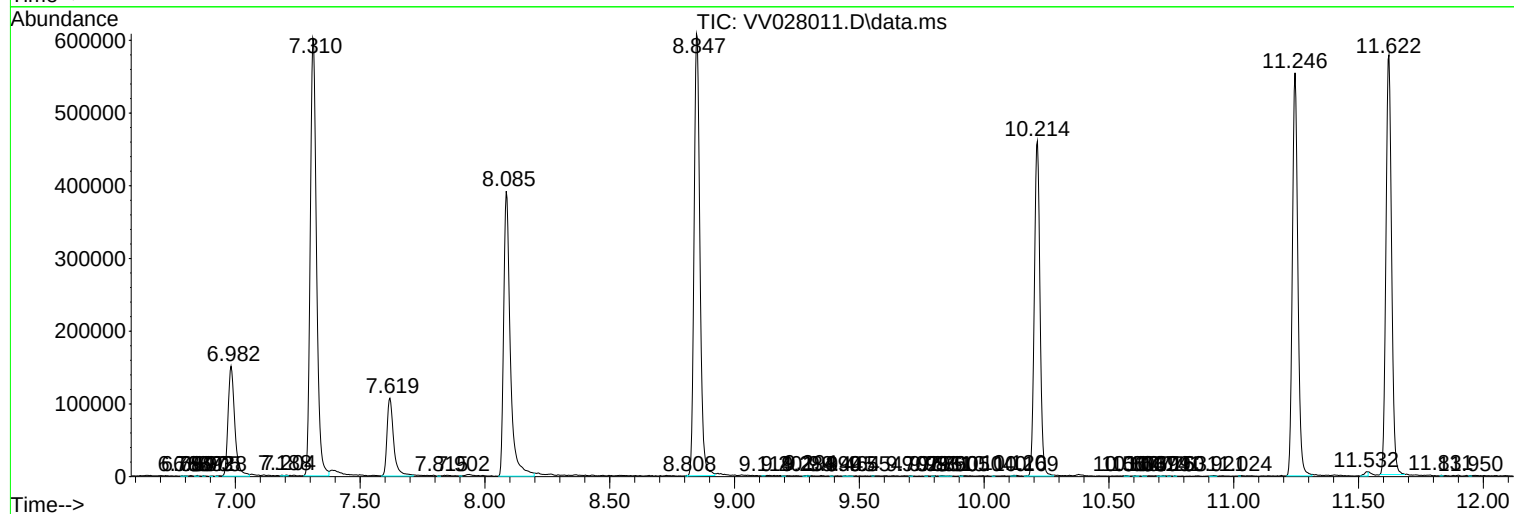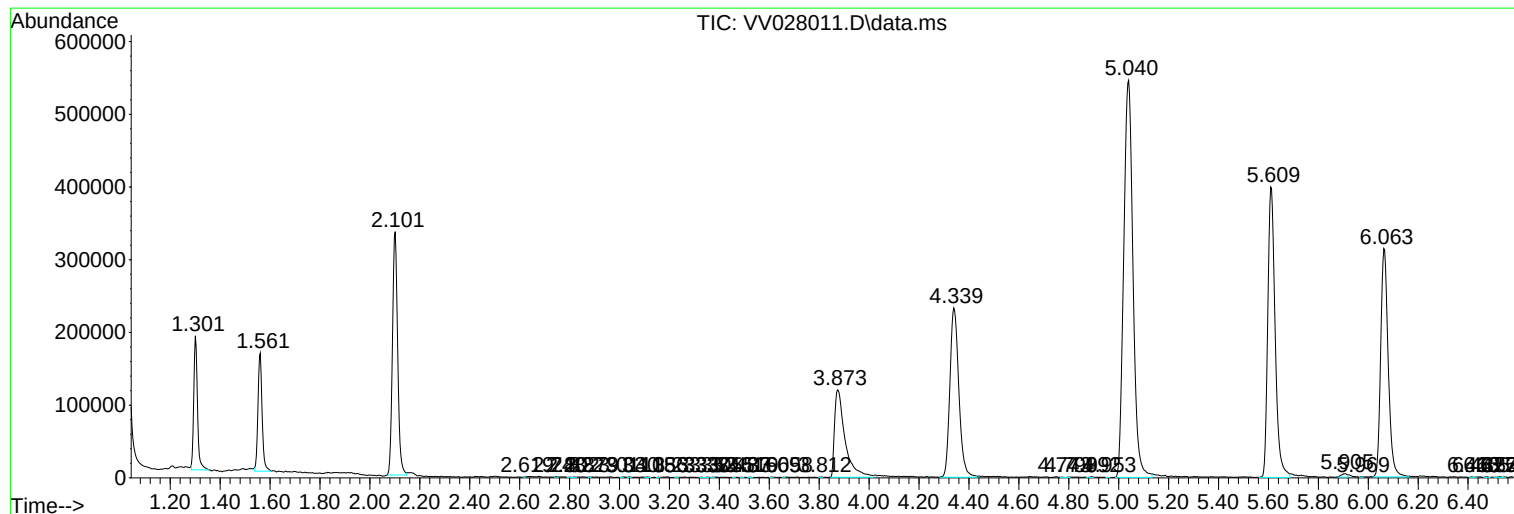

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028011.D
Acq On : 21 Sep 2022 13:02
Operator : SY/MD
Sample : N4674-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028011.D
Acq On : 21 Sep 2022 13:02
Operator : SY/MD
Sample : N4674-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
