

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028014.D
 Acq On : 21 Sep 2022 14:16
 Operator : SY/MD
 Sample : N4619-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	96	rVB	191144	198150	13.76%	1.875%
2	1.558	155	161	177	rVB	159883	187333	13.01%	1.773%
3	2.098	320	329	346	rBV	339757	492635	34.22%	4.661%
4	2.500	445	454	463	rBV9	3397	6958	0.48%	0.066%
5	2.651	499	501	504	rBV	461	294	0.02%	0.003%
6	2.889	572	575	577	rBV2	502	288	0.02%	0.003%
7	2.928	582	587	588	rBV3	642	548	0.04%	0.005%
8	2.966	596	599	602	rBV2	718	456	0.03%	0.004%
9	2.989	603	606	608	rVV	781	402	0.03%	0.004%
10	3.005	608	611	617	rVB4	812	819	0.06%	0.008%
11	3.027	617	618	620	rBV	606	239	0.02%	0.002%
12	3.063	627	629	633	rVB2	601	330	0.02%	0.003%
13	3.178	663	665	666	rBV2	486	239	0.02%	0.002%
14	3.223	677	679	683	rVB2	727	431	0.03%	0.004%
15	3.252	683	688	689	rBV2	482	368	0.03%	0.003%
16	3.297	701	702	708	rBV2	547	453	0.03%	0.004%
17	3.349	716	718	721	rBV	472	235	0.02%	0.002%
18	3.490	759	762	765	rBV2	427	317	0.02%	0.003%
19	3.574	785	788	790	rBV	537	332	0.02%	0.003%
20	3.638	807	808	812	rBV2	602	345	0.02%	0.003%
21	3.805	857	860	866	rBV2	436	445	0.03%	0.004%
22	3.873	871	881	916	rBV	135246	379792	26.38%	3.594%
23	4.243	994	996	1000	rBV3	399	248	0.02%	0.002%
24	4.339	1011	1026	1058	rVB	220370	547334	38.02%	5.179%
25	4.548	1087	1091	1094	rBV5	1160	1008	0.07%	0.010%
26	4.780	1161	1163	1166	rVB2	760	355	0.02%	0.003%
27	4.821	1173	1176	1178	rVB3	585	350	0.02%	0.003%
28	5.037	1226	1243	1274	rBV2	561793	1439671	100.00%	13.622%
29	5.400	1354	1356	1359	rBV3	556	385	0.03%	0.004%
30	5.487	1380	1383	1386	rBV4	890	550	0.04%	0.005%
31	5.609	1410	1421	1446	rBV	391184	795421	55.25%	7.526%
32	5.860	1497	1499	1502	rBV2	641	307	0.02%	0.003%
33	5.979	1534	1536	1540	rBV2	843	522	0.04%	0.005%
34	6.062	1549	1562	1590	rBV	316189	654202	45.44%	6.190%
35	6.339	1646	1648	1652	rVB3	661	472	0.03%	0.004%
36	6.358	1652	1654	1656	rBV2	521	260	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028014.D
 Acq On : 21 Sep 2022 14:16
 Operator : SY/MD
 Sample : N4619-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.381	1656	1661	1664	rBV3	421	441	0.03%	0.004%
38	6.407	1664	1669	1672	rBV4	746	562	0.04%	0.005%
39	6.423	1672	1674	1680	rBV4	857	569	0.04%	0.005%
40	6.464	1686	1687	1691	rVB3	603	299	0.02%	0.003%
41	6.538	1706	1710	1712	rBV3	512	444	0.03%	0.004%
42	6.558	1713	1716	1726	rVB6	690	1049	0.07%	0.010%
43	6.628	1736	1738	1740	rBV2	452	294	0.02%	0.003%
44	6.741	1771	1773	1776	rVB2	788	300	0.02%	0.003%
45	6.760	1776	1779	1780	rBV2	579	316	0.02%	0.003%
46	6.982	1837	1848	1872	rBV	167592	310183	21.55%	2.935%
47	7.310	1939	1950	1971	rBV	603960	1068149	74.19%	10.107%
48	7.619	2036	2046	2075	rBV	120043	216371	15.03%	2.047%
49	7.918	2137	2139	2141	rBV3	560	302	0.02%	0.003%
50	7.934	2141	2144	2147	rBV4	1280	1020	0.07%	0.010%
51	7.982	2157	2159	2163	rVB2	550	330	0.02%	0.003%
52	8.008	2163	2167	2169	rBV	720	246	0.02%	0.002%
53	8.085	2181	2191	2221	rBV	412576	739027	51.33%	6.993%
54	8.503	2319	2321	2324	rBV3	707	492	0.03%	0.005%
55	8.651	2365	2367	2370	rBV4	629	266	0.02%	0.003%
56	8.728	2389	2391	2395	rBV2	625	416	0.03%	0.004%
57	8.847	2418	2428	2448	rBV	593174	962838	66.88%	9.110%
58	9.127	2511	2515	2516	rBV3	872	719	0.05%	0.007%
59	9.262	2555	2557	2560	rBV4	476	247	0.02%	0.002%
60	9.352	2583	2585	2589	rBV2	500	250	0.02%	0.002%
61	9.377	2591	2593	2596	rBV2	607	334	0.02%	0.003%
62	9.394	2596	2598	2601	rBV3	690	309	0.02%	0.003%
63	9.484	2624	2626	2629	rVB2	877	383	0.03%	0.004%
64	9.513	2631	2635	2638	rBV	425	381	0.03%	0.004%
65	9.583	2654	2657	2658	rBV2	769	354	0.02%	0.003%
66	9.615	2665	2667	2672	rVB3	985	615	0.04%	0.006%
67	9.660	2676	2681	2685	rBV3	660	697	0.05%	0.007%
68	9.680	2685	2687	2690	rVV2	507	257	0.02%	0.002%
69	9.738	2702	2705	2707	rBV	588	420	0.03%	0.004%
70	9.831	2732	2734	2737	rVB3	537	267	0.02%	0.003%
71	9.847	2737	2739	2741	rBV2	488	272	0.02%	0.003%
72	9.876	2744	2748	2753	rBV6	908	1089	0.08%	0.010%
73	10.040	2796	2799	2800	rBV	581	269	0.02%	0.003%
74	10.072	2808	2809	2811	rBV2	740	249	0.02%	0.002%
75	10.213	2840	2853	2875	rBV	474049	748635	52.00%	7.083%
76	10.368	2897	2901	2902	rBV3	1117	666	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028014.D
 Acq On : 21 Sep 2022 14:16
 Operator : SY/MD
 Sample : N4619-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.429	2918	2920	2922	rVB2	595	236	0.02%	0.002%
78	10.500	2940	2942	2945	rBV2	459	298	0.02%	0.003%
79	10.570	2962	2964	2965	rBV2	559	267	0.02%	0.003%
80	10.670	2991	2995	2997	rBV3	920	696	0.05%	0.007%
81	10.760	3020	3023	3027	rBV5	703	584	0.04%	0.006%
82	10.905	3062	3068	3069	rBV4	1549	1239	0.09%	0.012%
83	11.017	3101	3103	3106	rBV	587	361	0.03%	0.003%
84	11.101	3127	3129	3132	rBV2	676	342	0.02%	0.003%
85	11.130	3136	3138	3141	rBV2	497	305	0.02%	0.003%
86	11.246	3161	3174	3196	rBV	552040	851548	59.15%	8.057%
87	11.622	3279	3291	3312	rBV	592516	932850	64.80%	8.826%
88	12.175	3456	3463	3468	rVB4	837	1136	0.08%	0.011%
89	12.268	3490	3492	3494	rBV3	655	249	0.02%	0.002%
90	12.528	3570	3573	3577	rBV2	532	404	0.03%	0.004%
91	12.570	3581	3586	3589	rBV2	507	571	0.04%	0.005%
92	12.641	3607	3608	3612	rBV3	431	278	0.02%	0.003%
93	12.705	3619	3628	3631	rBV4	1051	1088	0.08%	0.010%
94	13.564	3891	3895	3898	rBV2	641	618	0.04%	0.006%
95	13.737	3947	3949	3951	rBV	487	268	0.02%	0.003%
96	13.782	3961	3963	3969	rBV4	754	587	0.04%	0.006%
97	14.017	4033	4036	4039	rBV3	949	569	0.04%	0.005%
98	14.596	4213	4216	4217	rBV	944	566	0.04%	0.005%
99	14.638	4227	4229	4233	rBV5	1190	615	0.04%	0.006%
100	14.702	4247	4249	4250	rBV2	873	265	0.02%	0.003%




Sum of corrected areas: 10568761

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028014.D
Acq On : 21 Sep 2022 14:16
Operator : SY/MD
Sample : N4619-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

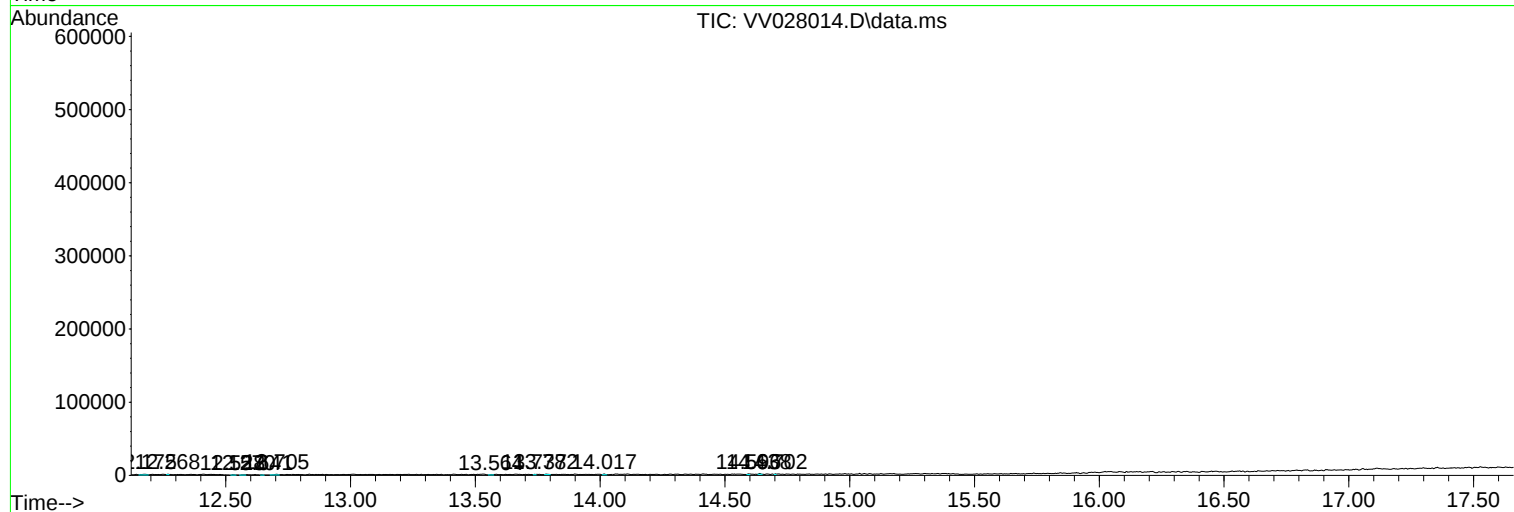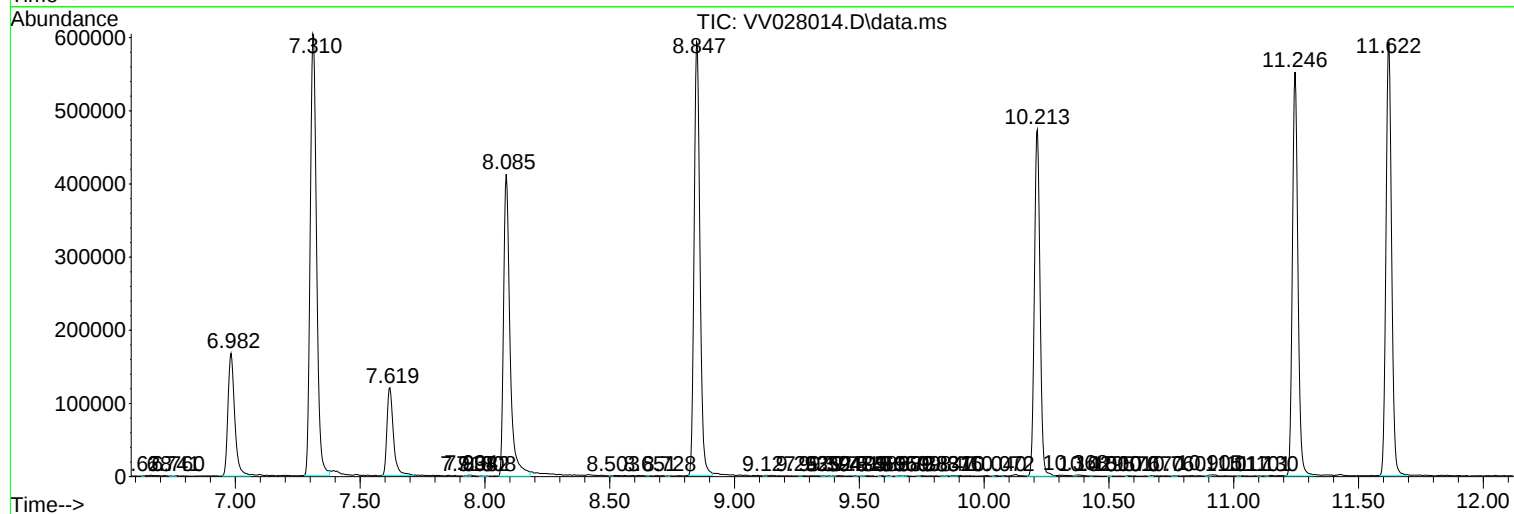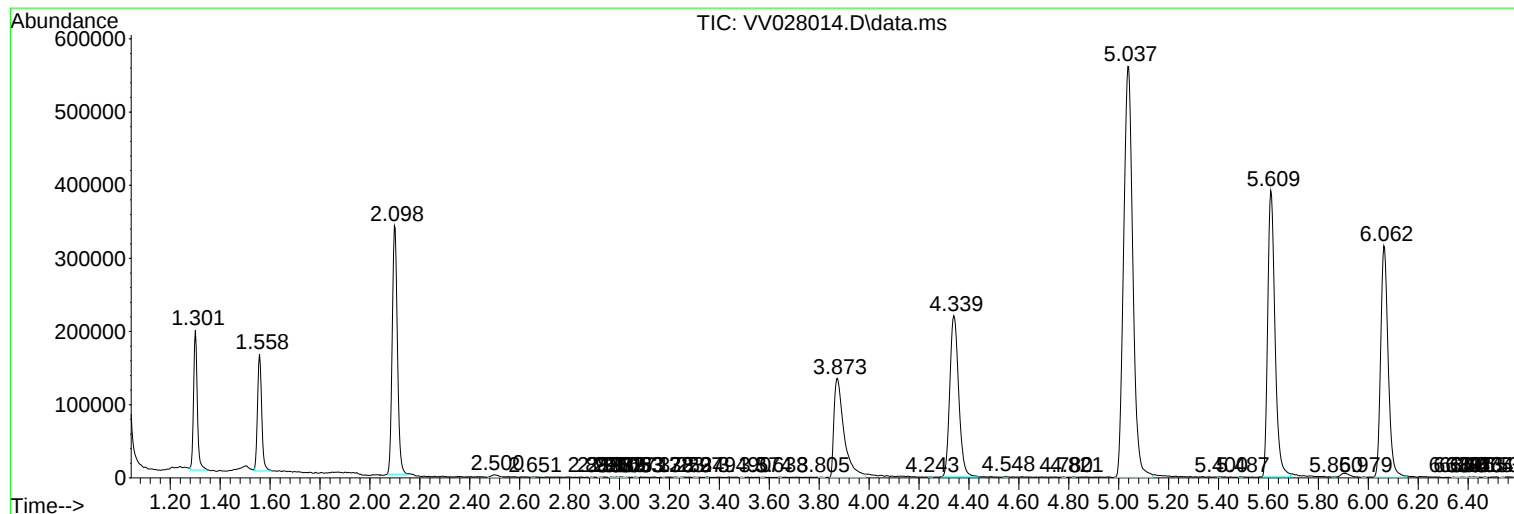

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028014.D
Acq On : 21 Sep 2022 14:16
Operator : SY/MD
Sample : N4619-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028014.D
Acq On : 21 Sep 2022 14:16
Operator : SY/MD
Sample : N4619-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc