

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028019.D
 Acq On : 21 Sep 2022 16:20
 Operator : SY/MD
 Sample : N4659-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	101	rVB	181976	194037	14.05%	1.793%
2	1.561	155	162	177	rVB	151074	172549	12.50%	1.594%
3	2.098	319	329	346	rBV	317175	455819	33.01%	4.212%
4	2.400	420	423	425	rBV3	704	496	0.04%	0.005%
5	2.484	446	449	451	rBV3	1323	770	0.06%	0.007%
6	2.638	491	497	502	rBV4	735	1043	0.08%	0.010%
7	2.725	522	524	527	rVB2	869	399	0.03%	0.004%
8	2.741	527	529	533	rBV4	803	451	0.03%	0.004%
9	2.773	535	539	542	rBV3	824	803	0.06%	0.007%
10	2.818	549	553	561	rBV5	877	968	0.07%	0.009%
11	2.915	579	583	586	rBV3	721	606	0.04%	0.006%
12	2.953	590	595	596	rBV3	1409	1191	0.09%	0.011%
13	3.108	641	643	647	rVB4	808	479	0.03%	0.004%
14	3.133	647	651	653	rBV3	564	422	0.03%	0.004%
15	3.198	668	671	676	rVB3	810	855	0.06%	0.008%
16	3.294	698	701	704	rVB5	636	460	0.03%	0.004%
17	3.442	745	747	751	rVB2	698	443	0.03%	0.004%
18	3.494	760	763	767	rVB2	635	470	0.03%	0.004%
19	3.551	779	781	788	rVB3	733	572	0.04%	0.005%
20	3.879	868	883	920	rBV2	130039	384953	27.88%	3.557%
21	4.339	1009	1026	1050	rBV	231106	565898	40.98%	5.229%
22	4.609	1105	1110	1113	rBV6	699	720	0.05%	0.007%
23	4.658	1121	1125	1130	rBV6	643	752	0.05%	0.007%
24	4.793	1163	1167	1170	rBV3	838	666	0.05%	0.006%
25	4.921	1202	1207	1211	rBV5	604	690	0.05%	0.006%
26	5.037	1224	1243	1272	rBV2	538871	1380798	100.00%	12.759%
27	5.262	1311	1313	1317	rVB4	978	471	0.03%	0.004%
28	5.285	1317	1320	1323	rBV4	749	467	0.03%	0.004%
29	5.304	1323	1326	1328	rBV4	848	564	0.04%	0.005%
30	5.362	1342	1344	1350	rBV4	541	417	0.03%	0.004%
31	5.413	1356	1360	1363	rBV5	901	617	0.04%	0.006%
32	5.494	1383	1385	1390	rVB6	1297	984	0.07%	0.009%
33	5.609	1404	1421	1445	rBV	448287	1091714	79.06%	10.088%
34	6.063	1550	1562	1592	rVB	296571	610485	44.21%	5.641%
35	6.612	1731	1733	1736	rBV4	1195	779	0.06%	0.007%
36	6.895	1818	1821	1823	rBV3	772	564	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028019.D
 Acq On : 21 Sep 2022 16:20
 Operator : SY/MD
 Sample : N4659-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.982	1837	1848	1876	rBV	167546	303073	21.95%	2.801%
38	7.310	1939	1950	1968	rBV	578670	1010465	73.18%	9.337%
39	7.619	2036	2046	2063	rBV	117320	205966	14.92%	1.903%
40	8.085	2181	2191	2222	rBV	462686	836655	60.59%	7.731%
41	8.850	2417	2429	2453	rBV	613041	1000971	72.49%	9.250%
42	9.008	2474	2478	2479	rBV3	1433	985	0.07%	0.009%
43	9.143	2511	2520	2528	rBV6	5540	9843	0.71%	0.091%
44	9.226	2540	2546	2548	rBV3	499	465	0.03%	0.004%
45	9.442	2609	2613	2617	rBV3	731	621	0.04%	0.006%
46	9.548	2638	2646	2654	rBV4	3144	5345	0.39%	0.049%
47	9.693	2686	2691	2694	rBV3	607	646	0.05%	0.006%
48	9.760	2709	2712	2716	rBV3	671	501	0.04%	0.005%
49	9.902	2752	2756	2759	rBV3	869	480	0.03%	0.004%
50	9.931	2763	2765	2767	rBV3	719	422	0.03%	0.004%
51	10.124	2816	2825	2828	rVV5	1997	2503	0.18%	0.023%
52	10.214	2841	2853	2872	rBV	471893	744558	53.92%	6.880%
53	10.304	2879	2881	2883	rBV3	866	436	0.03%	0.004%
54	10.378	2902	2904	2906	rBV3	786	440	0.03%	0.004%
55	10.426	2917	2919	2921	rBV3	778	527	0.04%	0.005%
56	10.445	2922	2925	2926	rBV2	1343	631	0.05%	0.006%
57	10.529	2948	2951	2953	rBV2	840	642	0.05%	0.006%
58	10.799	3034	3035	3039	rBV2	625	480	0.03%	0.004%
59	10.815	3039	3040	3047	rVB5	930	865	0.06%	0.008%
60	10.853	3047	3052	3054	rBV5	1035	850	0.06%	0.008%
61	10.918	3067	3072	3078	rBV9	2285	2888	0.21%	0.027%
62	11.024	3103	3105	3110	rVB5	778	649	0.05%	0.006%
63	11.082	3121	3123	3126	rBV3	674	426	0.03%	0.004%
64	11.111	3129	3132	3137	rVB4	614	593	0.04%	0.005%
65	11.133	3137	3139	3141	rBV2	954	498	0.04%	0.005%
66	11.246	3160	3174	3194	rBV	572954	883339	63.97%	8.163%
67	11.474	3242	3245	3246	rBV2	773	406	0.03%	0.004%
68	11.538	3254	3265	3271	rBV4	8521	16019	1.16%	0.148%
69	11.622	3280	3291	3311	rBV	570327	893703	64.72%	8.258%
70	11.805	3346	3348	3352	rVB3	862	433	0.03%	0.004%
71	11.953	3391	3394	3398	rVB4	1050	621	0.04%	0.006%
72	11.976	3398	3401	3404	rBV3	1058	696	0.05%	0.006%
73	12.017	3408	3414	3418	rBV6	875	1067	0.08%	0.010%
74	12.050	3422	3424	3427	rVB2	918	438	0.03%	0.004%
75	12.069	3428	3430	3434	rBV3	552	404	0.03%	0.004%
76	12.088	3434	3436	3441	rVB5	1096	789	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028019.D
 Acq On : 21 Sep 2022 16:20
 Operator : SY/MD
 Sample : N4659-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	12.233	3477	3481	3483	rBV3	1035	767	0.06%	0.007%
78	12.332	3509	3512	3514	rVV3	748	415	0.03%	0.004%
79	12.596	3589	3594	3601	rBV4	932	1147	0.08%	0.011%
80	12.657	3610	3613	3616	rBV2	829	606	0.04%	0.006%
81	12.834	3666	3668	3673	rVB2	1022	748	0.05%	0.007%
82	12.857	3673	3675	3677	rBV2	719	488	0.04%	0.005%
83	12.972	3708	3711	3713	rBV4	579	438	0.03%	0.004%
84	12.985	3713	3715	3717	rVV2	965	604	0.04%	0.006%
85	13.117	3754	3756	3761	rVB4	727	541	0.04%	0.005%
86	13.159	3767	3769	3770	rBV	966	420	0.03%	0.004%
87	13.345	3825	3827	3832	rVB3	935	635	0.05%	0.006%
88	13.390	3838	3841	3847	rVB3	595	579	0.04%	0.005%
89	13.506	3873	3877	3879	rBV4	793	581	0.04%	0.005%
90	13.831	3973	3978	3982	rVV6	727	699	0.05%	0.006%
91	13.969	4017	4021	4025	rBV3	649	714	0.05%	0.007%
92	14.030	4038	4040	4044	rBV3	746	600	0.04%	0.006%
93	14.117	4065	4067	4069	rBV2	929	462	0.03%	0.004%
94	14.165	4079	4082	4090	rVB6	827	1094	0.08%	0.010%
95	14.593	4212	4215	4218	rBV3	923	714	0.05%	0.007%
96	14.969	4328	4332	4334	rBV3	1299	938	0.07%	0.009%
97	15.188	4398	4400	4403	rVV3	868	433	0.03%	0.004%
98	15.455	4479	4483	4485	rBV3	996	758	0.05%	0.007%
99	15.821	4595	4597	4601	rBV4	1311	1022	0.07%	0.009%
100	15.863	4607	4610	4613	rBV4	905	726	0.05%	0.007%


Sum of corrected areas: 10821840

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028019.D
Acq On : 21 Sep 2022 16:20
Operator : SY/MD
Sample : N4659-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

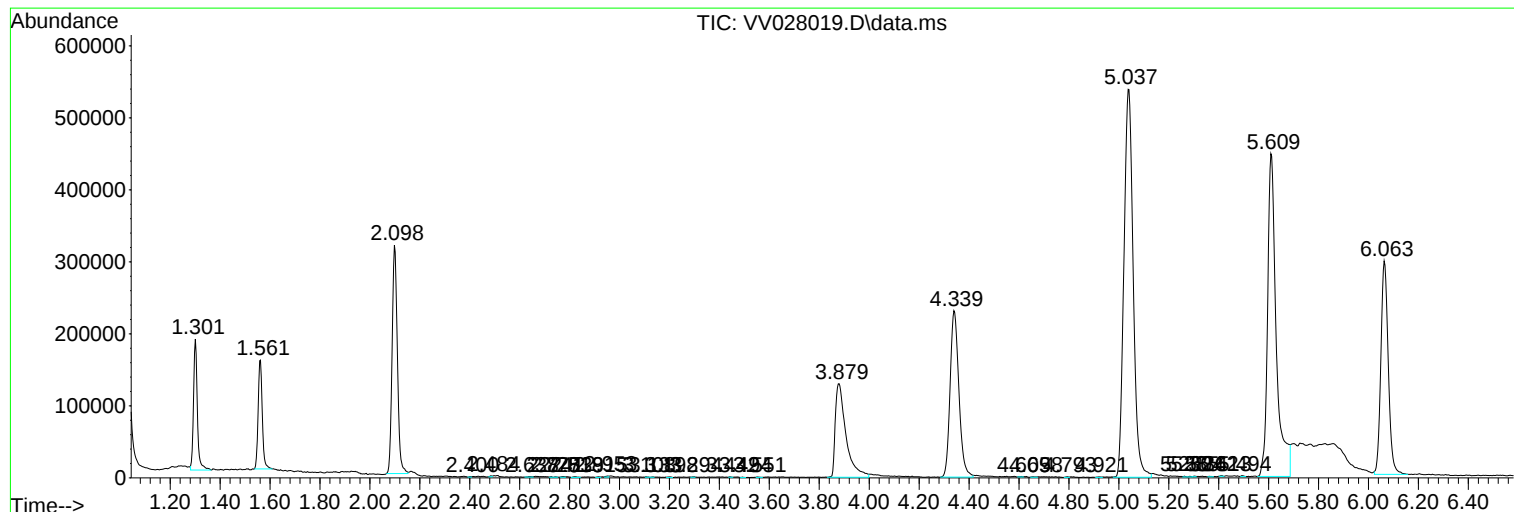

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028019.D
Acq On : 21 Sep 2022 16:20
Operator : SY/MD
Sample : N4659-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028019.D
Acq On : 21 Sep 2022 16:20
Operator : SY/MD
Sample : N4659-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------