

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028020.D
 Acq On : 21 Sep 2022 16:44
 Operator : SY/MD
 Sample : N4659-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	173241	178662	14.17%	1.802%
2	1.561	156	162	176	rVB	149437	166247	13.19%	1.676%
3	2.098	320	329	355	rVB	320739	471996	37.44%	4.759%
4	2.394	419	421	424	rBV3	564	357	0.03%	0.004%
5	2.593	480	483	488	rVB2	722	414	0.03%	0.004%
6	2.616	488	490	492	rBV2	286	129	0.01%	0.001%
7	2.635	492	496	498	rBV2	581	361	0.03%	0.004%
8	2.661	500	504	506	rBV2	790	756	0.06%	0.008%
9	2.770	535	538	540	rBV3	620	433	0.03%	0.004%
10	2.812	546	551	554	rBV3	582	500	0.04%	0.005%
11	2.828	554	556	561	rVB2	417	233	0.02%	0.002%
12	2.857	561	565	566	rBV	340	157	0.01%	0.002%
13	2.912	579	582	586	rBV3	423	218	0.02%	0.002%
14	2.957	593	596	598	rBV4	368	193	0.02%	0.002%
15	2.970	598	600	601	rVB2	276	71	0.01%	0.001%
16	3.024	614	617	618	rBV	248	101	0.01%	0.001%
17	3.069	627	631	633	rBV2	297	206	0.02%	0.002%
18	3.098	638	640	644	rBV2	377	301	0.02%	0.003%
19	3.143	651	654	658	rBV3	404	331	0.03%	0.003%
20	3.169	660	662	664	rVB	282	110	0.01%	0.001%
21	3.182	664	666	667	rBV	196	79	0.01%	0.001%
22	3.217	673	677	681	rVB2	385	229	0.02%	0.002%
23	3.243	681	685	687	rBV3	181	163	0.01%	0.002%
24	3.291	697	700	701	rBV3	291	147	0.01%	0.001%
25	3.323	707	710	711	rBV	168	93	0.01%	0.001%
26	3.355	716	720	723	rBV2	298	236	0.02%	0.002%
27	3.397	731	733	734	rBV2	168	79	0.01%	0.001%
28	3.404	734	735	736	rBV	200	64	0.01%	0.001%
29	3.442	745	747	749	rBV	142	68	0.01%	0.001%
30	3.458	749	752	753	rBV	171	93	0.01%	0.001%
31	3.474	753	757	759	rVV	278	196	0.02%	0.002%
32	3.506	765	767	773	rVB	292	193	0.02%	0.002%
33	3.532	773	775	777	rBV	232	124	0.01%	0.001%
34	3.580	787	790	795	rVB2	317	266	0.02%	0.003%
35	3.629	803	805	808	rBV2	148	99	0.01%	0.001%
36	3.645	808	810	811	rBV2	437	103	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028020.D
 Acq On : 21 Sep 2022 16:44
 Operator : SY/MD
 Sample : N4659-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	3.667	816	817	819	rVB2	258	99	0.01%	0.001%
38	3.732	835	837	840	rVB	338	161	0.01%	0.002%
39	3.760	840	846	849	rBV2	386	356	0.03%	0.004%
40	3.777	849	851	854	rVB2	237	103	0.01%	0.001%
41	3.796	854	857	859	rBV	268	162	0.01%	0.002%
42	3.841	868	871	873	rBV	247	151	0.01%	0.002%
43	3.879	873	883	919	rBV2	110293	326364	25.89%	3.291%
44	4.342	1010	1027	1054	rBV	209791	518319	41.12%	5.226%
45	4.571	1096	1098	1099	rBV2	496	182	0.01%	0.002%
46	4.613	1108	1111	1115	rBV4	623	438	0.03%	0.004%
47	4.696	1134	1137	1141	rBV3	588	482	0.04%	0.005%
48	4.741	1147	1151	1154	rBV2	502	327	0.03%	0.003%
49	4.760	1154	1157	1159	rBV	579	295	0.02%	0.003%
50	4.812	1170	1173	1175	rBV	356	166	0.01%	0.002%
51	4.822	1175	1176	1179	rVV	288	160	0.01%	0.002%
52	4.834	1179	1180	1184	rVV2	417	239	0.02%	0.002%
53	4.850	1184	1185	1189	rVB2	391	225	0.02%	0.002%
54	4.873	1189	1192	1196	rBV3	471	361	0.03%	0.004%
55	4.899	1198	1200	1202	rBV2	586	219	0.02%	0.002%
56	4.934	1209	1211	1213	rBV	336	143	0.01%	0.001%
57	4.944	1213	1214	1215	rBV	261	85	0.01%	0.001%
58	4.966	1218	1221	1223	rBV3	388	294	0.02%	0.003%
59	5.040	1226	1244	1273	rBV2	493749	1260511	100.00%	12.710%
60	5.252	1308	1310	1312	rVB3	552	205	0.02%	0.002%
61	5.336	1332	1336	1339	rBV4	744	603	0.05%	0.006%
62	5.394	1351	1354	1361	rBV5	725	591	0.05%	0.006%
63	5.429	1363	1365	1367	rBV	381	218	0.02%	0.002%
64	5.539	1395	1399	1401	rBV2	568	477	0.04%	0.005%
65	5.609	1409	1421	1442	rBV	381453	797606	63.28%	8.043%
66	6.063	1551	1562	1587	rVB	283619	573101	45.47%	5.779%
67	6.892	1818	1820	1822	rBV	408	201	0.02%	0.002%
68	6.982	1837	1848	1876	rBV	150762	278068	22.06%	2.804%
69	7.313	1939	1951	1968	rBV	536468	934333	74.12%	9.421%
70	7.619	2036	2046	2064	rBV	106709	186926	14.83%	1.885%
71	8.085	2181	2191	2226	rBV	413020	745865	59.17%	7.521%
72	8.702	2381	2383	2387	rVB3	693	377	0.03%	0.004%
73	8.728	2387	2391	2393	rBV3	485	365	0.03%	0.004%
74	8.850	2415	2429	2452	rBV	588879	966494	76.67%	9.746%
75	9.439	2607	2612	2615	rBV5	1457	1246	0.10%	0.013%
76	9.471	2621	2622	2626	rBV2	420	288	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028020.D
 Acq On : 21 Sep 2022 16:44
 Operator : SY/MD
 Sample : N4659-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.526	2637	2639	2642	rVB3	687	306	0.02%	0.003%
78	9.641	2673	2675	2676	rBV	846	387	0.03%	0.004%
79	9.741	2704	2706	2708	rBV3	886	610	0.05%	0.006%
80	9.792	2720	2722	2725	rBV2	758	389	0.03%	0.004%
81	9.995	2782	2785	2786	rBV2	486	209	0.02%	0.002%
82	10.214	2841	2853	2872	rBV	473247	742010	58.87%	7.482%
83	10.384	2900	2906	2913	rVB6	2788	3628	0.29%	0.037%
84	10.535	2951	2953	2955	rBV2	875	396	0.03%	0.004%
85	10.686	2997	3000	3004	rBV2	410	398	0.03%	0.004%
86	10.760	3021	3023	3025	rBV3	699	289	0.02%	0.003%
87	10.805	3035	3037	3040	rBV2	554	334	0.03%	0.003%
88	10.882	3057	3061	3064	rBV4	662	462	0.04%	0.005%
89	11.114	3131	3133	3135	rBV	456	177	0.01%	0.002%
90	11.133	3137	3139	3142	rVB2	1125	532	0.04%	0.005%
91	11.246	3163	3174	3196	rBV	543339	853285	67.69%	8.604%
92	11.535	3256	3264	3279	rBV8	6962	16935	1.34%	0.171%
93	11.622	3280	3291	3308	rVV	547263	872584	69.22%	8.799%
94	12.011	3408	3412	3414	rBV3	710	531	0.04%	0.005%
95	12.069	3428	3430	3433	rBV2	715	396	0.03%	0.004%
96	12.316	3504	3507	3512	rBV4	1127	849	0.07%	0.009%
97	13.178	3773	3775	3778	rBV2	447	285	0.02%	0.003%
98	13.426	3850	3852	3855	rBV	567	396	0.03%	0.004%
99	13.985	4024	4026	4028	rBV2	783	214	0.02%	0.002%
100	14.123	4067	4069	4075	rBV5	889	779	0.06%	0.008%




Sum of corrected areas: 9917195

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028020.D
Acq On : 21 Sep 2022 16:44
Operator : SY/MD
Sample : N4659-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

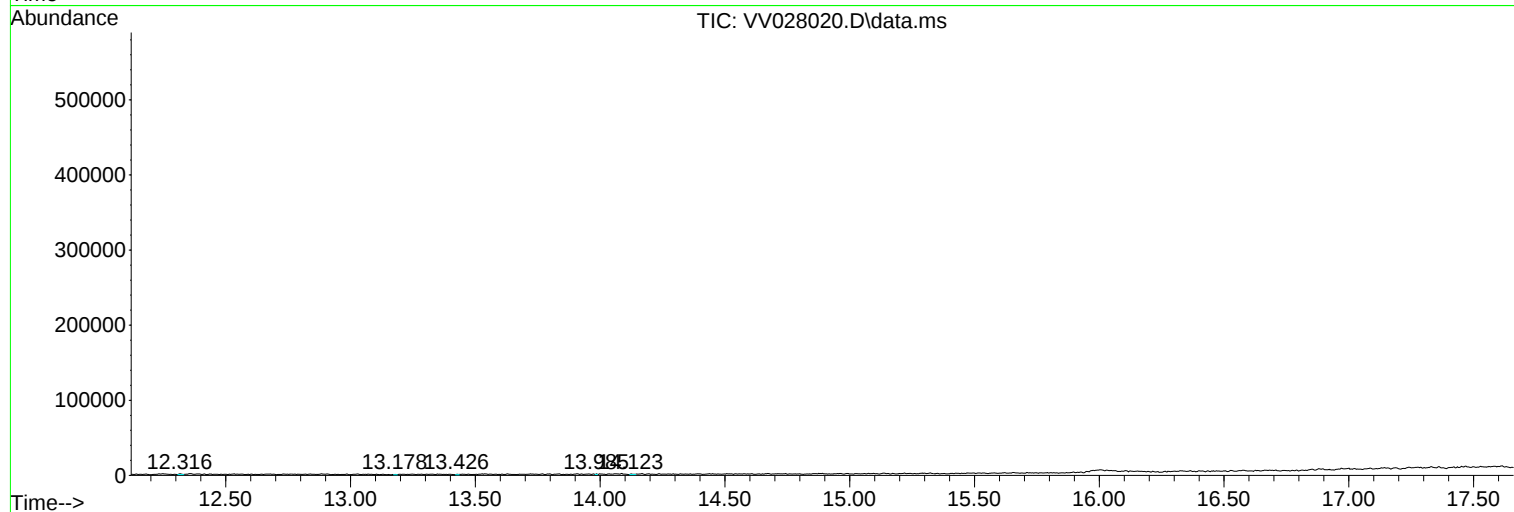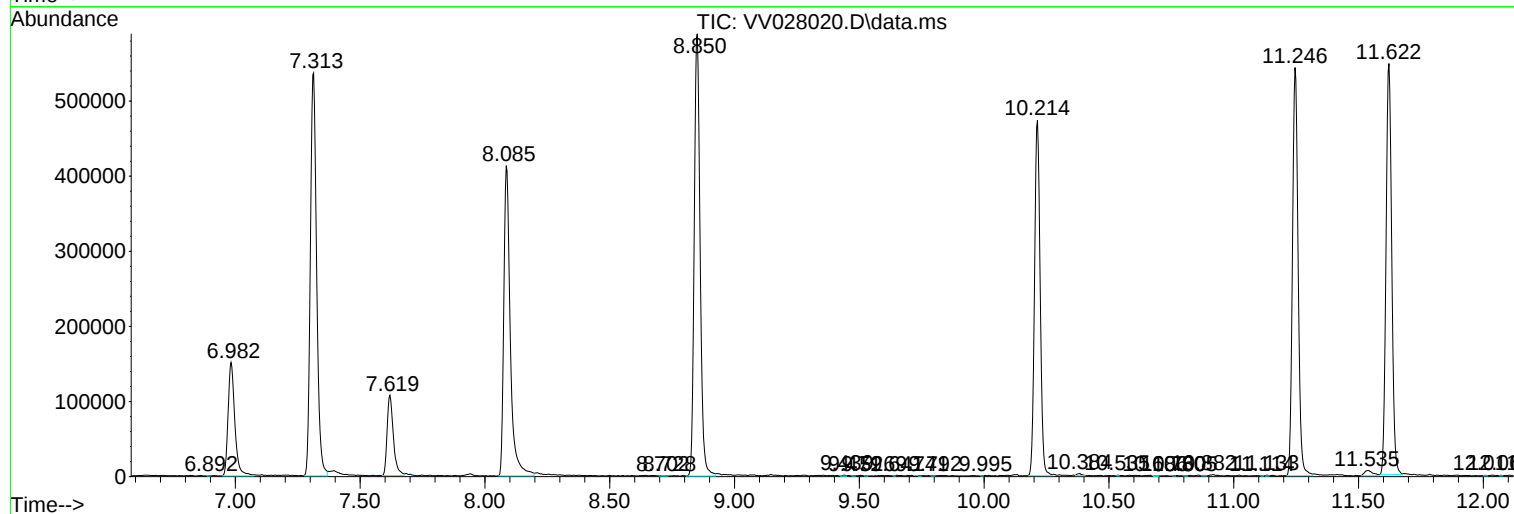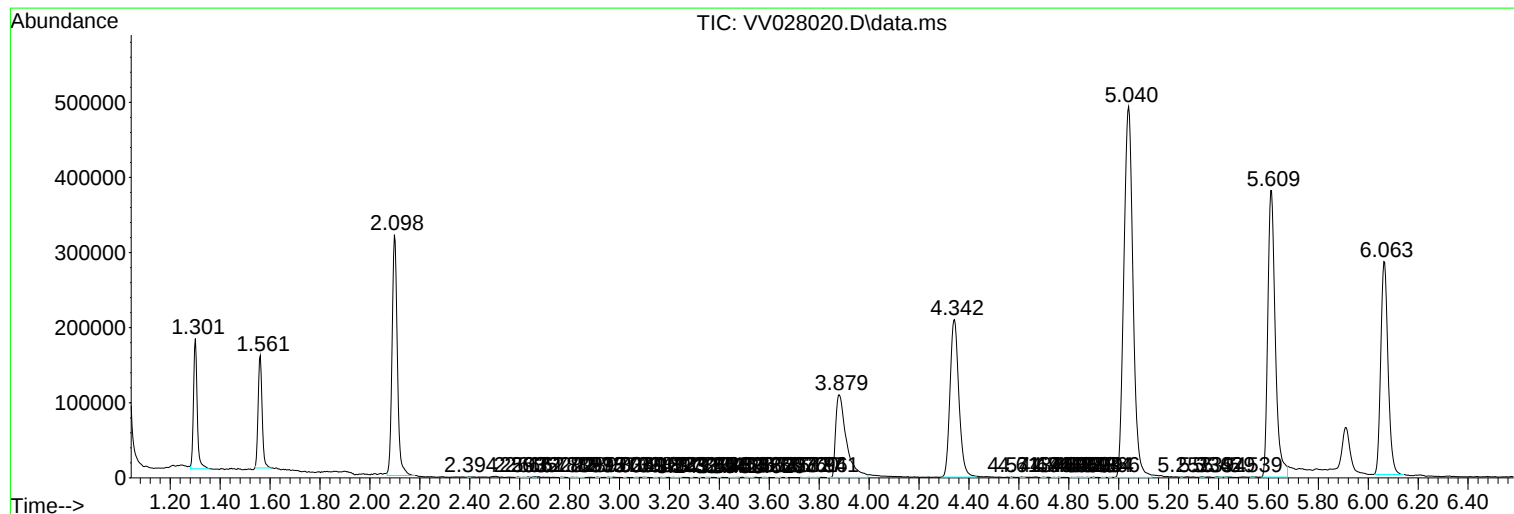

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028020.D
Acq On : 21 Sep 2022 16:44
Operator : SY/MD
Sample : N4659-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028020.D
Acq On : 21 Sep 2022 16:44
Operator : SY/MD
Sample : N4659-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc