

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028022.D
 Acq On : 21 Sep 2022 17:59
 Operator : SY/MD
 Sample : N4677-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV028022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	95	rVB	163546	163622	12.78%	1.678%
2	1.558	154	161	174	rVB	132577	153877	12.02%	1.578%
3	2.098	320	329	344	rBV	293342	425424	33.22%	4.363%
4	2.593	481	483	485	rBV2	414	209	0.02%	0.002%
5	2.683	508	511	514	rVB3	739	400	0.03%	0.004%
6	2.757	530	534	541	rVV5	1386	1502	0.12%	0.015%
7	2.950	586	594	596	rBV5	2478	3250	0.25%	0.033%
8	3.015	612	614	618	rVB4	660	485	0.04%	0.005%
9	3.043	618	623	624	rBV2	809	625	0.05%	0.006%
10	3.098	638	640	643	rBV	468	330	0.03%	0.003%
11	3.288	697	699	702	rVB2	442	233	0.02%	0.002%
12	3.307	702	705	708	rBV3	520	328	0.03%	0.003%
13	3.404	733	735	738	rBV	722	429	0.03%	0.004%
14	3.481	757	759	761	rBV	543	306	0.02%	0.003%
15	3.568	783	786	788	rVB3	790	319	0.02%	0.003%
16	3.584	788	791	793	rBV3	547	314	0.02%	0.003%
17	3.654	809	813	814	rBV3	720	446	0.03%	0.005%
18	3.709	826	830	832	rVV3	873	565	0.04%	0.006%
19	3.735	835	838	843	rBV2	729	624	0.05%	0.006%
20	3.870	870	880	920	rBV	119891	332747	25.98%	3.413%
21	4.278	1005	1007	1010	rBV3	430	306	0.02%	0.003%
22	4.339	1010	1026	1053	rVV	203583	512872	40.05%	5.260%
23	4.751	1151	1154	1157	rBV4	669	449	0.04%	0.005%
24	4.777	1160	1162	1165	rVV4	420	239	0.02%	0.002%
25	4.879	1191	1194	1196	rVB2	652	323	0.03%	0.003%
26	4.899	1196	1200	1202	rBV2	609	419	0.03%	0.004%
27	4.947	1213	1215	1219	rVB2	468	290	0.02%	0.003%
28	5.037	1226	1243	1270	rBV2	496935	1280702	100.00%	13.135%
29	5.423	1361	1363	1367	rVB2	920	461	0.04%	0.005%
30	5.442	1367	1369	1370	rBV	502	220	0.02%	0.002%
31	5.500	1386	1387	1392	rVB4	701	467	0.04%	0.005%
32	5.532	1395	1397	1398	rBV	635	287	0.02%	0.003%
33	5.564	1404	1407	1409	rBV3	765	398	0.03%	0.004%
34	5.609	1409	1421	1443	rBV	390992	787408	61.48%	8.076%
35	6.063	1551	1562	1589	rVB	291980	593606	46.35%	6.088%
36	6.407	1667	1669	1671	rBV2	740	361	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028022.D
 Acq On : 21 Sep 2022 17:59
 Operator : SY/MD
 Sample : N4677-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.622	1734	1736	1739	rBV3	1107	647	0.05%	0.007%
38	6.982	1838	1848	1873	rBV	150922	276191	21.57%	2.833%
39	7.310	1939	1950	1971	rBV	529130	924484	72.19%	9.482%
40	7.619	2036	2046	2072	rBV	109655	194771	15.21%	1.998%
41	8.085	2179	2191	2215	rBV	431407	749703	58.54%	7.689%
42	8.616	2353	2356	2357	rBV3	632	355	0.03%	0.004%
43	8.686	2376	2378	2380	rVB3	588	244	0.02%	0.003%
44	8.715	2385	2387	2389	rVV3	452	208	0.02%	0.002%
45	8.738	2392	2394	2398	rVB3	675	331	0.03%	0.003%
46	8.767	2398	2403	2405	rBV3	666	504	0.04%	0.005%
47	8.783	2405	2408	2411	rBV2	690	563	0.04%	0.006%
48	8.850	2417	2429	2461	rBV	562233	933223	72.87%	9.571%
49	9.085	2500	2502	2505	rBV4	742	312	0.02%	0.003%
50	9.230	2545	2547	2549	rBV3	520	209	0.02%	0.002%
51	9.284	2561	2564	2565	rBV2	602	306	0.02%	0.003%
52	9.352	2583	2585	2591	rVB5	407	270	0.02%	0.003%
53	9.429	2606	2609	2610	rBV2	566	271	0.02%	0.003%
54	9.497	2627	2630	2632	rBV3	670	443	0.03%	0.005%
55	9.574	2651	2654	2656	rBV3	719	539	0.04%	0.006%
56	9.834	2731	2735	2738	rBV3	636	539	0.04%	0.006%
57	9.850	2738	2740	2741	rBV	461	204	0.02%	0.002%
58	9.873	2745	2747	2752	rVB3	932	645	0.05%	0.007%
59	9.895	2752	2754	2758	rBV2	577	443	0.03%	0.005%
60	9.992	2782	2784	2787	rVB3	652	246	0.02%	0.003%
61	10.050	2796	2802	2807	rBV4	961	1122	0.09%	0.012%
62	10.091	2813	2815	2816	rBV2	573	213	0.02%	0.002%
63	10.214	2839	2853	2871	rBV	443521	701152	54.75%	7.191%
64	10.352	2893	2896	2897	rBV3	657	421	0.03%	0.004%
65	10.493	2935	2940	2942	rBV5	674	607	0.05%	0.006%
66	10.513	2942	2946	2948	rBV4	800	710	0.06%	0.007%
67	10.567	2960	2963	2964	rBV3	1104	533	0.04%	0.005%
68	10.699	3003	3004	3008	rVB3	1097	550	0.04%	0.006%
69	10.722	3008	3011	3015	rBV2	1147	962	0.08%	0.010%
70	10.757	3020	3022	3026	rVB2	611	308	0.02%	0.003%
71	10.789	3030	3032	3034	rBV	450	294	0.02%	0.003%
72	10.898	3063	3066	3067	rBV	1069	523	0.04%	0.005%
73	11.107	3127	3131	3132	rBV3	417	306	0.02%	0.003%
74	11.143	3138	3142	3146	rBV4	536	607	0.05%	0.006%
75	11.191	3150	3157	3161	rBV4	1102	1245	0.10%	0.013%
76	11.246	3163	3174	3199	rBV	538103	822266	64.20%	8.433%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028022.D
 Acq On : 21 Sep 2022 17:59
 Operator : SY/MD
 Sample : N4677-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.490	3246	3250	3251	rBV2	591	330	0.03%	0.003%
78	11.622	3280	3291	3309	rBV	542948	854072	66.69%	8.759%
79	12.017	3408	3414	3421	rBV7	1125	1811	0.14%	0.019%
80	12.053	3421	3425	3426	rBV2	620	502	0.04%	0.005%
81	12.088	3433	3436	3438	rBV4	653	464	0.04%	0.005%
82	12.172	3460	3462	3465	rBV2	515	223	0.02%	0.002%
83	12.300	3498	3502	3505	rBV3	1027	703	0.05%	0.007%
84	12.416	3535	3538	3544	rBV4	952	1050	0.08%	0.011%
85	12.493	3559	3562	3564	rBV2	883	457	0.04%	0.005%
86	12.699	3624	3626	3628	rBV3	1022	572	0.04%	0.006%
87	12.844	3667	3671	3673	rBV3	616	523	0.04%	0.005%
88	12.869	3677	3679	3681	rBV2	664	423	0.03%	0.004%
89	12.937	3698	3700	3703	rBV5	878	637	0.05%	0.007%
90	13.091	3746	3748	3751	rBV3	661	504	0.04%	0.005%
91	13.143	3761	3764	3765	rBV2	491	328	0.03%	0.003%
92	13.175	3770	3774	3780	rBV4	977	1162	0.09%	0.012%
93	13.451	3859	3860	3863	rVB	730	364	0.03%	0.004%
94	13.773	3958	3960	3963	rBV3	1017	409	0.03%	0.004%
95	13.866	3987	3989	3992	rVB2	799	318	0.02%	0.003%
96	13.940	4010	4012	4014	rBV2	506	346	0.03%	0.004%
97	14.017	4031	4036	4037	rBV3	993	823	0.06%	0.008%
98	14.066	4047	4051	4054	rBV2	774	625	0.05%	0.006%
99	14.455	4170	4172	4175	rBV2	771	429	0.03%	0.004%
100	14.599	4214	4217	4221	rBV3	1237	944	0.07%	0.010%




Sum of corrected areas: 9750332

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028022.D
Acq On : 21 Sep 2022 17:59
Operator : SY/MD
Sample : N4677-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

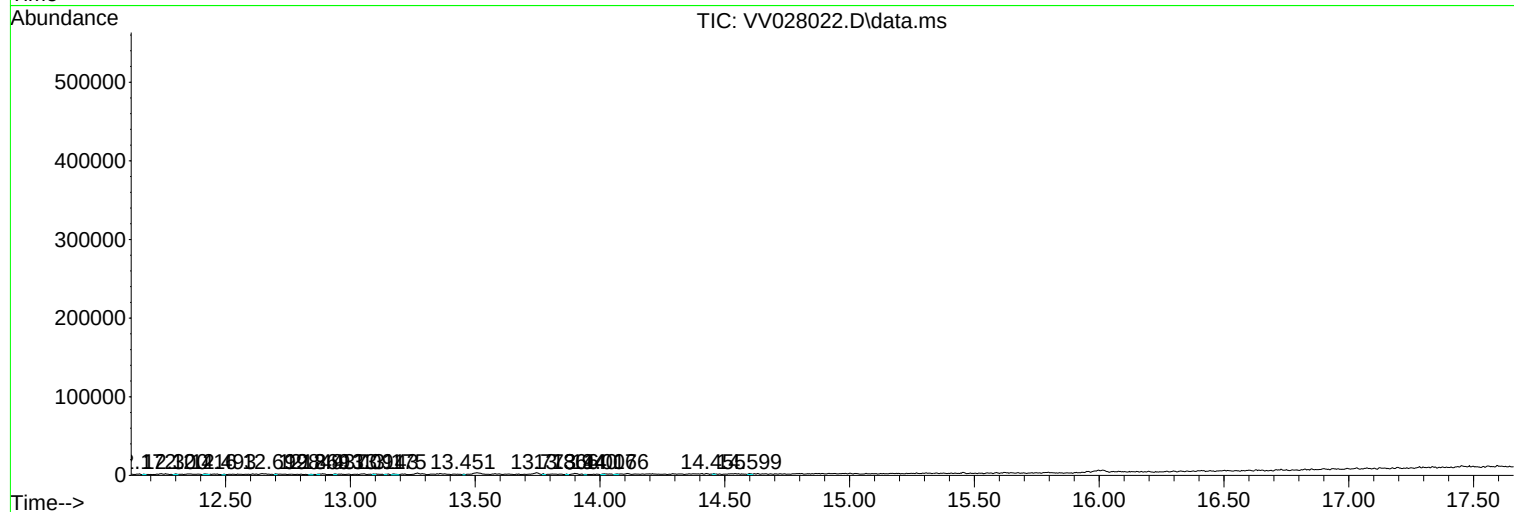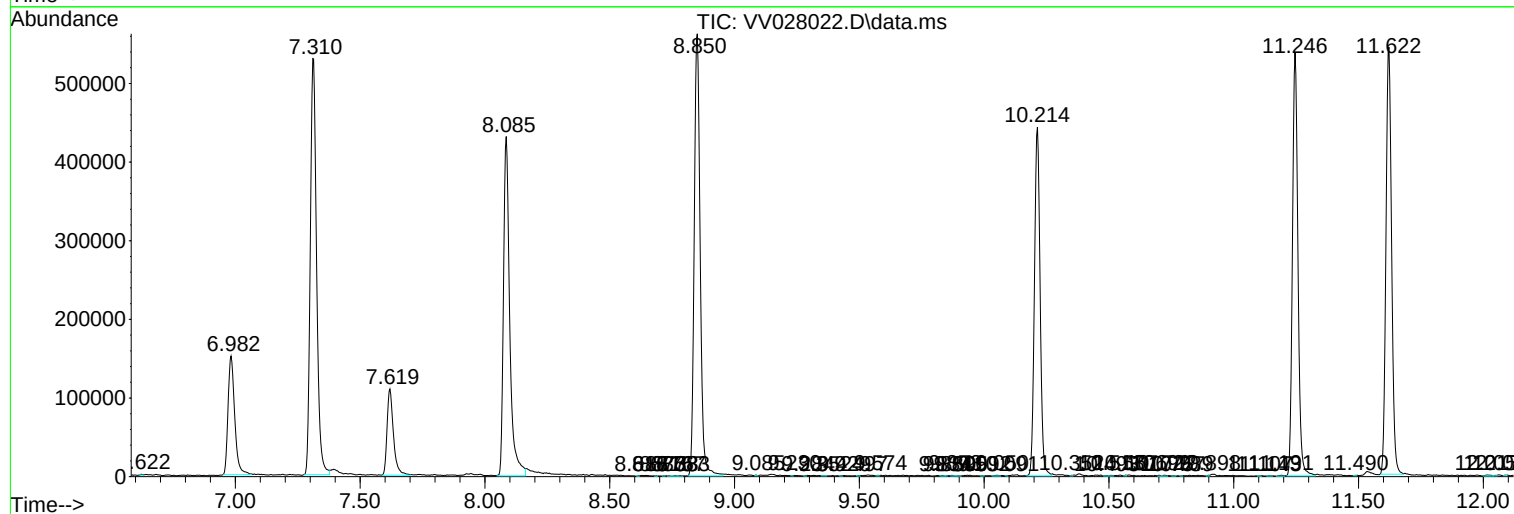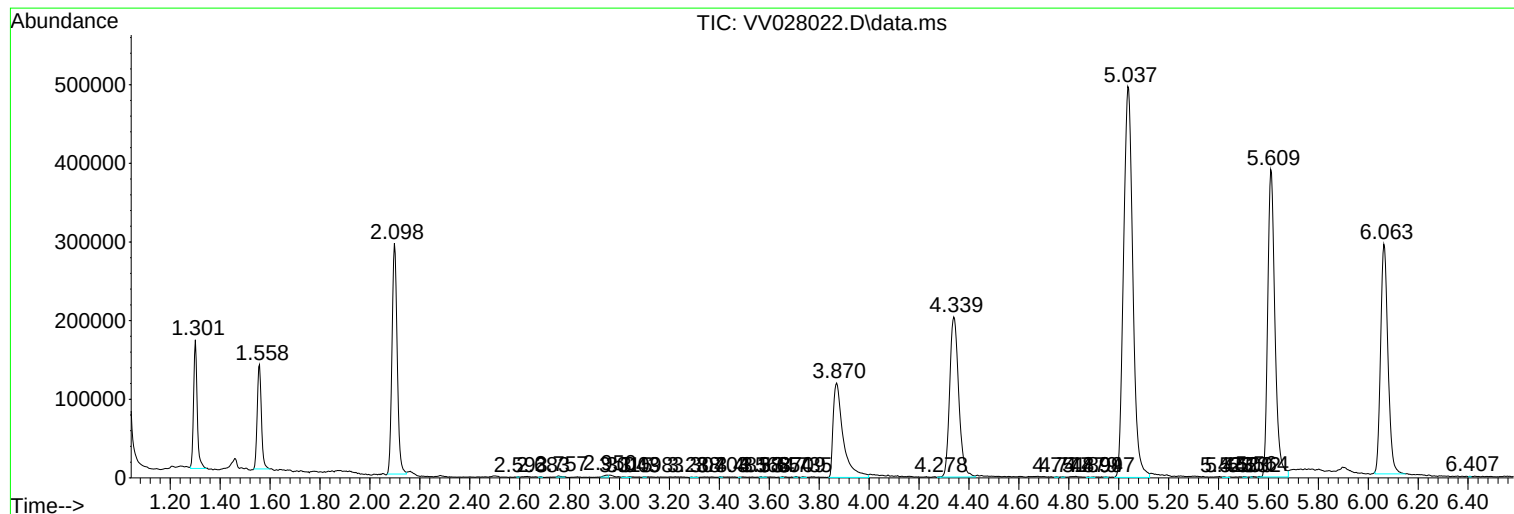

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028022.D
Acq On : 21 Sep 2022 17:59
Operator : SY/MD
Sample : N4677-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028022.D
Acq On : 21 Sep 2022 17:59
Operator : SY/MD
Sample : N4677-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc