

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028024.D
 Acq On : 21 Sep 2022 18:49
 Operator : SY/MD
 Sample : N4677-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	95	rVB	162331	160716	13.22%	1.491%
2	1.558	155	161	175	rVB	142360	159540	13.13%	1.480%
3	2.098	320	329	363	rVB2	312165	496941	40.89%	4.611%
4	2.535	464	465	468	rBV3	734	416	0.03%	0.004%
5	2.879	565	572	575	rBV3	649	824	0.07%	0.008%
6	3.153	654	657	658	rBV2	391	244	0.02%	0.002%
7	3.272	692	694	695	rBV2	382	166	0.01%	0.002%
8	3.297	700	702	705	rVB2	343	183	0.02%	0.002%
9	3.339	713	715	716	rBV2	301	109	0.01%	0.001%
10	3.410	734	737	740	rBV	383	235	0.02%	0.002%
11	3.436	743	745	748	rBV	383	136	0.01%	0.001%
12	3.449	748	749	752	rBV2	424	235	0.02%	0.002%
13	3.474	753	757	758	rVB	401	212	0.02%	0.002%
14	3.519	769	771	772	rBV2	428	156	0.01%	0.001%
15	3.548	778	780	785	rVB2	353	264	0.02%	0.002%
16	3.584	789	791	793	rBV2	205	94	0.01%	0.001%
17	3.651	808	812	813	rBV	428	278	0.02%	0.003%
18	3.683	820	822	826	rVB3	645	490	0.04%	0.005%
19	3.776	850	851	853	rBV	360	112	0.01%	0.001%
20	3.879	872	883	919	rBV	129666	416020	34.23%	3.860%
21	4.339	1013	1026	1046	rBV	195672	480448	39.53%	4.458%
22	4.603	1095	1108	1125	rBV4	7706	19289	1.59%	0.179%
23	4.702	1135	1139	1142	rBV4	632	431	0.04%	0.004%
24	4.748	1151	1153	1156	rBV	467	228	0.02%	0.002%
25	4.809	1170	1172	1173	rVB2	462	134	0.01%	0.001%
26	4.838	1178	1181	1185	rBV2	317	234	0.02%	0.002%
27	4.857	1185	1187	1191	rVB2	198	110	0.01%	0.001%
28	4.892	1196	1198	1199	rBV	305	151	0.01%	0.001%
29	4.899	1199	1200	1205	rBV2	373	221	0.02%	0.002%
30	4.944	1209	1214	1216	rBV	376	237	0.02%	0.002%
31	4.960	1216	1219	1222	rVB2	470	271	0.02%	0.003%
32	4.982	1222	1226	1227	rBV	267	168	0.01%	0.002%
33	5.037	1227	1243	1272	rBV2	473122	1215265	100.00%	11.276%
34	5.378	1347	1349	1350	rBV	659	262	0.02%	0.002%
35	5.391	1350	1353	1356	rVV3	610	411	0.03%	0.004%
36	5.436	1365	1367	1370	rBV2	363	205	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028024.D
 Acq On : 21 Sep 2022 18:49
 Operator : SY/MD
 Sample : N4677-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.532	1394	1397	1398	rBV2	648	364	0.03%	0.003%
38	5.609	1410	1421	1442	rBV	384272	778597	64.07%	7.225%
39	5.908	1501	1514	1544	rBV	509518	1009700	83.08%	9.369%
40	6.063	1551	1562	1592	rVB	286501	587220	48.32%	5.449%
41	6.538	1708	1710	1714	rBV2	418	261	0.02%	0.002%
42	6.651	1743	1745	1751	rVB5	1021	772	0.06%	0.007%
43	6.764	1776	1780	1784	rBV3	1083	1112	0.09%	0.010%
44	6.982	1837	1848	1868	rBV	148074	271261	22.32%	2.517%
45	7.313	1939	1951	1971	rBV	518090	914053	75.21%	8.482%
46	7.619	2036	2046	2063	rBV	106491	187378	15.42%	1.739%
47	7.741	2083	2084	2086	rBV2	654	251	0.02%	0.002%
48	7.921	2137	2140	2141	rBV2	1402	774	0.06%	0.007%
49	7.979	2155	2158	2160	rBV3	963	693	0.06%	0.006%
50	8.085	2181	2191	2224	rBV	413554	770810	63.43%	7.152%
51	8.362	2273	2277	2280	rBV4	964	895	0.07%	0.008%
52	8.612	2352	2355	2357	rBV	651	355	0.03%	0.003%
53	8.673	2372	2374	2375	rBV	325	128	0.01%	0.001%
54	8.699	2379	2382	2385	rBV2	517	349	0.03%	0.003%
55	8.731	2390	2392	2395	rBV2	581	355	0.03%	0.003%
56	8.847	2417	2428	2451	rBV	578381	951789	78.32%	8.832%
57	9.101	2506	2507	2510	rBV	584	306	0.03%	0.003%
58	9.194	2534	2536	2537	rBV	850	420	0.03%	0.004%
59	9.233	2546	2548	2549	rBV	570	168	0.01%	0.002%
60	9.355	2584	2586	2590	rBV	448	383	0.03%	0.004%
61	9.406	2600	2602	2608	rVB5	658	381	0.03%	0.004%
62	9.847	2737	2739	2743	rBV3	467	366	0.03%	0.003%
63	9.889	2747	2752	2755	rBV5	914	817	0.07%	0.008%
64	9.976	2777	2779	2783	rVB	698	425	0.03%	0.004%
65	10.159	2833	2836	2838	rBV2	422	300	0.02%	0.003%
66	10.214	2841	2853	2866	rBV	416387	650316	53.51%	6.034%
67	10.355	2894	2897	2898	rBV	458	253	0.02%	0.002%
68	10.432	2920	2921	2925	rVB	365	156	0.01%	0.001%
69	10.451	2925	2927	2928	rBV	428	152	0.01%	0.001%
70	10.513	2942	2946	2947	rBV2	386	222	0.02%	0.002%
71	10.541	2953	2955	2957	rBV	375	87	0.01%	0.001%
72	10.632	2981	2983	2985	rBV	495	225	0.02%	0.002%
73	10.712	3006	3008	3011	rVB2	334	184	0.02%	0.002%
74	10.728	3011	3013	3014	rBV2	212	87	0.01%	0.001%
75	10.760	3019	3023	3024	rBV2	369	220	0.02%	0.002%
76	10.792	3030	3033	3034	rBV2	271	111	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028024.D
 Acq On : 21 Sep 2022 18:49
 Operator : SY/MD
 Sample : N4677-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E86

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.802	3034	3036	3043	rVB3	486	329	0.03%	0.003%
78	10.831	3043	3045	3048	rVB	411	198	0.02%	0.002%
79	10.853	3048	3052	3053	rBV2	635	477	0.04%	0.004%
80	10.985	3091	3093	3094	rBV	305	125	0.01%	0.001%
81	11.069	3117	3119	3121	rBV4	651	417	0.03%	0.004%
82	11.246	3163	3174	3200	rBV	540484	827859	68.12%	7.682%
83	11.535	3258	3264	3277	rBV4	6857	12507	1.03%	0.116%
84	11.622	3280	3291	3316	rVB	535824	838765	69.02%	7.783%
85	11.895	3373	3376	3378	rBV2	728	402	0.03%	0.004%
86	11.988	3399	3405	3408	rBV3	886	895	0.07%	0.008%
87	12.091	3433	3437	3441	rBV6	805	740	0.06%	0.007%
88	12.194	3468	3469	3471	rBV	447	249	0.02%	0.002%
89	12.226	3477	3479	3481	rBV	486	258	0.02%	0.002%
90	12.281	3494	3496	3501	rBV3	789	535	0.04%	0.005%
91	12.310	3502	3505	3507	rBV3	871	418	0.03%	0.004%
92	12.506	3564	3566	3568	rVB3	635	250	0.02%	0.002%
93	12.699	3622	3626	3631	rBV4	596	825	0.07%	0.008%
94	12.911	3689	3692	3695	rBV3	601	460	0.04%	0.004%
95	13.046	3729	3734	3736	rBV3	682	686	0.06%	0.006%
96	13.316	3815	3818	3819	rBV2	529	334	0.03%	0.003%
97	13.840	3979	3981	3985	rBV2	874	730	0.06%	0.007%
98	14.284	4117	4119	4121	rBV	595	327	0.03%	0.003%
99	14.487	4179	4182	4188	rBV5	662	591	0.05%	0.005%
100	15.065	4360	4362	4365	rVB4	1063	468	0.04%	0.004%




Sum of corrected areas: 10776977

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028024.D
Acq On : 21 Sep 2022 18:49
Operator : SY/MD
Sample : N4677-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

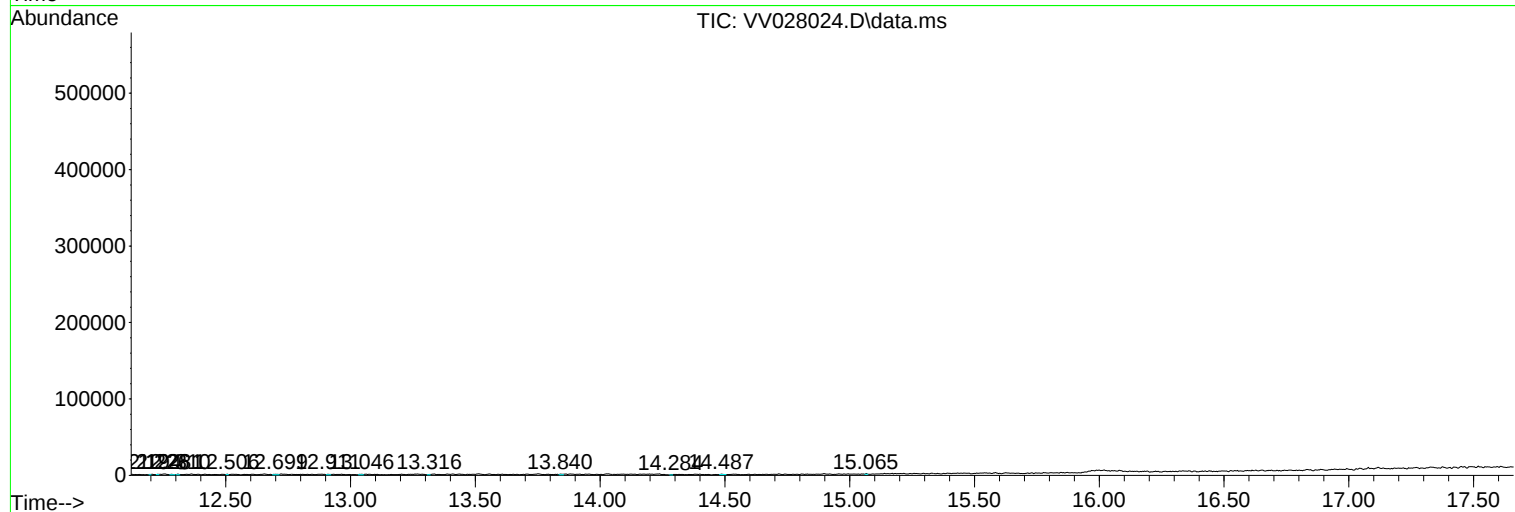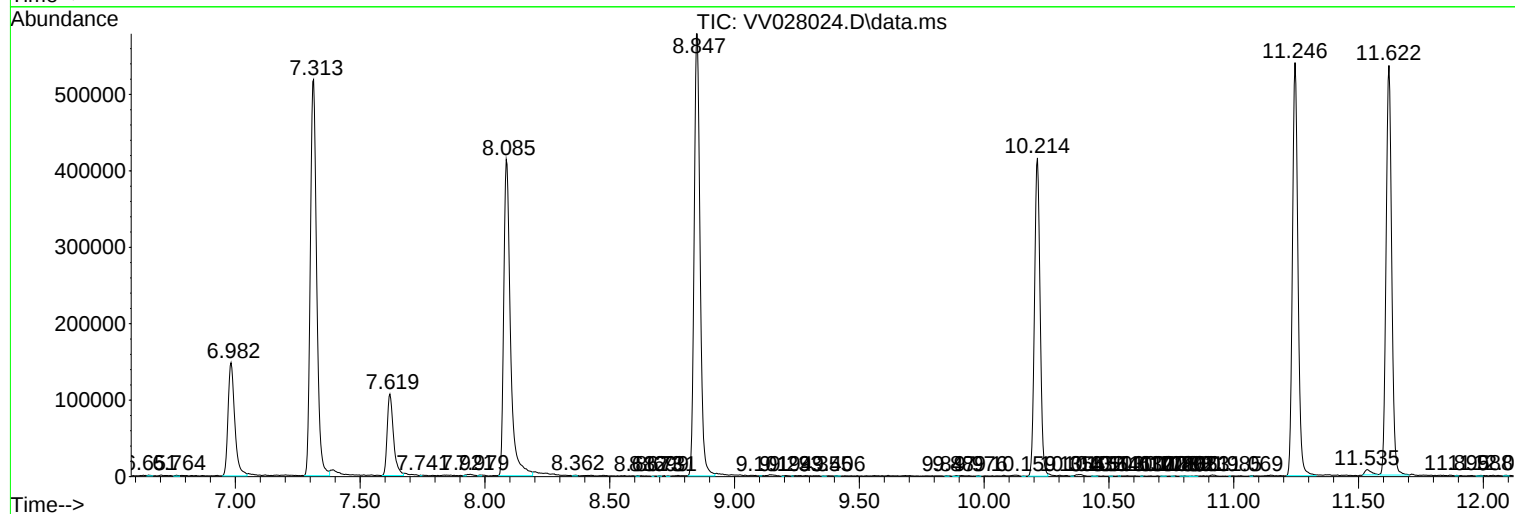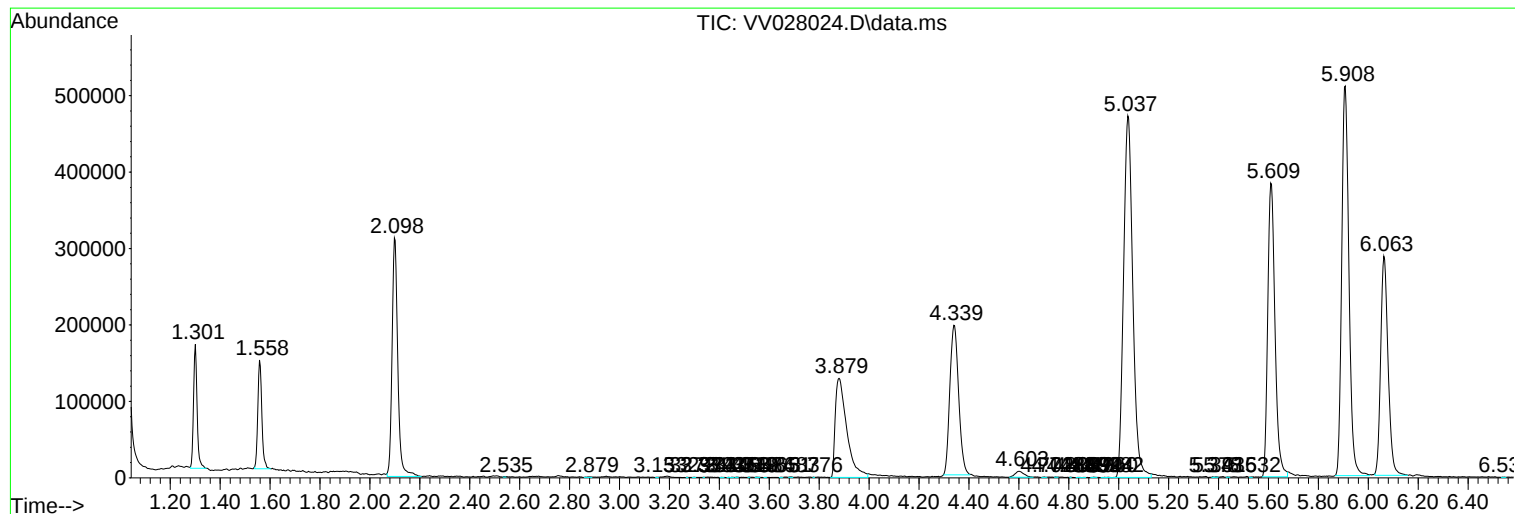

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028024.D
Acq On : 21 Sep 2022 18:49
Operator : SY/MD
Sample : N4677-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028024.D
Acq On : 21 Sep 2022 18:49
Operator : SY/MD
Sample : N4677-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc