

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028025.D
 Acq On : 21 Sep 2022 19:14
 Operator : SY/MD
 Sample : N4677-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028025.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	93	rVB	155407	156390	12.35%	1.642%
2	1.558	155	161	171	rVB	135334	152128	12.01%	1.597%
3	2.098	320	329	343	rBV	293914	414745	32.75%	4.353%
4	2.738	524	528	530	rBV3	767	629	0.05%	0.007%
5	2.757	530	534	542	rVV8	828	1134	0.09%	0.012%
6	2.838	556	559	561	rBV3	546	325	0.03%	0.003%
7	2.915	580	583	585	rBV2	388	259	0.02%	0.003%
8	2.928	585	587	589	rBV2	581	313	0.02%	0.003%
9	2.992	605	607	610	rBV2	469	337	0.03%	0.004%
10	3.027	615	618	620	rBV2	576	434	0.03%	0.005%
11	3.069	628	631	635	rBV2	729	515	0.04%	0.005%
12	3.375	724	726	737	rVB4	1004	1085	0.09%	0.011%
13	3.420	737	740	743	rBV3	1019	780	0.06%	0.008%
14	3.596	792	795	797	rBV2	578	323	0.03%	0.003%
15	3.638	806	808	812	rVB2	526	347	0.03%	0.004%
16	3.667	812	817	818	rBV2	399	381	0.03%	0.004%
17	3.764	842	847	848	rBV2	351	224	0.02%	0.002%
18	3.873	872	881	924	rBV	117881	334493	26.41%	3.511%
19	4.339	1007	1026	1054	rBV	206664	522897	41.29%	5.489%
20	4.596	1099	1106	1109	rBV4	1807	2359	0.19%	0.025%
21	4.725	1143	1146	1149	rBV4	444	367	0.03%	0.004%
22	4.940	1210	1213	1214	rVV	686	311	0.02%	0.003%
23	4.960	1217	1219	1223	rVV3	525	342	0.03%	0.004%
24	5.037	1228	1243	1272	rBV2	492218	1266473	100.00%	13.294%
25	5.423	1361	1363	1369	rVV5	539	479	0.04%	0.005%
26	5.452	1369	1372	1377	rVB2	270	249	0.02%	0.003%
27	5.535	1396	1398	1400	rBV3	466	245	0.02%	0.003%
28	5.609	1409	1421	1449	rBV	368752	755786	59.68%	7.933%
29	6.063	1549	1562	1593	rBV	288832	595085	46.99%	6.246%
30	6.548	1711	1713	1715	rBV2	755	236	0.02%	0.002%
31	6.786	1785	1787	1789	rBV2	1162	710	0.06%	0.007%
32	6.876	1810	1815	1818	rBV4	779	776	0.06%	0.008%
33	6.982	1838	1848	1871	rBV	146046	266287	21.03%	2.795%
34	7.310	1938	1950	1970	rBV	512331	907818	71.68%	9.529%
35	7.619	2036	2046	2064	rBV	102913	180569	14.26%	1.895%
36	7.931	2139	2143	2145	rBV4	1716	1483	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028025.D
 Acq On : 21 Sep 2022 19:14
 Operator : SY/MD
 Sample : N4677-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	8.001	2162	2165	2167	rBV	383	244	0.02%	0.003%
38	8.046	2178	2179	2181	rBV	498	243	0.02%	0.003%
39	8.085	2181	2191	2227	rVV	399799	733255	57.90%	7.697%
40	8.599	2349	2351	2354	rBV2	572	352	0.03%	0.004%
41	8.667	2368	2372	2373	rBV2	588	385	0.03%	0.004%
42	8.706	2381	2384	2386	rVB	741	451	0.04%	0.005%
43	8.735	2389	2393	2396	rBV3	1023	884	0.07%	0.009%
44	8.751	2396	2398	2403	rVB2	1005	677	0.05%	0.007%
45	8.850	2418	2429	2450	rBV	571112	932294	73.61%	9.786%
46	9.156	2520	2524	2525	rBV2	698	463	0.04%	0.005%
47	9.188	2532	2534	2536	rBV	500	240	0.02%	0.003%
48	9.249	2551	2553	2557	rVB2	609	312	0.02%	0.003%
49	9.310	2570	2572	2574	rBV	598	249	0.02%	0.003%
50	9.342	2579	2582	2585	rBV3	932	744	0.06%	0.008%
51	9.439	2610	2612	2614	rVB	485	240	0.02%	0.003%
52	9.477	2622	2624	2626	rBV	782	360	0.03%	0.004%
53	9.538	2640	2643	2644	rBV2	606	390	0.03%	0.004%
54	9.702	2691	2694	2696	rBV2	529	382	0.03%	0.004%
55	9.728	2700	2702	2705	rVV2	566	237	0.02%	0.002%
56	9.853	2737	2741	2745	rBV4	697	576	0.05%	0.006%
57	9.915	2756	2760	2761	rBV3	609	438	0.03%	0.005%
58	10.030	2793	2796	2797	rVV3	481	290	0.02%	0.003%
59	10.062	2800	2806	2808	rVV3	751	619	0.05%	0.006%
60	10.114	2818	2822	2823	rBV2	931	631	0.05%	0.007%
61	10.159	2833	2836	2838	rBV	469	335	0.03%	0.004%
62	10.214	2841	2853	2874	rVV	439650	684684	54.06%	7.187%
63	10.345	2892	2894	2898	rVB4	832	489	0.04%	0.005%
64	10.378	2898	2904	2909	rBV6	2345	2880	0.23%	0.030%
65	10.583	2966	2968	2970	rVB2	818	292	0.02%	0.003%
66	10.667	2990	2994	2996	rBV2	347	211	0.02%	0.002%
67	10.680	2996	2998	3004	rVB3	406	262	0.02%	0.003%
68	10.741	3013	3017	3020	rBV3	621	410	0.03%	0.004%
69	10.779	3026	3029	3032	rVB	482	384	0.03%	0.004%
70	10.799	3032	3035	3040	rBV3	480	317	0.03%	0.003%
71	10.834	3040	3046	3047	rBV2	317	291	0.02%	0.003%
72	10.873	3055	3058	3059	rVB	534	260	0.02%	0.003%
73	10.886	3059	3062	3063	rBV	281	206	0.02%	0.002%
74	10.911	3066	3070	3075	rBV6	1425	1431	0.11%	0.015%
75	10.969	3083	3088	3092	rBV3	376	392	0.03%	0.004%
76	11.098	3125	3128	3130	rBV	327	229	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028025.D
 Acq On : 21 Sep 2022 19:14
 Operator : SY/MD
 Sample : N4677-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.133	3135	3139	3140	rBV2	781	498	0.04%	0.005%
78	11.191	3155	3157	3161	rVB2	372	291	0.02%	0.003%
79	11.246	3162	3174	3197	rBV	496515	765881	60.47%	8.039%
80	11.378	3212	3215	3216	rBV2	902	454	0.04%	0.005%
81	11.461	3237	3241	3246	rBV5	1176	1018	0.08%	0.011%
82	11.535	3256	3264	3268	rBV6	6093	8945	0.71%	0.094%
83	11.622	3280	3291	3310	rBV	514318	804151	63.50%	8.441%
84	11.876	3367	3370	3373	rBV4	631	488	0.04%	0.005%
85	12.258	3481	3489	3492	rVB6	1167	1371	0.11%	0.014%
86	12.403	3529	3534	3536	rBV2	673	512	0.04%	0.005%
87	12.455	3545	3550	3551	rBV2	708	572	0.05%	0.006%
88	12.615	3597	3600	3604	rBV3	744	737	0.06%	0.008%
89	12.895	3684	3687	3691	rBV4	730	676	0.05%	0.007%
90	12.947	3697	3703	3706	rBV4	584	638	0.05%	0.007%
91	13.316	3816	3818	3822	rVB3	439	245	0.02%	0.003%
92	13.596	3902	3905	3911	rBV2	835	787	0.06%	0.008%
93	13.625	3911	3914	3917	rVB3	816	545	0.04%	0.006%
94	13.651	3917	3922	3925	rBV4	726	660	0.05%	0.007%
95	13.741	3945	3950	3951	rBV2	999	672	0.05%	0.007%
96	13.786	3962	3964	3966	rBV2	635	281	0.02%	0.003%
97	13.815	3969	3973	3978	rBV4	863	876	0.07%	0.009%
98	14.030	4037	4040	4042	rBV4	590	305	0.02%	0.003%
99	14.043	4042	4044	4049	rVV3	918	653	0.05%	0.007%
100	14.435	4164	4166	4168	rBV	664	237	0.02%	0.002%




Sum of corrected areas: 9526836

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028025.D
Acq On : 21 Sep 2022 19:14
Operator : SY/MD
Sample : N4677-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

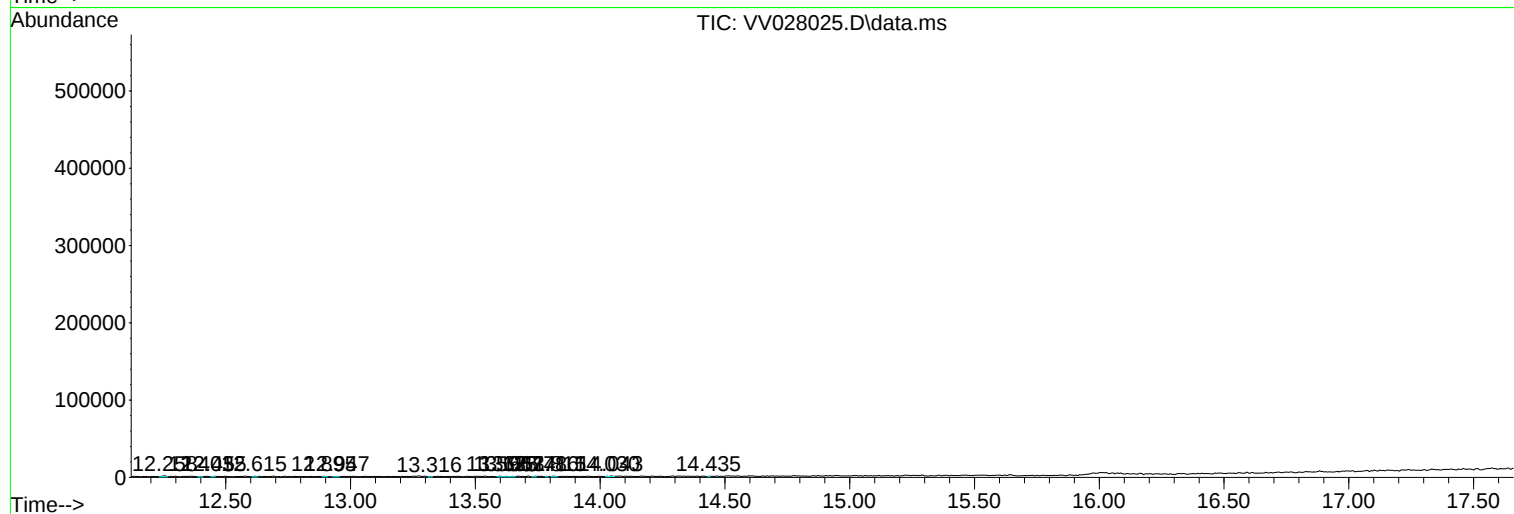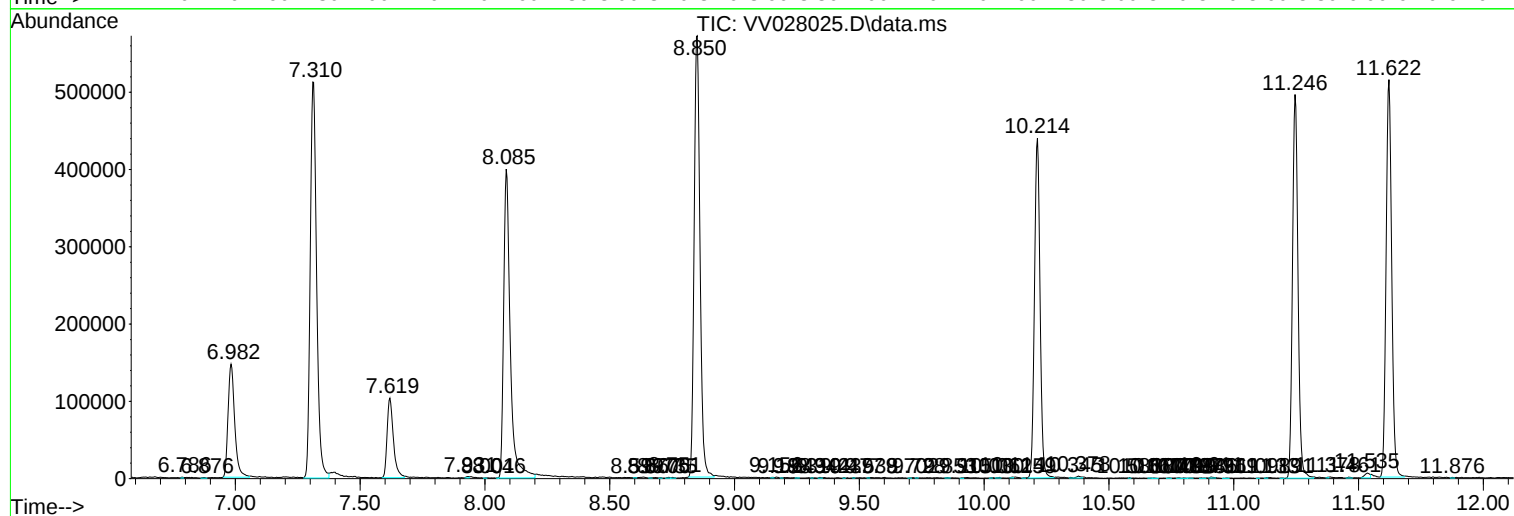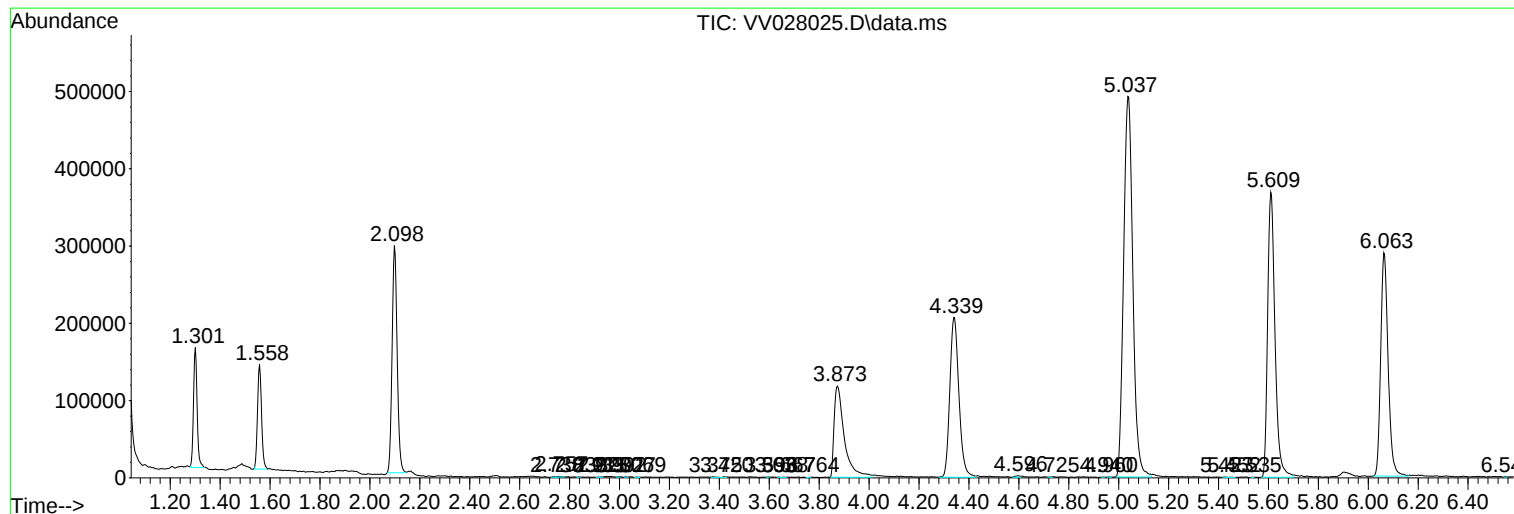

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028025.D
Acq On : 21 Sep 2022 19:14
Operator : SY/MD
Sample : N4677-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028025.D
Acq On : 21 Sep 2022 19:14
Operator : SY/MD
Sample : N4677-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc