

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028026.D
 Acq On : 21 Sep 2022 19:39
 Operator : SY/MD
 Sample : N4677-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	161981	169390	13.65%	1.725%
2	1.558	156	161	176	rVB	146025	167325	13.48%	1.704%
3	2.098	320	329	345	rBV	297546	427982	34.49%	4.359%
4	2.269	380	382	384	rBV2	677	391	0.03%	0.004%
5	2.478	445	447	449	rBV2	806	413	0.03%	0.004%
6	2.561	471	473	474	rBV	741	306	0.02%	0.003%
7	2.619	487	491	493	rBV3	763	613	0.05%	0.006%
8	2.757	531	534	535	rBV3	638	348	0.03%	0.004%
9	2.818	550	553	556	rVB3	485	341	0.03%	0.003%
10	2.838	556	559	562	rBV3	701	539	0.04%	0.005%
11	2.928	583	587	589	rBV2	659	565	0.05%	0.006%
12	3.021	612	616	618	rBV2	540	451	0.04%	0.005%
13	3.082	630	635	640	rBV4	636	653	0.05%	0.007%
14	3.346	712	717	721	rBV2	614	472	0.04%	0.005%
15	3.384	725	729	731	rBV4	1072	767	0.06%	0.008%
16	3.416	735	739	741	rBV2	640	489	0.04%	0.005%
17	3.481	753	759	760	rBV4	802	461	0.04%	0.005%
18	3.793	853	856	858	rBV2	725	413	0.03%	0.004%
19	3.815	858	863	864	rBV2	646	538	0.04%	0.005%
20	3.834	867	869	872	rVB3	841	460	0.04%	0.005%
21	3.876	872	882	918	rBV	127152	360086	29.01%	3.668%
22	4.339	1011	1026	1047	rBV	216359	528392	42.58%	5.382%
23	4.555	1090	1093	1096	rVB2	1017	590	0.05%	0.006%
24	4.571	1096	1098	1102	rBV3	920	704	0.06%	0.007%
25	4.667	1126	1128	1130	rBV	811	416	0.03%	0.004%
26	4.828	1174	1178	1180	rBV3	770	570	0.05%	0.006%
27	5.037	1226	1243	1269	rBV2	482133	1241047	100.00%	12.641%
28	5.301	1323	1325	1329	rVB2	970	693	0.06%	0.007%
29	5.336	1333	1336	1341	rVV4	541	508	0.04%	0.005%
30	5.400	1354	1356	1359	rVB4	920	396	0.03%	0.004%
31	5.429	1363	1365	1367	rBV2	1076	556	0.04%	0.006%
32	5.484	1378	1382	1383	rBV3	641	410	0.03%	0.004%
33	5.609	1409	1421	1449	rBV	383857	786338	63.36%	8.009%
34	6.063	1550	1562	1584	rBV	299674	599174	48.28%	6.103%
35	6.506	1698	1700	1705	rBV4	687	690	0.06%	0.007%
36	6.600	1724	1729	1733	rVB4	753	682	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028026.D
 Acq On : 21 Sep 2022 19:39
 Operator : SY/MD
 Sample : N4677-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.741	1770	1773	1774	rBV	516	323	0.03%	0.003%
38	6.776	1779	1784	1786	rBV3	524	410	0.03%	0.004%
39	6.789	1786	1788	1791	rVB4	556	312	0.03%	0.003%
40	6.809	1791	1794	1797	rVB3	644	411	0.03%	0.004%
41	6.889	1816	1819	1823	rVB2	720	530	0.04%	0.005%
42	6.982	1835	1848	1871	rBV2	139521	261897	21.10%	2.668%
43	7.165	1901	1905	1906	rBV2	849	560	0.05%	0.006%
44	7.259	1930	1934	1938	rBV4	973	824	0.07%	0.008%
45	7.313	1938	1951	1971	rBV	519812	922899	74.36%	9.400%
46	7.619	2036	2046	2069	rBV	104500	189436	15.26%	1.930%
47	7.812	2103	2106	2110	rBV4	1007	790	0.06%	0.008%
48	7.899	2130	2133	2135	rBV3	879	635	0.05%	0.006%
49	8.085	2181	2191	2223	rBV	429495	786836	63.40%	8.014%
50	8.651	2364	2367	2372	rVV3	1002	834	0.07%	0.008%
51	8.850	2417	2429	2453	rVV	584378	952166	76.72%	9.698%
52	9.159	2521	2525	2529	rBV3	883	915	0.07%	0.009%
53	9.249	2550	2553	2556	rBV2	694	500	0.04%	0.005%
54	9.384	2592	2595	2599	rBV2	669	597	0.05%	0.006%
55	9.580	2653	2656	2660	rBV3	510	354	0.03%	0.004%
56	9.712	2694	2697	2701	rVB3	767	391	0.03%	0.004%
57	9.734	2701	2704	2706	rBV2	645	447	0.04%	0.005%
58	9.812	2726	2728	2730	rVB3	951	341	0.03%	0.003%
59	9.963	2771	2775	2780	rBV3	576	525	0.04%	0.005%
60	9.985	2780	2782	2783	rBV2	741	301	0.02%	0.003%
61	10.159	2834	2836	2839	rBV2	525	389	0.03%	0.004%
62	10.214	2841	2853	2874	rVV	448397	710841	57.28%	7.240%
63	10.448	2923	2926	2928	rBV	842	527	0.04%	0.005%
64	10.538	2949	2954	2955	rBV3	798	476	0.04%	0.005%
65	10.596	2969	2972	2976	rBV4	574	399	0.03%	0.004%
66	10.644	2985	2987	2990	rBV2	542	371	0.03%	0.004%
67	10.812	3036	3039	3041	rBV2	514	303	0.02%	0.003%
68	10.985	3090	3093	3100	rVB3	761	832	0.07%	0.008%
69	11.246	3163	3174	3196	rBV	518697	813629	65.56%	8.287%
70	11.487	3245	3249	3253	rBV4	1020	864	0.07%	0.009%
71	11.535	3254	3264	3279	rBV5	7851	19001	1.53%	0.194%
72	11.622	3279	3291	3306	rBV	519480	837302	67.47%	8.528%
73	11.786	3340	3342	3345	rBV4	1241	792	0.06%	0.008%
74	11.998	3407	3408	3414	rVB3	597	410	0.03%	0.004%
75	12.053	3422	3425	3427	rBV2	729	455	0.04%	0.005%
76	12.123	3445	3447	3453	rVB5	985	707	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028026.D
 Acq On : 21 Sep 2022 19:39
 Operator : SY/MD
 Sample : N4677-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	12.239	3479	3483	3489	rBV5	1316	1640	0.13%	0.017%
78	12.422	3538	3540	3545	rBV	926	401	0.03%	0.004%
79	12.680	3617	3620	3622	rBV3	728	435	0.04%	0.004%
80	12.879	3680	3682	3689	rBV5	849	811	0.07%	0.008%
81	12.995	3716	3718	3722	rVB2	601	345	0.03%	0.004%
82	13.020	3722	3726	3729	rBV4	516	476	0.04%	0.005%
83	13.069	3738	3741	3745	rVB2	923	589	0.05%	0.006%
84	13.085	3745	3746	3749	rVB2	598	312	0.03%	0.003%
85	13.229	3788	3791	3793	rVV4	825	425	0.03%	0.004%
86	13.336	3821	3824	3826	rBV4	915	729	0.06%	0.007%
87	13.545	3887	3889	3893	rVB2	696	343	0.03%	0.003%
88	13.574	3893	3898	3900	rBV4	886	883	0.07%	0.009%
89	13.657	3922	3924	3929	rBV2	700	351	0.03%	0.004%
90	13.692	3932	3935	3937	rBV2	724	424	0.03%	0.004%
91	13.770	3956	3959	3963	rBV4	403	304	0.02%	0.003%
92	13.885	3992	3995	3999	rBV3	686	469	0.04%	0.005%
93	13.995	4027	4029	4035	rVB5	650	601	0.05%	0.006%
94	14.024	4035	4038	4041	rBV2	709	453	0.04%	0.005%
95	14.043	4041	4044	4048	rBV4	676	549	0.04%	0.006%
96	14.088	4054	4058	4060	rBV	873	613	0.05%	0.006%
97	14.210	4093	4096	4103	rVB4	830	750	0.06%	0.008%
98	14.342	4133	4137	4138	rBV2	567	443	0.04%	0.005%
99	14.435	4164	4166	4170	rBV2	489	330	0.03%	0.003%
100	14.789	4273	4276	4278	rBV2	850	493	0.04%	0.005%




Sum of corrected areas: 9817870

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028026.D
Acq On : 21 Sep 2022 19:39
Operator : SY/MD
Sample : N4677-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

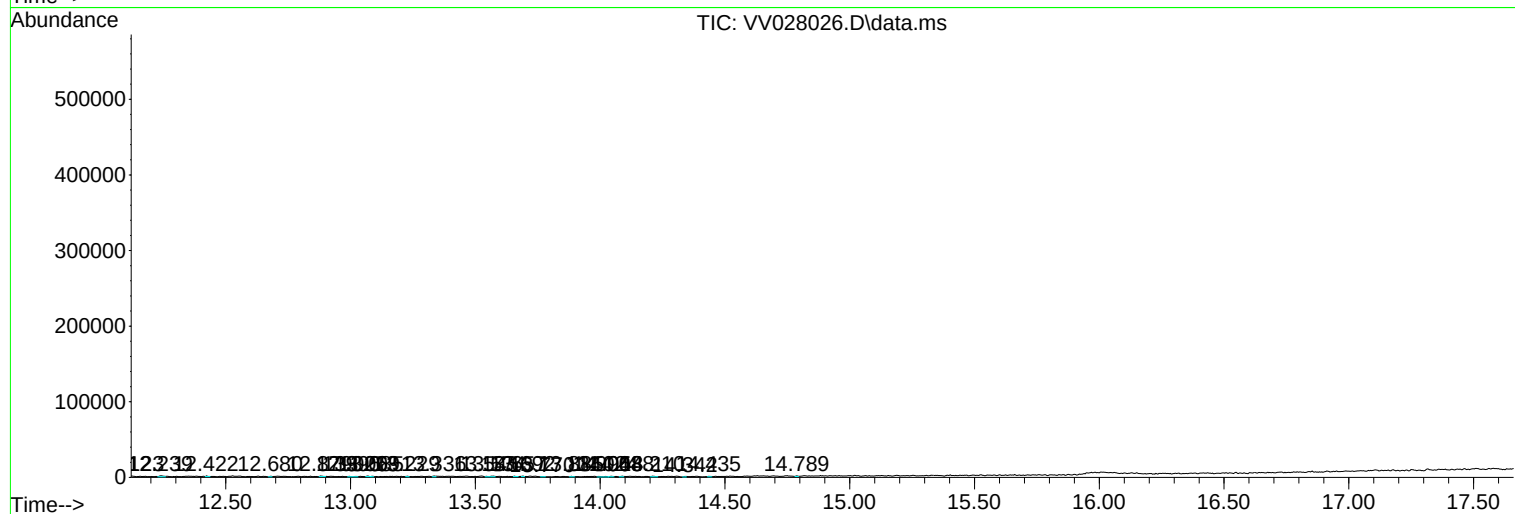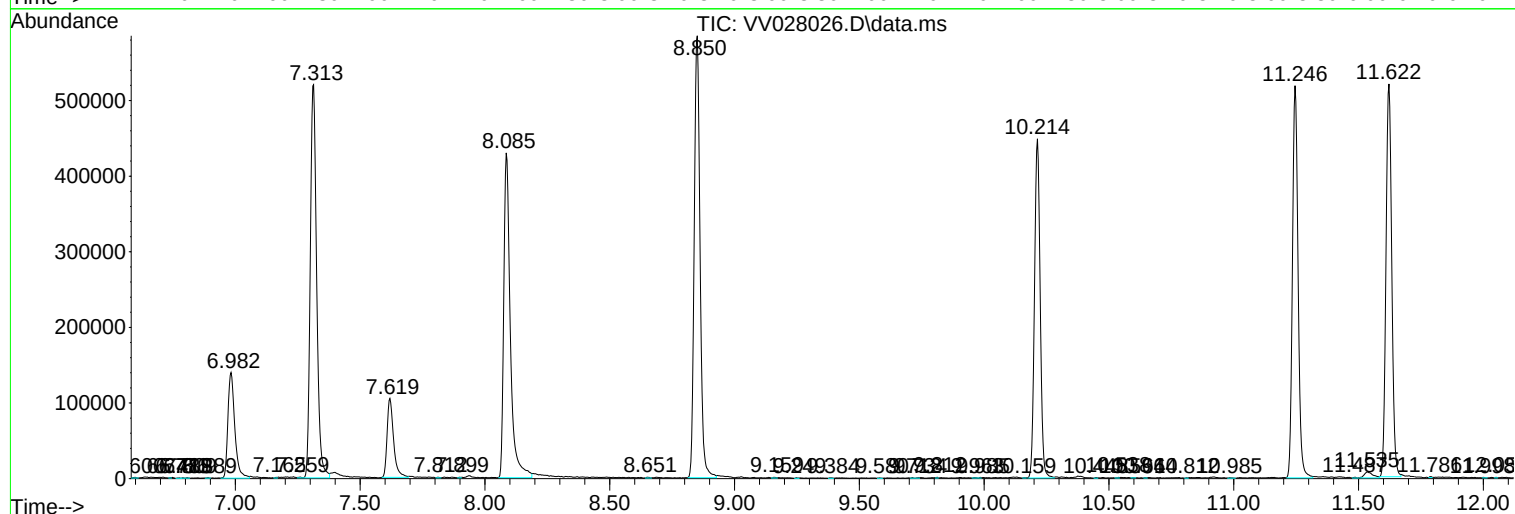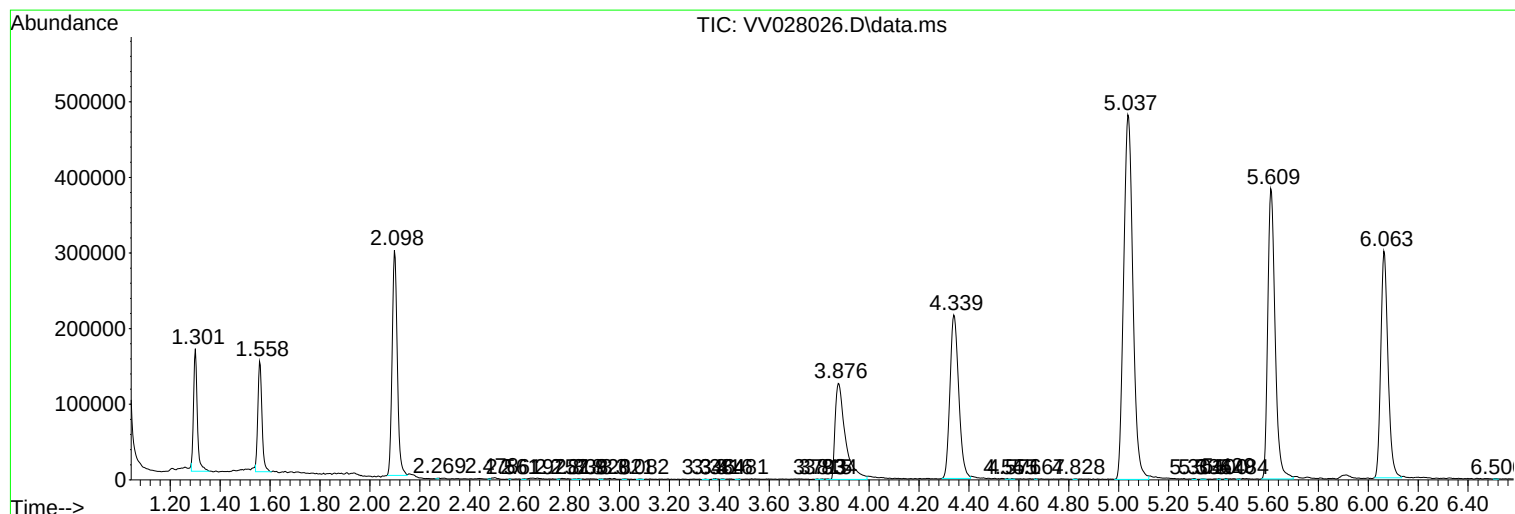

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028026.D
Acq On : 21 Sep 2022 19:39
Operator : SY/MD
Sample : N4677-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028026.D
Acq On : 21 Sep 2022 19:39
Operator : SY/MD
Sample : N4677-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc