

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028027.D
 Acq On : 21 Sep 2022 20:04
 Operator : SY/MD
 Sample : N4677-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV028027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	98	rVB	157742	169421	13.90%	1.757%
2	1.558	155	161	180	rVB	150977	173587	14.24%	1.800%
3	2.098	320	329	346	rBV2	312061	476575	39.11%	4.942%
4	2.468	443	444	446	rBV2	386	198	0.02%	0.002%
5	2.892	574	576	577	rBV2	261	73	0.01%	0.001%
6	2.908	579	581	582	rVB	366	103	0.01%	0.001%
7	2.921	582	585	586	rBV	228	112	0.01%	0.001%
8	3.021	613	616	619	rBV2	302	189	0.02%	0.002%
9	3.043	619	623	625	rBV3	706	395	0.03%	0.004%
10	3.085	635	636	639	rBV2	335	140	0.01%	0.001%
11	3.127	648	649	651	rBV2	219	97	0.01%	0.001%
12	3.301	700	703	707	rBV2	468	299	0.02%	0.003%
13	3.317	707	708	709	rVV	342	84	0.01%	0.001%
14	3.339	713	715	716	rVB	255	81	0.01%	0.001%
15	3.371	716	725	727	rBV3	460	563	0.05%	0.006%
16	3.458	750	752	754	rBV	301	134	0.01%	0.001%
17	3.497	761	764	767	rBV	250	172	0.01%	0.002%
18	3.516	768	770	772	rBV2	302	174	0.01%	0.002%
19	3.558	781	783	785	rBV2	217	96	0.01%	0.001%
20	3.577	788	789	791	rVB2	365	138	0.01%	0.001%
21	3.590	791	793	794	rBV2	354	170	0.01%	0.002%
22	3.613	798	800	802	rVV	194	82	0.01%	0.001%
23	3.622	802	803	804	rVB	295	57	0.00%	0.001%
24	3.661	813	815	818	rBV3	262	146	0.01%	0.002%
25	3.693	822	825	827	rVB	315	148	0.01%	0.002%
26	3.712	829	831	838	rVB	263	224	0.02%	0.002%
27	3.744	838	841	843	rBV2	299	186	0.02%	0.002%
28	3.777	849	851	852	rBV	170	50	0.00%	0.001%
29	3.802	858	859	860	rBV	169	54	0.00%	0.001%
30	3.841	870	871	873	rBV	249	108	0.01%	0.001%
31	3.876	873	882	925	rBV	117362	372841	30.59%	3.866%
32	4.339	1012	1026	1051	rBV	202590	494701	40.59%	5.130%
33	4.680	1131	1132	1134	rBV2	413	217	0.02%	0.002%
34	4.732	1146	1148	1152	rVB3	505	206	0.02%	0.002%
35	4.818	1167	1175	1176	rBV5	1305	1263	0.10%	0.013%
36	5.037	1227	1243	1267	rBV2	475954	1218678	100.00%	12.638%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028027.D
 Acq On : 21 Sep 2022 20:04
 Operator : SY/MD
 Sample : N4677-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.429	1363	1365	1367	rBV2	478	206	0.02%	0.002%
38	5.468	1373	1377	1380	rBV4	671	560	0.05%	0.006%
39	5.609	1409	1421	1449	rBV	376718	772220	63.37%	8.008%
40	6.063	1550	1562	1591	rVB	290130	585484	48.04%	6.071%
41	6.551	1710	1714	1716	rBV4	828	664	0.05%	0.007%
42	6.622	1733	1736	1737	rBV	776	392	0.03%	0.004%
43	6.773	1781	1783	1785	rVB	332	107	0.01%	0.001%
44	6.866	1809	1812	1813	rBV	619	364	0.03%	0.004%
45	6.982	1837	1848	1872	rBV	145634	270849	22.22%	2.809%
46	7.313	1939	1951	1971	rBV	520152	906363	74.37%	9.399%
47	7.619	2037	2046	2065	rBV	104832	181520	14.89%	1.882%
48	8.085	2181	2191	2221	rBV	411851	756688	62.09%	7.847%
49	8.776	2403	2406	2407	rBV2	555	381	0.03%	0.004%
50	8.847	2417	2428	2456	rBV	568320	940845	77.20%	9.757%
51	9.133	2514	2517	2521	rVB3	1084	620	0.05%	0.006%
52	9.310	2569	2572	2577	rVB5	438	448	0.04%	0.005%
53	9.503	2631	2632	2634	rBV	495	223	0.02%	0.002%
54	9.513	2634	2635	2637	rVV	512	228	0.02%	0.002%
55	9.609	2663	2665	2667	rBV2	342	197	0.02%	0.002%
56	9.641	2671	2675	2678	rBV3	693	548	0.04%	0.006%
57	9.670	2682	2684	2687	rBV	357	283	0.02%	0.003%
58	9.699	2691	2693	2694	rBV	404	154	0.01%	0.002%
59	9.728	2701	2702	2703	rBV	348	119	0.01%	0.001%
60	9.767	2712	2714	2718	rVB	529	307	0.03%	0.003%
61	9.837	2730	2736	2737	rBV2	362	313	0.03%	0.003%
62	9.854	2737	2741	2743	rVB	418	255	0.02%	0.003%
63	9.866	2743	2745	2746	rBV	320	141	0.01%	0.001%
64	9.947	2768	2770	2772	rBV2	381	125	0.01%	0.001%
65	10.014	2788	2791	2793	rBV2	587	386	0.03%	0.004%
66	10.043	2797	2800	2802	rBV2	614	357	0.03%	0.004%
67	10.117	2818	2823	2825	rBV4	1172	1073	0.09%	0.011%
68	10.214	2841	2853	2876	rBV	442279	684255	56.15%	7.096%
69	10.490	2938	2939	2941	rBV2	456	260	0.02%	0.003%
70	10.599	2972	2973	2976	rBV	321	195	0.02%	0.002%
71	10.734	3014	3015	3017	rVB	642	181	0.01%	0.002%
72	10.786	3026	3031	3033	rBV5	923	824	0.07%	0.009%
73	10.815	3039	3040	3041	rBV	452	152	0.01%	0.002%
74	10.847	3048	3050	3052	rBV2	606	252	0.02%	0.003%
75	10.998	3095	3097	3098	rBV	429	159	0.01%	0.002%
76	11.037	3107	3109	3110	rBV2	539	206	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028027.D
 Acq On : 21 Sep 2022 20:04
 Operator : SY/MD
 Sample : N4677-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.072	3118	3120	3123	rBV2	927	384	0.03%	0.004%
78	11.095	3125	3127	3129	rBV3	453	206	0.02%	0.002%
79	11.246	3161	3174	3191	rBV	521709	798763	65.54%	8.283%
80	11.622	3279	3291	3315	rBV	518067	818520	67.16%	8.488%
81	11.779	3337	3340	3341	rBV2	680	340	0.03%	0.004%
82	12.091	3434	3437	3440	rBV2	906	665	0.05%	0.007%
83	12.140	3449	3452	3456	rBV2	1229	896	0.07%	0.009%
84	12.358	3515	3520	3521	rBV4	958	697	0.06%	0.007%
85	12.477	3556	3557	3562	rVB2	691	372	0.03%	0.004%
86	13.056	3735	3737	3741	rVB3	685	405	0.03%	0.004%
87	13.191	3776	3779	3781	rBV2	552	341	0.03%	0.004%
88	13.361	3829	3832	3834	rBV2	371	222	0.02%	0.002%
89	13.374	3834	3836	3842	rVB3	531	436	0.04%	0.005%
90	14.230	4099	4102	4103	rBV2	556	327	0.03%	0.003%




Sum of corrected areas: 9643240

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028027.D
Acq On : 21 Sep 2022 20:04
Operator : SY/MD
Sample : N4677-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

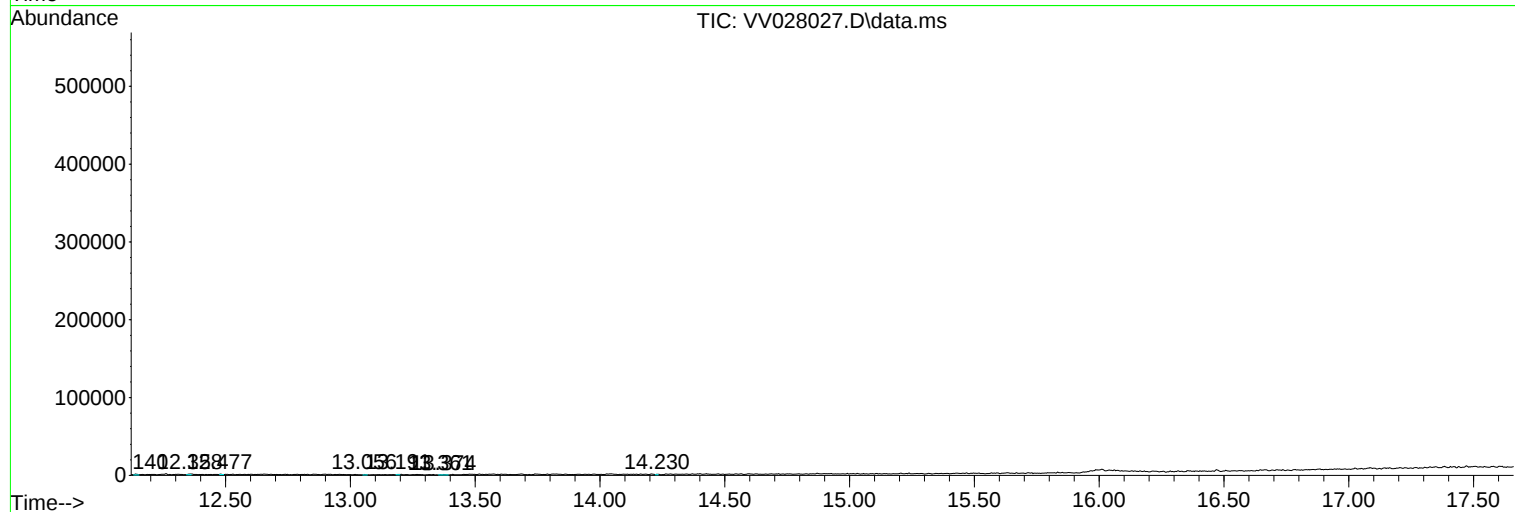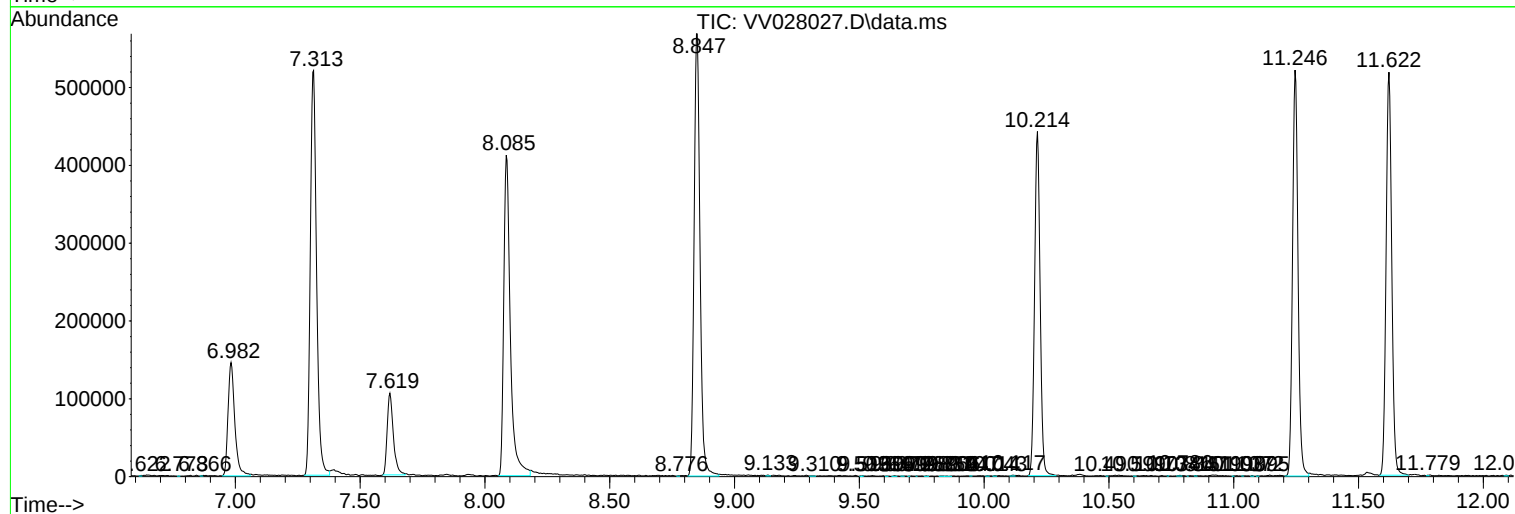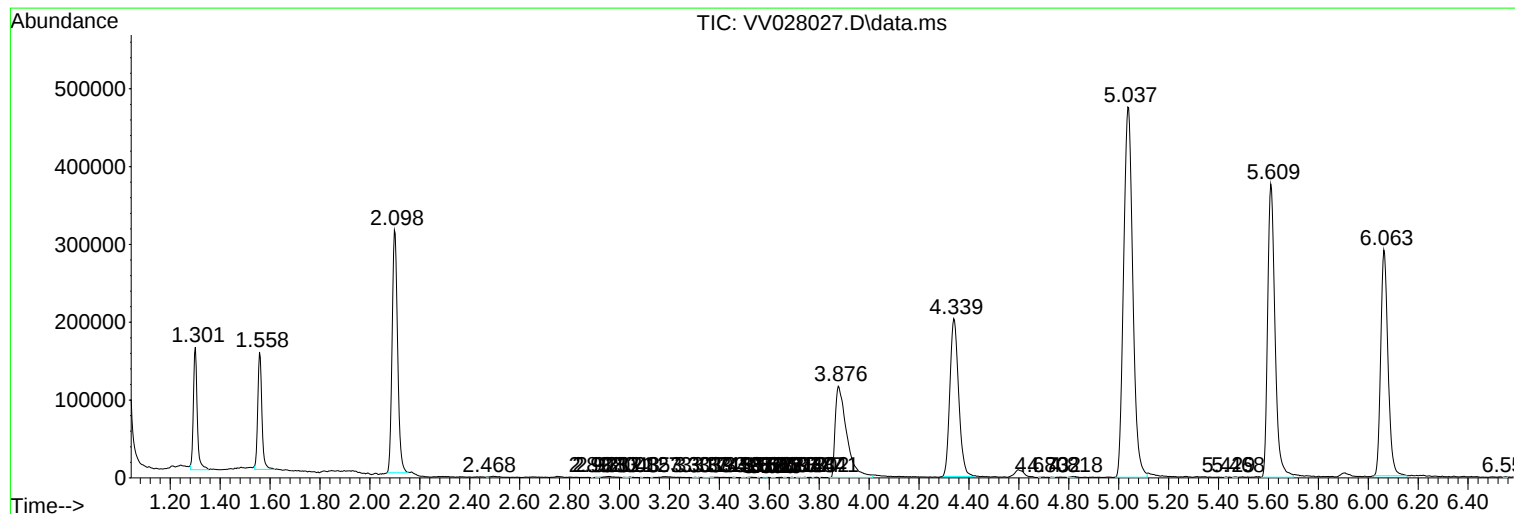

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028027.D
Acq On : 21 Sep 2022 20:04
Operator : SY/MD
Sample : N4677-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028027.D
Acq On : 21 Sep 2022 20:04
Operator : SY/MD
Sample : N4677-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc