

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028028.D
 Acq On : 21 Sep 2022 20:28
 Operator : SY/MD
 Sample : N4677-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028028.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	100	rVB	154723	163157	13.23%	1.551%
2	1.558	156	161	172	rVB	146452	157342	12.76%	1.495%
3	2.098	320	329	349	rBV2	300774	458423	37.16%	4.357%
4	2.912	579	582	585	rBV3	530	338	0.03%	0.003%
5	3.011	610	613	617	rBV2	805	648	0.05%	0.006%
6	3.060	625	628	631	rBV3	634	528	0.04%	0.005%
7	3.134	648	651	653	rBV3	649	436	0.04%	0.004%
8	3.182	662	666	670	rBV6	1516	1488	0.12%	0.014%
9	3.237	681	683	688	rVB3	628	265	0.02%	0.003%
10	3.259	688	690	692	rBV	664	230	0.02%	0.002%
11	3.272	692	694	697	rVB	560	298	0.02%	0.003%
12	3.288	697	699	701	rBV	633	355	0.03%	0.003%
13	3.394	728	732	736	rBV2	426	318	0.03%	0.003%
14	3.491	760	762	769	rVB3	578	511	0.04%	0.005%
15	3.523	769	772	776	rVB2	525	292	0.02%	0.003%
16	3.552	776	781	784	rBV3	370	314	0.03%	0.003%
17	3.577	786	789	792	rBV2	382	251	0.02%	0.002%
18	3.626	802	804	805	rBV2	442	172	0.01%	0.002%
19	3.658	810	814	816	rBV2	446	229	0.02%	0.002%
20	3.880	872	883	915	rBV	125387	389085	31.54%	3.698%
21	4.339	1010	1026	1049	rBV	215345	530733	43.02%	5.044%
22	4.552	1089	1092	1094	rBV3	844	434	0.04%	0.004%
23	4.606	1094	1109	1122	rBV4	8748	22968	1.86%	0.218%
24	4.690	1133	1135	1140	rVV2	592	429	0.03%	0.004%
25	4.722	1143	1145	1147	rBV	467	188	0.02%	0.002%
26	4.735	1147	1149	1153	rVB2	784	453	0.04%	0.004%
27	4.754	1153	1155	1158	rBV	388	218	0.02%	0.002%
28	4.780	1158	1163	1164	rBV	502	406	0.03%	0.004%
29	4.812	1169	1173	1174	rBV	362	247	0.02%	0.002%
30	4.857	1186	1187	1190	rBV	273	166	0.01%	0.002%
31	4.908	1201	1203	1207	rBV3	531	288	0.02%	0.003%
32	4.970	1219	1222	1223	rVB	492	235	0.02%	0.002%
33	5.040	1223	1244	1268	rBV2	483029	1233567	100.00%	11.725%
34	5.314	1327	1329	1334	rVB4	669	539	0.04%	0.005%
35	5.532	1393	1397	1399	rBV2	582	422	0.03%	0.004%
36	5.609	1408	1421	1452	rBV	395592	809919	65.66%	7.698%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028028.D
 Acq On : 21 Sep 2022 20:28
 Operator : SY/MD
 Sample : N4677-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.908	1500	1514	1541	rBV	378701	753957	61.12%	7.166%
38	6.063	1550	1562	1583	rBV	290192	591750	47.97%	5.624%
39	6.616	1730	1734	1735	rBV	614	497	0.04%	0.005%
40	6.699	1758	1760	1768	rVB6	951	817	0.07%	0.008%
41	6.748	1773	1775	1778	rVB3	431	192	0.02%	0.002%
42	6.773	1782	1783	1788	rVB2	486	267	0.02%	0.003%
43	6.796	1788	1790	1792	rBV3	495	223	0.02%	0.002%
44	6.809	1792	1794	1797	rVB2	450	210	0.02%	0.002%
45	6.834	1799	1802	1804	rBV	445	273	0.02%	0.003%
46	6.915	1825	1827	1830	rVB2	656	271	0.02%	0.003%
47	6.982	1834	1848	1874	rBV	140288	260533	21.12%	2.476%
48	7.243	1927	1929	1932	rVB4	499	239	0.02%	0.002%
49	7.262	1932	1935	1939	rBV4	415	345	0.03%	0.003%
50	7.310	1939	1950	1970	rBV	489361	863423	69.99%	8.207%
51	7.619	2035	2046	2064	rBV	104419	185663	15.05%	1.765%
52	7.822	2106	2109	2111	rBV3	826	572	0.05%	0.005%
53	7.928	2138	2142	2143	rBV4	1388	1040	0.08%	0.010%
54	8.085	2181	2191	2223	rBV	411104	756054	61.29%	7.186%
55	8.680	2371	2376	2377	rBV2	837	630	0.05%	0.006%
56	8.767	2401	2403	2404	rBV2	402	175	0.01%	0.002%
57	8.847	2417	2428	2452	rBV	598189	973279	78.90%	9.251%
58	9.069	2494	2497	2500	rBV3	1079	716	0.06%	0.007%
59	9.423	2602	2607	2609	rBV4	480	518	0.04%	0.005%
60	9.596	2658	2661	2663	rBV3	309	214	0.02%	0.002%
61	9.686	2684	2689	2692	rBV3	485	402	0.03%	0.004%
62	9.709	2694	2696	2698	rVV2	462	181	0.01%	0.002%
63	9.725	2698	2701	2703	rVB3	416	184	0.01%	0.002%
64	9.783	2717	2719	2722	rBV	356	189	0.02%	0.002%
65	9.809	2725	2727	2731	rVV	272	172	0.01%	0.002%
66	9.838	2735	2736	2738	rVV	578	207	0.02%	0.002%
67	9.863	2740	2744	2748	rVB3	813	637	0.05%	0.006%
68	9.973	2774	2778	2782	rBV2	675	400	0.03%	0.004%
69	9.992	2782	2784	2786	rBV2	393	230	0.02%	0.002%
70	10.056	2800	2804	2806	rVV	439	260	0.02%	0.002%
71	10.120	2819	2824	2826	rBV3	1138	1000	0.08%	0.010%
72	10.214	2841	2853	2876	rBV	432268	665151	53.92%	6.322%
73	10.313	2881	2884	2887	rVB2	1050	638	0.05%	0.006%
74	10.365	2897	2900	2901	rBV2	1509	687	0.06%	0.007%
75	10.442	2922	2924	2926	rVB2	556	223	0.02%	0.002%
76	10.522	2947	2949	2951	rBV2	647	287	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028028.D
 Acq On : 21 Sep 2022 20:28
 Operator : SY/MD
 Sample : N4677-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.616	2976	2978	2981	rBV2	539	261	0.02%	0.002%
78	10.709	3005	3007	3010	rBV2	554	338	0.03%	0.003%
79	10.728	3011	3013	3016	rVV2	549	287	0.02%	0.003%
80	10.770	3024	3026	3028	rBB2	406	175	0.01%	0.002%
81	10.992	3092	3095	3098	rBV3	725	584	0.05%	0.006%
82	11.021	3102	3104	3105	rBV	524	220	0.02%	0.002%
83	11.185	3153	3155	3156	rBV	682	215	0.02%	0.002%
84	11.246	3163	3174	3196	rBV	530620	832165	67.46%	7.910%
85	11.538	3258	3265	3279	rBV3	6050	11402	0.92%	0.108%
86	11.622	3279	3291	3308	rBV	528119	831671	67.42%	7.905%
87	12.040	3419	3421	3423	rBV2	620	272	0.02%	0.003%
88	12.165	3457	3460	3464	rBV4	595	597	0.05%	0.006%
89	12.580	3586	3589	3591	rBV2	569	420	0.03%	0.004%
90	12.638	3604	3607	3609	rBV2	957	512	0.04%	0.005%
91	12.706	3625	3628	3631	rBV2	508	431	0.03%	0.004%
92	12.808	3658	3660	3662	rVB2	619	232	0.02%	0.002%
93	12.821	3662	3664	3666	rBV3	784	424	0.03%	0.004%
94	12.934	3697	3699	3701	rBV2	489	251	0.02%	0.002%
95	13.117	3754	3756	3760	rVB3	1013	549	0.04%	0.005%
96	13.191	3776	3779	3782	rVV2	658	493	0.04%	0.005%
97	13.628	3913	3915	3917	rBV2	423	180	0.01%	0.002%
98	13.815	3970	3973	3974	rBV2	466	186	0.02%	0.002%
99	13.972	4020	4022	4023	rBV2	423	189	0.02%	0.002%
100	14.300	4121	4124	4125	rBV2	645	401	0.03%	0.004%




Sum of corrected areas: 10521053

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028028.D
Acq On : 21 Sep 2022 20:28
Operator : SY/MD
Sample : N4677-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

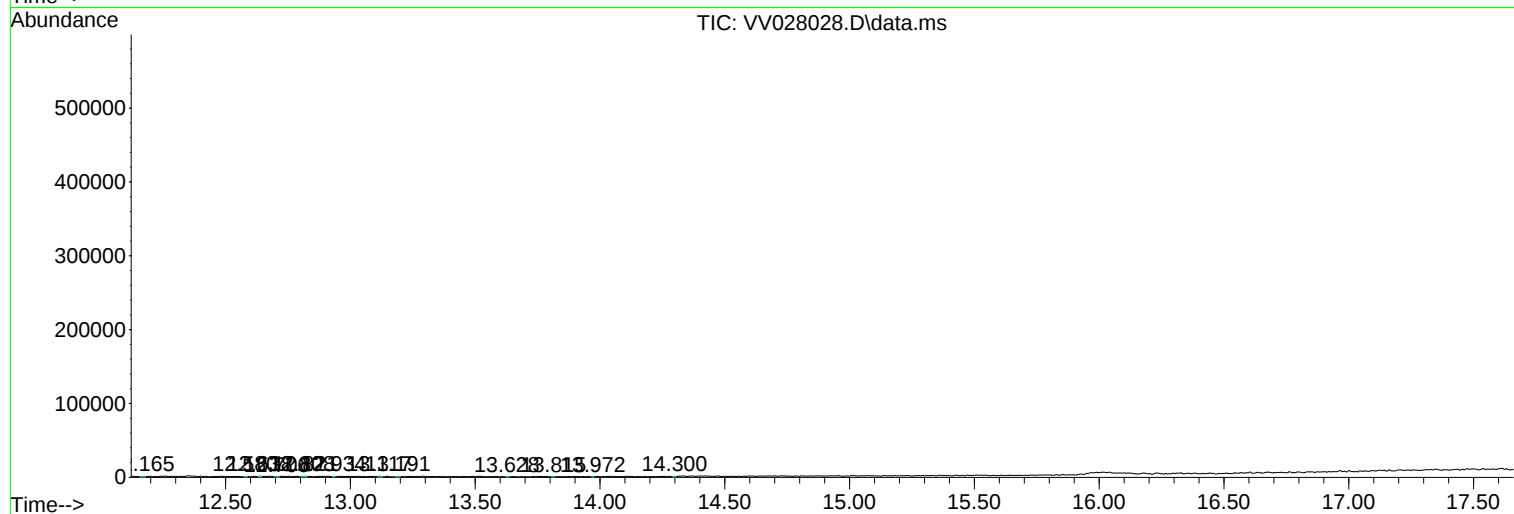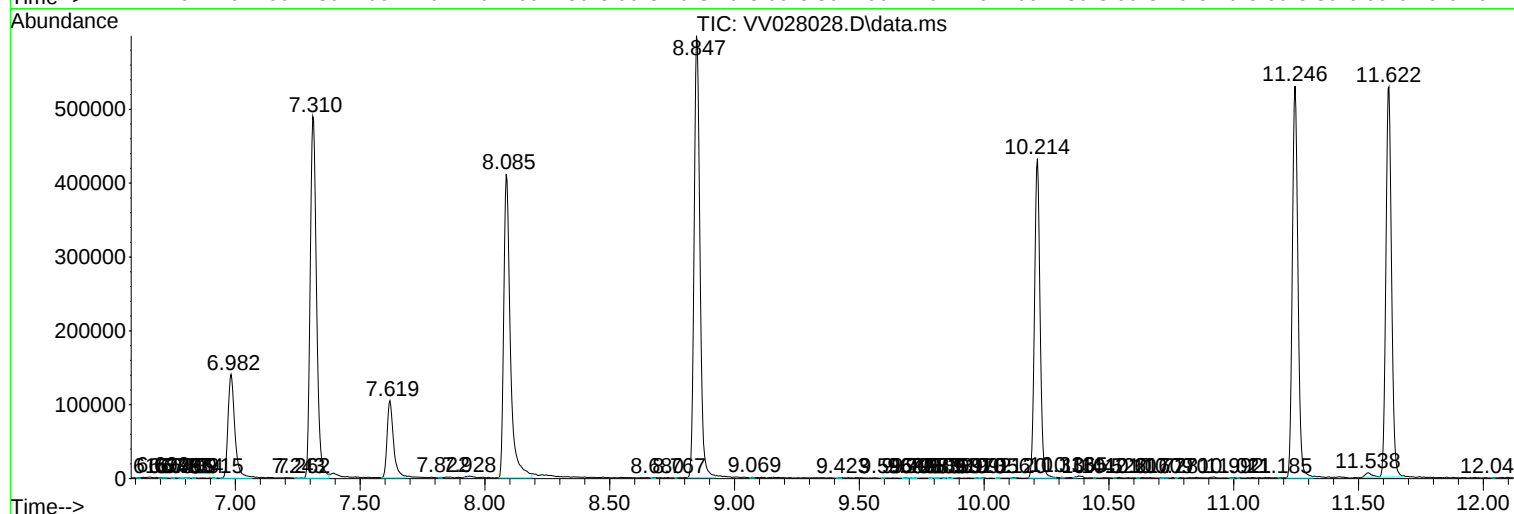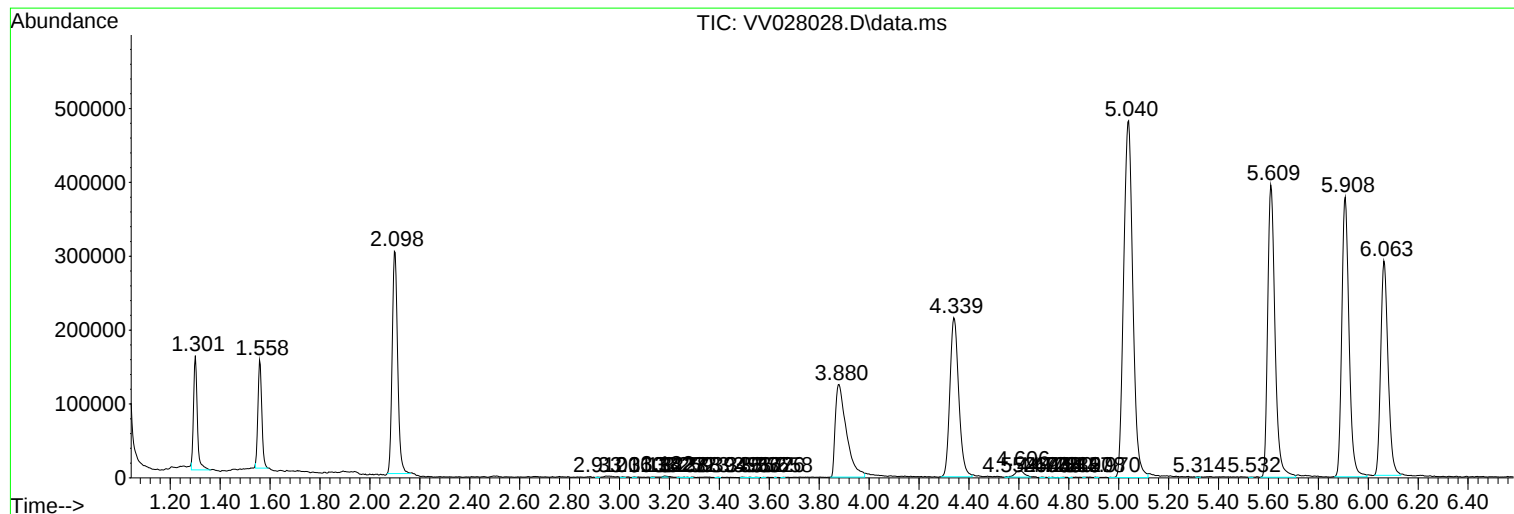

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028028.D
Acq On : 21 Sep 2022 20:28
Operator : SY/MD
Sample : N4677-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028028.D
Acq On : 21 Sep 2022 20:28
Operator : SY/MD
Sample : N4677-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc