

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028029.D
 Acq On : 21 Sep 2022 20:53
 Operator : SY/MD
 Sample : N4677-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028029.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	94	rVB	162028	163775	13.83%	1.703%
2	1.558	155	161	175	rVB	147905	168114	14.20%	1.749%
3	2.098	320	329	343	rBV	295283	425527	35.94%	4.426%
4	2.423	426	430	433	rBV4	597	597	0.05%	0.006%
5	2.481	444	448	449	rBV2	509	324	0.03%	0.003%
6	2.491	449	451	452	rBV	827	418	0.04%	0.004%
7	2.655	496	502	504	rBV3	881	602	0.05%	0.006%
8	2.700	513	516	520	rBV2	824	421	0.04%	0.004%
9	2.741	522	529	532	rBV3	888	812	0.07%	0.008%
10	2.757	532	534	536	rVV2	587	285	0.02%	0.003%
11	2.815	548	552	554	rVB	398	217	0.02%	0.002%
12	2.876	567	571	573	rBV	293	243	0.02%	0.003%
13	2.947	586	593	597	rBV6	1271	1606	0.14%	0.017%
14	3.118	640	646	653	rBV3	387	448	0.04%	0.005%
15	3.227	676	680	682	rBV2	490	385	0.03%	0.004%
16	3.507	761	767	769	rVB2	272	214	0.02%	0.002%
17	3.523	769	772	776	rBV	536	345	0.03%	0.004%
18	3.661	812	815	818	rVB3	491	268	0.02%	0.003%
19	3.844	867	872	873	rBV2	493	331	0.03%	0.003%
20	3.876	873	882	909	rBV2	110574	313949	26.51%	3.265%
21	4.275	1004	1006	1008	rBV2	412	231	0.02%	0.002%
22	4.339	1011	1026	1061	rVV	225283	558200	47.14%	5.806%
23	4.581	1099	1101	1105	rBV2	679	637	0.05%	0.007%
24	4.603	1106	1108	1112	rVB3	589	347	0.03%	0.004%
25	4.703	1137	1139	1142	rBV2	440	235	0.02%	0.002%
26	4.741	1148	1151	1155	rBV	506	302	0.03%	0.003%
27	4.899	1197	1200	1204	rBV2	534	450	0.04%	0.005%
28	4.918	1204	1206	1210	rVB3	599	424	0.04%	0.004%
29	4.950	1214	1216	1219	rVB2	416	239	0.02%	0.002%
30	4.979	1219	1225	1226	rBV2	577	344	0.03%	0.004%
31	5.037	1226	1243	1271	rBV2	460606	1184058	100.00%	12.315%
32	5.410	1356	1359	1363	rVB2	901	618	0.05%	0.006%
33	5.452	1369	1372	1375	rBV4	390	266	0.02%	0.003%
34	5.535	1395	1398	1401	rVB2	666	288	0.02%	0.003%
35	5.552	1401	1403	1406	rBV	503	367	0.03%	0.004%
36	5.609	1409	1421	1451	rBV	375894	761234	64.29%	7.918%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028029.D
 Acq On : 21 Sep 2022 20:53
 Operator : SY/MD
 Sample : N4677-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.847	1493	1495	1497	rBV3	712	370	0.03%	0.004%
38	5.912	1506	1515	1531	rVB8	6302	14699	1.24%	0.153%
39	5.966	1531	1532	1534	rBV8	625	262	0.02%	0.003%
40	5.979	1534	1536	1539	rVB3	625	264	0.02%	0.003%
41	6.063	1550	1562	1585	rBV	274731	565129	47.73%	5.878%
42	6.719	1763	1766	1770	rBV3	961	766	0.06%	0.008%
43	6.777	1781	1784	1789	rVB3	612	404	0.03%	0.004%
44	6.809	1789	1794	1796	rBV3	665	537	0.05%	0.006%
45	6.982	1837	1848	1874	rBV	145714	269951	22.80%	2.808%
46	7.153	1900	1901	1904	rBV3	637	350	0.03%	0.004%
47	7.310	1938	1950	1972	rBV	514792	909437	76.81%	9.459%
48	7.564	2026	2029	2032	rVB4	1128	815	0.07%	0.008%
49	7.619	2034	2046	2064	rBV	102913	181734	15.35%	1.890%
50	8.037	2172	2176	2179	rBV3	847	834	0.07%	0.009%
51	8.085	2180	2191	2227	rBV	418684	767352	64.81%	7.981%
52	8.494	2315	2318	2319	rBV2	558	276	0.02%	0.003%
53	8.577	2342	2344	2348	rBV3	628	501	0.04%	0.005%
54	8.625	2357	2359	2364	rVB6	772	459	0.04%	0.005%
55	8.699	2380	2382	2384	rBV2	564	245	0.02%	0.003%
56	8.722	2387	2389	2391	rBV	696	390	0.03%	0.004%
57	8.777	2405	2406	2410	rVB3	724	253	0.02%	0.003%
58	8.847	2417	2428	2450	rBV	578874	951378	80.35%	9.895%
59	9.092	2502	2504	2509	rVB3	823	502	0.04%	0.005%
60	9.207	2538	2540	2543	rVB3	509	224	0.02%	0.002%
61	9.239	2548	2550	2552	rBV2	828	448	0.04%	0.005%
62	9.336	2578	2580	2582	rBV	477	221	0.02%	0.002%
63	9.439	2608	2612	2613	rBV4	593	282	0.02%	0.003%
64	9.461	2615	2619	2622	rBV4	638	525	0.04%	0.005%
65	9.506	2631	2633	2636	rBV	309	232	0.02%	0.002%
66	9.632	2670	2672	2673	rBV	611	251	0.02%	0.003%
67	9.738	2702	2705	2711	rVB4	374	289	0.02%	0.003%
68	9.764	2711	2713	2716	rBV4	829	481	0.04%	0.005%
69	9.796	2721	2723	2727	rVB3	817	449	0.04%	0.005%
70	9.854	2739	2741	2743	rBV3	425	248	0.02%	0.003%
71	9.873	2743	2747	2749	rBV2	598	431	0.04%	0.004%
72	10.021	2789	2793	2796	rBV4	879	567	0.05%	0.006%
73	10.066	2805	2807	2810	rBV2	381	251	0.02%	0.003%
74	10.214	2841	2853	2874	rVV	445232	695840	58.77%	7.237%
75	10.452	2921	2927	2930	rBV3	311	280	0.02%	0.003%
76	10.538	2952	2954	2958	rBV3	906	579	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028029.D
 Acq On : 21 Sep 2022 20:53
 Operator : SY/MD
 Sample : N4677-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.584	2966	2968	2970	rVB2	771	292	0.02%	0.003%
78	10.670	2989	2995	2999	rBV3	872	879	0.07%	0.009%
79	10.715	3007	3009	3015	rVB4	867	736	0.06%	0.008%
80	10.812	3035	3039	3041	rBV3	474	408	0.03%	0.004%
81	10.883	3059	3061	3063	rBV2	521	237	0.02%	0.002%
82	11.014	3097	3102	3104	rBV3	725	490	0.04%	0.005%
83	11.165	3147	3149	3152	rVB2	802	357	0.03%	0.004%
84	11.246	3162	3174	3204	rBV	536179	825079	69.68%	8.582%
85	11.622	3279	3291	3315	rBV	519784	823795	69.57%	8.568%
86	11.841	3357	3359	3363	rBV2	706	459	0.04%	0.005%
87	12.053	3423	3425	3427	rBV3	484	257	0.02%	0.003%
88	12.927	3696	3697	3700	rBV3	555	231	0.02%	0.002%
89	12.985	3712	3715	3719	rBV	845	515	0.04%	0.005%
90	13.034	3728	3730	3732	rBV2	504	258	0.02%	0.003%
91	13.111	3749	3754	3757	rBV2	373	253	0.02%	0.003%
92	13.317	3816	3818	3822	rVB2	562	291	0.02%	0.003%
93	13.735	3946	3948	3952	rBV3	748	564	0.05%	0.006%
94	13.924	4002	4007	4011	rBV4	940	1005	0.08%	0.010%
95	14.072	4051	4053	4057	rBV3	797	739	0.06%	0.008%
96	14.104	4062	4063	4065	rBV2	789	243	0.02%	0.003%
97	14.477	4177	4179	4182	rBV3	665	326	0.03%	0.003%
98	14.493	4182	4184	4186	rBV2	1131	544	0.05%	0.006%
99	14.574	4208	4209	4212	rBV2	708	375	0.03%	0.004%
100	14.635	4226	4228	4230	rBV2	822	445	0.04%	0.005%


Sum of corrected areas: 9614405

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028029.D
Acq On : 21 Sep 2022 20:53
Operator : SY/MD
Sample : N4677-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

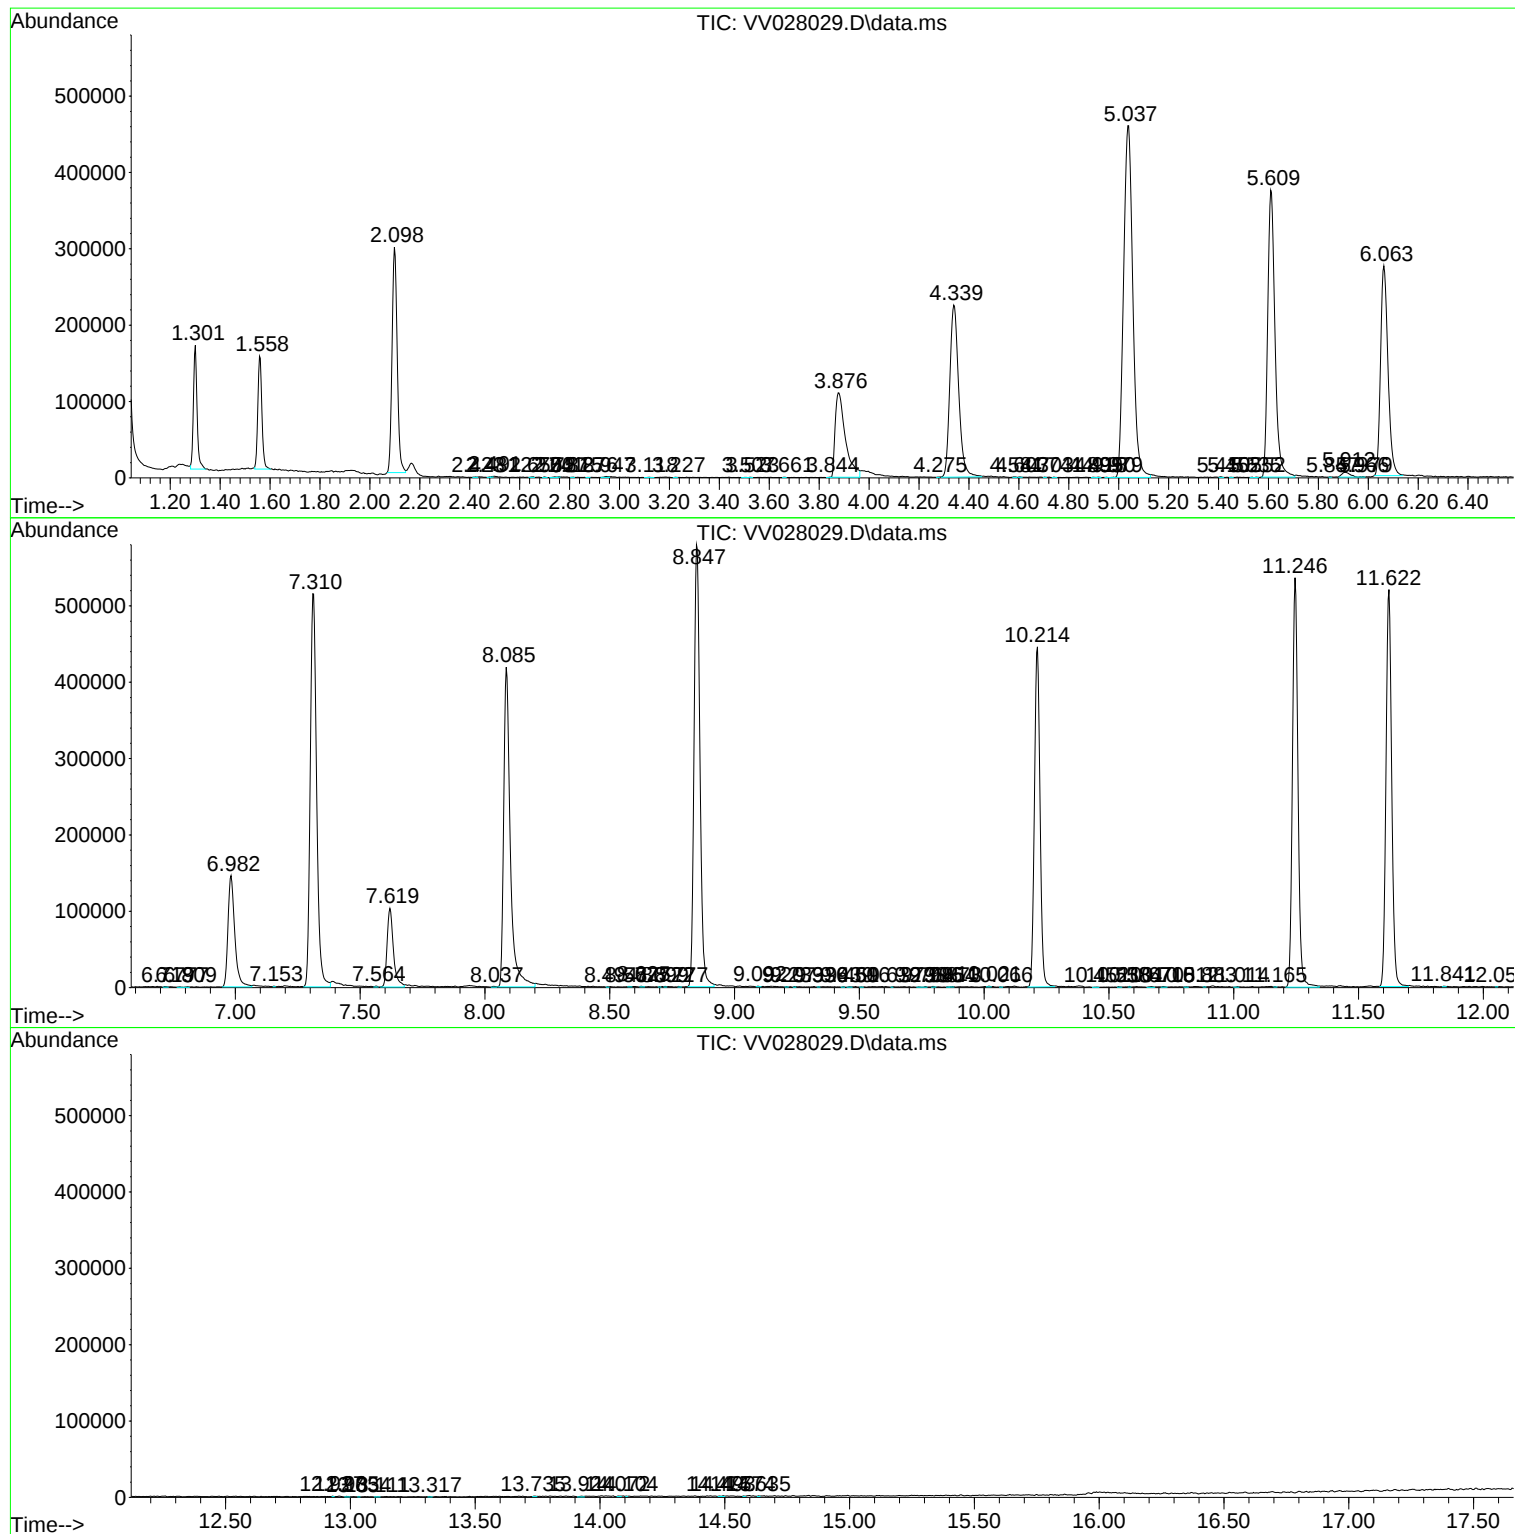

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028029.D
Acq On : 21 Sep 2022 20:53
Operator : SY/MD
Sample : N4677-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028029.D
Acq On : 21 Sep 2022 20:53
Operator : SY/MD
Sample : N4677-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------