

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028032.D
 Acq On : 21 Sep 2022 22:34
 Operator : SY/MD
 Sample : N4689-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	93	rVB	191283	190263	12.97%	1.743%
2	1.558	155	161	177	rVB	172601	198649	13.54%	1.820%
3	2.098	320	329	346	rVB	347976	504527	34.38%	4.623%
4	2.423	427	430	434	rBV2	832	696	0.05%	0.006%
5	2.500	445	454	462	rBV6	3699	5920	0.40%	0.054%
6	2.629	492	494	495	rVB	549	155	0.01%	0.001%
7	2.687	510	512	517	rBV3	692	317	0.02%	0.003%
8	2.745	526	530	531	rBV	739	514	0.04%	0.005%
9	2.854	562	564	567	rBV3	308	174	0.01%	0.002%
10	2.896	575	577	578	rBV	499	149	0.01%	0.001%
11	2.905	578	580	582	rVB	322	126	0.01%	0.001%
12	2.934	584	589	592	rBV3	608	548	0.04%	0.005%
13	2.982	601	604	613	rVB4	705	667	0.05%	0.006%
14	3.044	617	623	626	rBV4	630	597	0.04%	0.005%
15	3.130	648	650	655	rVB2	855	460	0.03%	0.004%
16	3.179	659	665	667	rBV4	885	812	0.06%	0.007%
17	3.214	675	676	678	rBV2	401	149	0.01%	0.001%
18	3.346	715	717	723	rVB5	639	551	0.04%	0.005%
19	3.526	772	773	776	rBV2	584	335	0.02%	0.003%
20	3.552	779	781	784	rVB2	443	175	0.01%	0.002%
21	3.629	803	805	808	rBV3	590	326	0.02%	0.003%
22	3.651	811	812	813	rBV	352	93	0.01%	0.001%
23	3.796	855	857	859	rBV	441	177	0.01%	0.002%
24	3.815	859	863	865	rBV4	666	549	0.04%	0.005%
25	3.876	872	882	923	rBV	140758	411811	28.06%	3.773%
26	4.339	1012	1026	1053	rBV	241256	587297	40.02%	5.381%
27	4.773	1157	1161	1165	rVB3	889	777	0.05%	0.007%
28	4.796	1165	1168	1169	rBV	263	151	0.01%	0.001%
29	5.037	1226	1243	1275	rBV2	569036	1467503	100.00%	13.447%
30	5.346	1337	1339	1341	rBV3	918	585	0.04%	0.005%
31	5.564	1403	1407	1409	rBV3	958	656	0.04%	0.006%
32	5.609	1409	1421	1449	rBV2	413471	852446	58.09%	7.811%
33	5.905	1501	1513	1527	rBV9	6859	18405	1.25%	0.169%
34	5.986	1537	1538	1539	rBV	392	115	0.01%	0.001%
35	6.063	1549	1562	1593	rBV	311778	644337	43.91%	5.904%
36	6.333	1645	1646	1650	rBV3	602	427	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028032.D
 Acq On : 21 Sep 2022 22:34
 Operator : SY/MD
 Sample : N4689-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.371	1656	1658	1659	rBV	510	239	0.02%	0.002%
38	6.481	1690	1692	1693	rBV	449	156	0.01%	0.001%
39	6.606	1725	1731	1734	rBV2	617	634	0.04%	0.006%
40	6.751	1773	1776	1777	rBV2	370	198	0.01%	0.002%
41	6.780	1782	1785	1787	rVV2	575	334	0.02%	0.003%
42	6.809	1791	1794	1796	rBV2	582	303	0.02%	0.003%
43	6.847	1801	1806	1808	rBV	401	351	0.02%	0.003%
44	6.982	1837	1848	1876	rBV	154413	293040	19.97%	2.685%
45	7.310	1939	1950	1970	rBV	609798	1067215	72.72%	9.779%
46	7.619	2036	2046	2069	rBV	113734	204439	13.93%	1.873%
47	8.085	2181	2191	2226	rBV	467560	853642	58.17%	7.822%
48	8.526	2327	2328	2331	rBV2	532	320	0.02%	0.003%
49	8.686	2377	2378	2379	rBV	390	146	0.01%	0.001%
50	8.696	2379	2381	2384	rVV3	733	414	0.03%	0.004%
51	8.770	2402	2404	2406	rBV	508	210	0.01%	0.002%
52	8.847	2417	2428	2456	rBV	628430	1027850	70.04%	9.418%
53	9.149	2517	2522	2523	rBV4	1471	1276	0.09%	0.012%
54	9.214	2539	2542	2543	rBV3	708	451	0.03%	0.004%
55	9.281	2559	2563	2565	rBV4	446	314	0.02%	0.003%
56	9.291	2565	2566	2568	rBV	524	226	0.02%	0.002%
57	9.365	2585	2589	2590	rBV3	448	268	0.02%	0.002%
58	9.416	2603	2605	2607	rVB3	466	175	0.01%	0.002%
59	9.452	2612	2616	2621	rBV3	1081	1028	0.07%	0.009%
60	9.532	2639	2641	2642	rBV	666	218	0.01%	0.002%
61	9.654	2677	2679	2680	rBV	229	82	0.01%	0.001%
62	9.680	2683	2687	2694	rVB4	453	564	0.04%	0.005%
63	9.722	2698	2700	2701	rBV4	237	74	0.01%	0.001%
64	9.793	2717	2722	2725	rBV4	320	322	0.02%	0.003%
65	9.809	2725	2727	2730	rBV	438	234	0.02%	0.002%
66	9.860	2737	2743	2744	rBV4	523	531	0.04%	0.005%
67	9.908	2755	2758	2760	rVB4	499	250	0.02%	0.002%
68	9.982	2777	2781	2785	rVB3	631	445	0.03%	0.004%
69	10.001	2785	2787	2791	rVB	216	105	0.01%	0.001%
70	10.027	2791	2795	2796	rBV	446	256	0.02%	0.002%
71	10.047	2799	2801	2805	rVB3	412	274	0.02%	0.003%
72	10.066	2805	2807	2810	rBV	319	133	0.01%	0.001%
73	10.088	2810	2814	2817	rBV2	393	388	0.03%	0.004%
74	10.156	2832	2835	2839	rVB2	582	409	0.03%	0.004%
75	10.214	2839	2853	2880	rBV	442423	714313	48.68%	6.545%
76	10.333	2888	2890	2892	rVB3	593	237	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028032.D
 Acq On : 21 Sep 2022 22:34
 Operator : SY/MD
 Sample : N4689-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.352	2892	2896	2898	rBV2	824	542	0.04%	0.005%
78	10.365	2898	2900	2903	rBV2	1019	850	0.06%	0.008%
79	10.423	2916	2918	2920	rBV	743	416	0.03%	0.004%
80	10.529	2947	2951	2953	rBV2	867	594	0.04%	0.005%
81	10.641	2984	2986	2987	rBV2	279	97	0.01%	0.001%
82	10.680	2994	2998	3002	rBV3	707	462	0.03%	0.004%
83	10.702	3002	3005	3008	rBV3	571	401	0.03%	0.004%
84	10.760	3020	3023	3026	rBV3	463	281	0.02%	0.003%
85	10.847	3049	3050	3052	rBV	446	145	0.01%	0.001%
86	10.918	3068	3072	3079	rVV9	1647	2018	0.14%	0.018%
87	10.953	3081	3083	3085	rBV2	535	280	0.02%	0.003%
88	10.992	3093	3095	3098	rBV2	561	317	0.02%	0.003%
89	11.120	3133	3135	3136	rBV	396	171	0.01%	0.002%
90	11.178	3151	3153	3154	rBV2	1228	572	0.04%	0.005%
91	11.246	3163	3174	3194	rBV	575458	885830	60.36%	8.117%
92	11.461	3238	3241	3242	rBV	564	297	0.02%	0.003%
93	11.561	3268	3272	3277	rBV5	804	872	0.06%	0.008%
94	11.622	3279	3291	3315	rVV	604388	952701	64.92%	8.730%
95	12.625	3600	3603	3605	rBV2	705	442	0.03%	0.004%
96	13.037	3729	3731	3732	rBV	623	244	0.02%	0.002%
97	13.114	3751	3755	3757	rBV4	855	642	0.04%	0.006%
98	13.230	3789	3791	3793	rBV	412	167	0.01%	0.002%
99	13.259	3796	3800	3801	rBV	1277	866	0.06%	0.008%
100	13.445	3853	3858	3861	rBV5	818	814	0.06%	0.007%


Sum of corrected areas: 10913524

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028032.D
Acq On : 21 Sep 2022 22:34
Operator : SY/MD
Sample : N4689-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

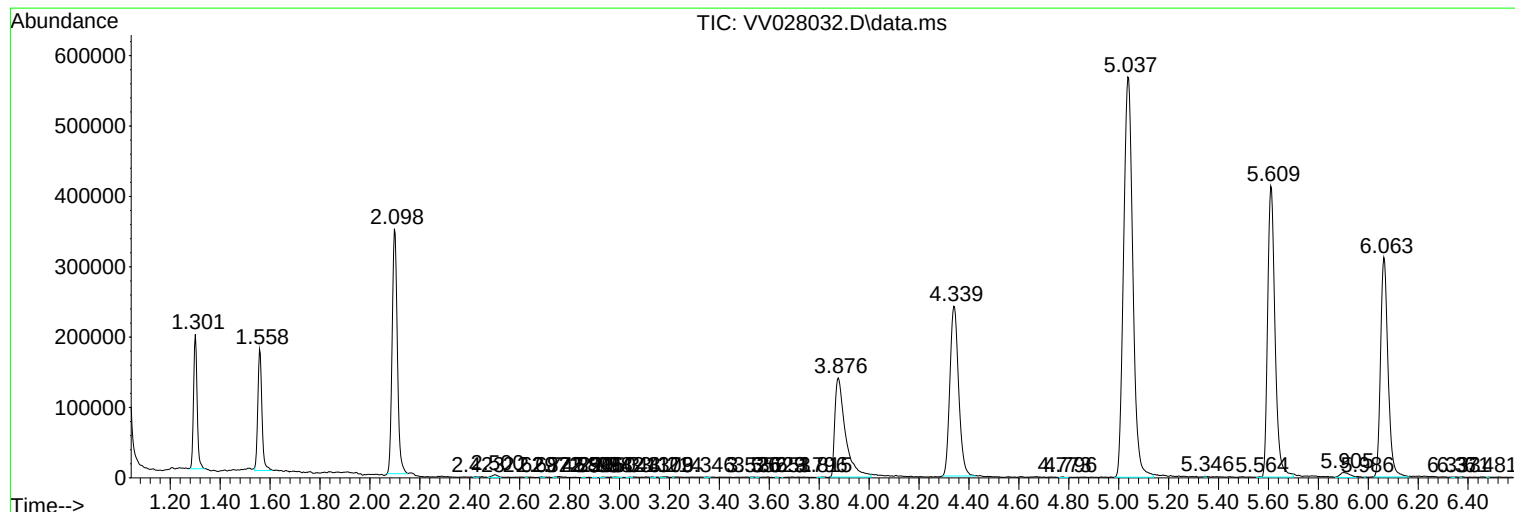

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028032.D
Acq On : 21 Sep 2022 22:34
Operator : SY/MD
Sample : N4689-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028032.D
Acq On : 21 Sep 2022 22:34
Operator : SY/MD
Sample : N4689-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------