

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028033.D
 Acq On : 21 Sep 2022 22:59
 Operator : SY/MD
 Sample : N4659-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV028033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	96	rVB	154323	159667	13.06%	1.636%
2	1.561	156	162	173	rVB	138875	155763	12.74%	1.596%
3	2.098	320	329	347	rBV	288213	414079	33.88%	4.244%
4	2.372	409	414	416	rBV3	795	614	0.05%	0.006%
5	2.410	424	426	428	rBV	400	215	0.02%	0.002%
6	2.565	471	474	475	rBV	404	210	0.02%	0.002%
7	2.684	510	511	516	rBV3	516	324	0.03%	0.003%
8	2.738	524	528	530	rVB	330	231	0.02%	0.002%
9	2.751	530	532	536	rBV3	655	387	0.03%	0.004%
10	2.812	549	551	554	rBV2	628	295	0.02%	0.003%
11	2.938	586	590	591	rBV2	766	451	0.04%	0.005%
12	3.073	629	632	636	rBB3	687	516	0.04%	0.005%
13	3.269	688	693	697	rBV2	272	222	0.02%	0.002%
14	3.291	697	700	704	rBV2	346	222	0.02%	0.002%
15	3.343	713	716	718	rBV3	364	238	0.02%	0.002%
16	3.439	744	746	749	rBV2	498	216	0.02%	0.002%
17	3.497	763	764	766	rVB	577	219	0.02%	0.002%
18	3.516	766	770	773	rVB2	399	246	0.02%	0.003%
19	3.651	810	812	816	rVB	347	222	0.02%	0.002%
20	3.741	836	840	842	rBV2	282	197	0.02%	0.002%
21	3.786	851	854	858	rBV3	449	335	0.03%	0.003%
22	3.835	865	869	870	rBV2	504	277	0.02%	0.003%
23	3.880	870	883	914	rBV	110969	336213	27.51%	3.446%
24	4.339	1011	1026	1054	rBV	219399	541873	44.33%	5.553%
25	4.581	1099	1101	1105	rVB2	500	320	0.03%	0.003%
26	4.600	1105	1107	1109	rBV	794	436	0.04%	0.004%
27	4.651	1120	1123	1124	rBV2	373	222	0.02%	0.002%
28	4.716	1141	1143	1146	rBV2	477	216	0.02%	0.002%
29	4.757	1154	1156	1159	rVB3	692	257	0.02%	0.003%
30	4.773	1159	1161	1164	rVB3	461	249	0.02%	0.003%
31	4.847	1181	1184	1185	rBV2	602	267	0.02%	0.003%
32	4.918	1202	1206	1208	rBV4	626	395	0.03%	0.004%
33	4.954	1215	1217	1221	rVB	495	335	0.03%	0.003%
34	4.976	1221	1224	1225	rBV2	561	384	0.03%	0.004%
35	5.037	1226	1243	1271	rBV2	478306	1222260	100.00%	12.527%
36	5.265	1312	1314	1319	rBV3	1054	992	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028033.D
 Acq On : 21 Sep 2022 22:59
 Operator : SY/MD
 Sample : N4659-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.452	1369	1372	1373	rBV	417	248	0.02%	0.003%
38	5.523	1390	1394	1395	rBV3	864	580	0.05%	0.006%
39	5.609	1409	1421	1448	rBV	407398	831637	68.04%	8.523%
40	5.812	1481	1484	1486	rBV3	731	426	0.03%	0.004%
41	5.979	1533	1536	1538	rBV3	790	517	0.04%	0.005%
42	6.063	1549	1562	1587	rBV	289344	590634	48.32%	6.053%
43	6.417	1669	1672	1673	rBV	536	313	0.03%	0.003%
44	6.574	1719	1721	1723	rBV3	637	266	0.02%	0.003%
45	6.609	1730	1732	1737	rBV5	848	752	0.06%	0.008%
46	6.844	1803	1805	1806	rBV2	578	273	0.02%	0.003%
47	6.867	1810	1812	1814	rBV4	374	197	0.02%	0.002%
48	6.941	1831	1835	1837	rBV3	544	406	0.03%	0.004%
49	6.982	1837	1848	1876	rVV2	138149	261559	21.40%	2.681%
50	7.146	1897	1899	1902	rBV4	682	404	0.03%	0.004%
51	7.269	1935	1937	1938	rBV	695	349	0.03%	0.004%
52	7.310	1939	1950	1970	rVV	510225	891262	72.92%	9.134%
53	7.577	2031	2033	2035	rBV3	571	358	0.03%	0.004%
54	7.619	2036	2046	2073	rVV	98512	178555	14.61%	1.830%
55	7.838	2112	2114	2116	rBV2	557	253	0.02%	0.003%
56	7.851	2116	2118	2120	rVV2	483	216	0.02%	0.002%
57	7.934	2134	2144	2145	rBV5	2525	2692	0.22%	0.028%
58	8.085	2181	2191	2223	rBV	412979	773030	63.25%	7.923%
59	8.703	2382	2383	2387	rVB3	478	205	0.02%	0.002%
60	8.799	2410	2413	2416	rBV3	589	486	0.04%	0.005%
61	8.847	2416	2428	2447	rBV	616333	998305	81.68%	10.231%
62	9.114	2509	2511	2514	rBV4	660	260	0.02%	0.003%
63	9.249	2551	2553	2556	rBV3	708	545	0.04%	0.006%
64	9.330	2577	2578	2582	rBV	588	367	0.03%	0.004%
65	9.352	2582	2585	2587	rBV2	537	325	0.03%	0.003%
66	9.529	2636	2640	2643	rBV4	846	596	0.05%	0.006%
67	9.545	2643	2645	2647	rBV2	645	377	0.03%	0.004%
68	9.600	2660	2662	2666	rBV	538	354	0.03%	0.004%
69	9.870	2744	2746	2750	rVB	628	265	0.02%	0.003%
70	9.889	2750	2752	2754	rBV2	824	442	0.04%	0.005%
71	9.931	2763	2765	2770	rBV2	663	597	0.05%	0.006%
72	9.992	2781	2784	2785	rBV	623	374	0.03%	0.004%
73	10.214	2841	2853	2872	rBV	443527	699312	57.21%	7.167%
74	10.442	2921	2924	2925	rBV2	402	254	0.02%	0.003%
75	10.490	2936	2939	2944	rVB2	673	610	0.05%	0.006%
76	10.539	2949	2954	2955	rBV3	725	602	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028033.D
 Acq On : 21 Sep 2022 22:59
 Operator : SY/MD
 Sample : N4659-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.606	2972	2975	2979	rBV3	262	229	0.02%	0.002%
78	10.722	3007	3011	3015	rBV2	558	379	0.03%	0.004%
79	10.783	3027	3030	3031	rBV	524	255	0.02%	0.003%
80	10.850	3049	3051	3055	rVB4	324	215	0.02%	0.002%
81	10.876	3055	3059	3064	rVB3	433	446	0.04%	0.005%
82	10.912	3064	3070	3071	rBV	1381	1153	0.09%	0.012%
83	10.979	3087	3091	3093	rBV	255	204	0.02%	0.002%
84	10.995	3093	3096	3098	rBV	392	278	0.02%	0.003%
85	11.101	3126	3129	3134	rBV5	452	500	0.04%	0.005%
86	11.246	3162	3174	3192	rBV	542105	841942	68.88%	8.629%
87	11.535	3256	3264	3275	rBV6	5215	11315	0.93%	0.116%
88	11.619	3280	3290	3308	rVV	520039	816869	66.83%	8.372%
89	11.924	3383	3385	3386	rBV2	576	307	0.03%	0.003%
90	12.175	3461	3463	3464	rBV2	694	304	0.02%	0.003%
91	12.423	3535	3540	3542	rBV3	738	641	0.05%	0.007%
92	12.950	3702	3704	3706	rBV3	456	208	0.02%	0.002%
93	13.091	3743	3748	3750	rBV2	697	506	0.04%	0.005%
94	13.143	3762	3764	3768	rBV	796	399	0.03%	0.004%
95	13.448	3855	3859	3860	rBV2	653	484	0.04%	0.005%
96	13.580	3898	3900	3902	rBV2	560	321	0.03%	0.003%
97	13.625	3912	3914	3917	rVB2	1073	373	0.03%	0.004%
98	14.024	4036	4038	4041	rBV2	745	338	0.03%	0.003%
99	14.146	4074	4076	4079	rBV2	486	316	0.03%	0.003%
100	14.220	4096	4099	4101	rBV3	1059	615	0.05%	0.006%




Sum of corrected areas: 9757365

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028033.D
Acq On : 21 Sep 2022 22:59
Operator : SY/MD
Sample : N4659-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

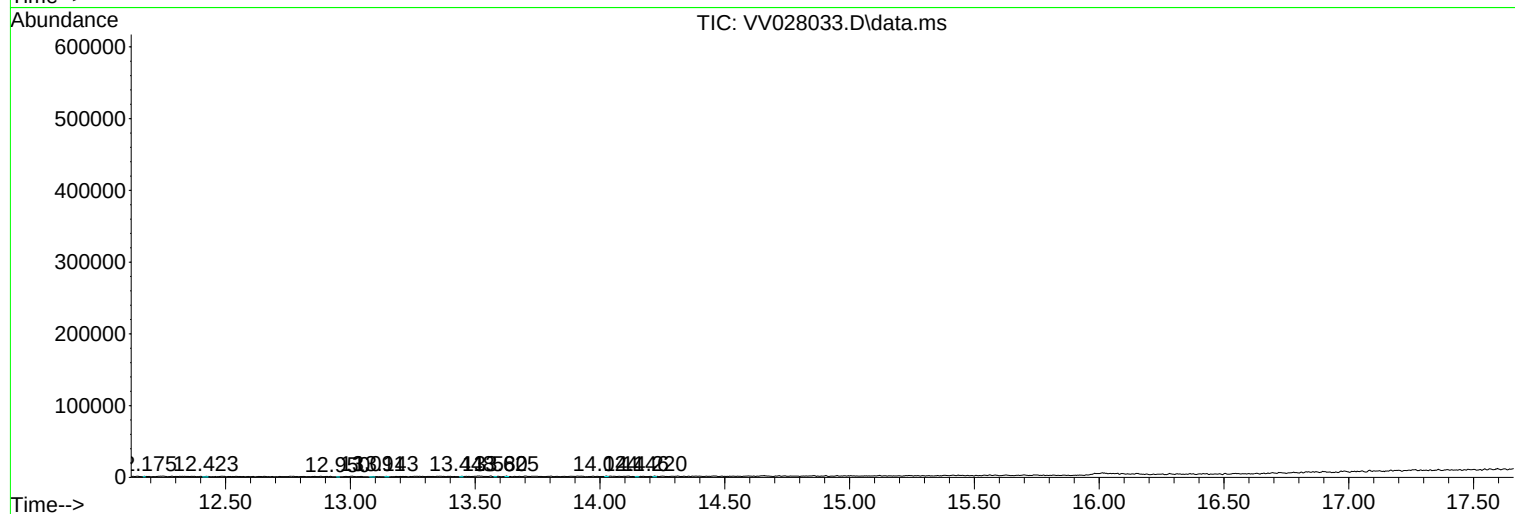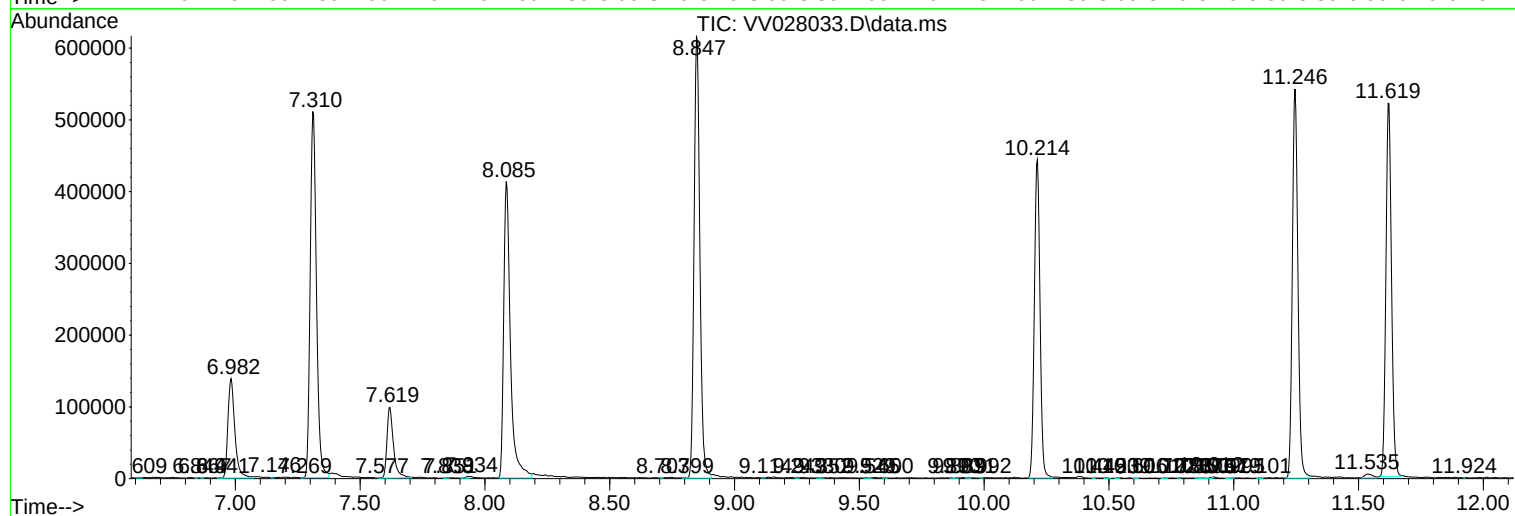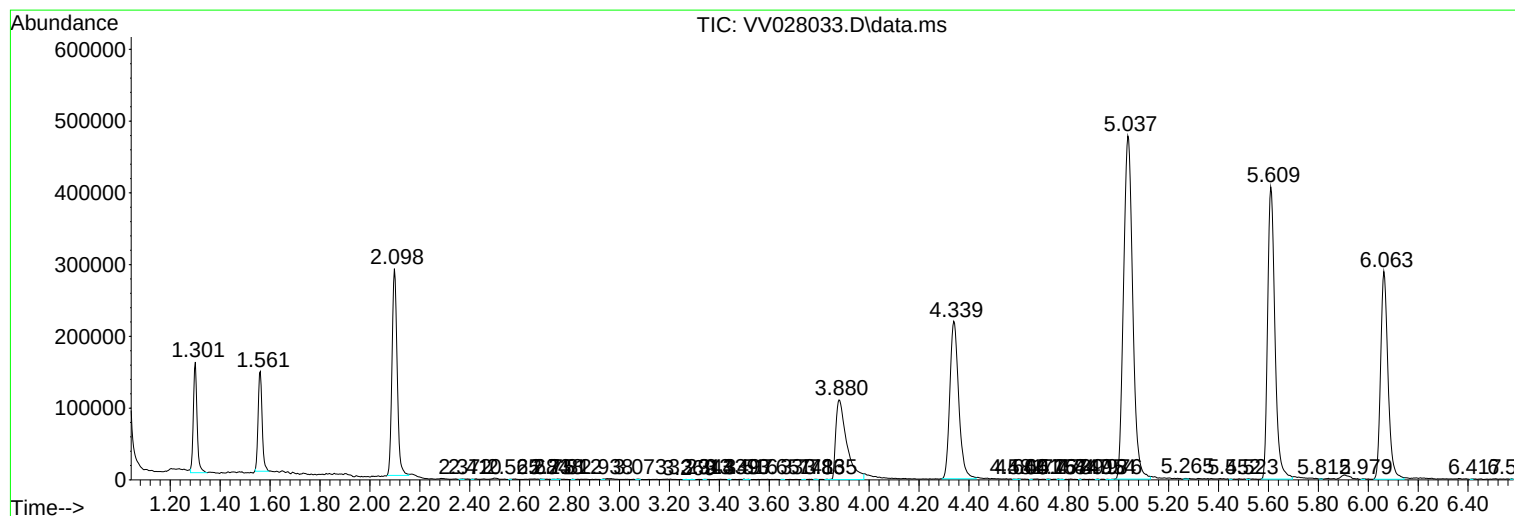

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028033.D
Acq On : 21 Sep 2022 22:59
Operator : SY/MD
Sample : N4659-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028033.D
Acq On : 21 Sep 2022 22:59
Operator : SY/MD
Sample : N4659-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc