

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028034.D
 Acq On : 21 Sep 2022 23:24
 Operator : SY/MD
 Sample : N4659-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	98	rVB	168577	175125	13.75%	1.751%
2	1.561	156	162	175	rVB	144813	161017	12.64%	1.610%
3	2.098	320	329	349	rBV	297152	429106	33.69%	4.291%
4	2.638	495	497	498	rBV	675	305	0.02%	0.003%
5	2.880	568	572	573	rBV2	522	290	0.02%	0.003%
6	3.207	672	674	677	rBV	691	430	0.03%	0.004%
7	3.224	677	679	681	rBV2	417	205	0.02%	0.002%
8	3.278	692	696	700	rBV3	528	563	0.04%	0.006%
9	3.375	725	726	729	rBV3	362	236	0.02%	0.002%
10	3.410	735	737	738	rBV2	418	194	0.02%	0.002%
11	3.436	743	745	749	rVB2	412	329	0.03%	0.003%
12	3.523	768	772	775	rVB	903	541	0.04%	0.005%
13	3.555	775	782	785	rBV2	850	871	0.07%	0.009%
14	3.632	804	806	808	rBV2	726	319	0.03%	0.003%
15	3.677	817	820	822	rBV2	595	422	0.03%	0.004%
16	3.825	862	866	869	rVB3	486	451	0.04%	0.005%
17	3.879	874	883	920	rBV	115904	360961	28.34%	3.609%
18	4.243	994	996	998	rBV2	652	395	0.03%	0.004%
19	4.339	1010	1026	1050	rBV	216951	540274	42.41%	5.402%
20	4.568	1095	1097	1100	rVV3	479	236	0.02%	0.002%
21	4.600	1104	1107	1109	rBV2	406	214	0.02%	0.002%
22	4.613	1109	1111	1114	rVB3	644	382	0.03%	0.004%
23	4.748	1151	1153	1155	rBV2	377	216	0.02%	0.002%
24	4.796	1162	1168	1171	rBV2	688	674	0.05%	0.007%
25	4.828	1173	1178	1179	rBV3	434	333	0.03%	0.003%
26	4.879	1191	1194	1196	rVB	567	319	0.03%	0.003%
27	4.973	1221	1223	1226	rVB2	655	292	0.02%	0.003%
28	5.037	1226	1243	1284	rBV2	493457	1273826	100.00%	12.737%
29	5.269	1313	1315	1323	rVB5	979	656	0.05%	0.007%
30	5.301	1323	1325	1329	rBV3	678	530	0.04%	0.005%
31	5.387	1349	1352	1353	rBV3	467	273	0.02%	0.003%
32	5.548	1401	1402	1404	rBV3	481	219	0.02%	0.002%
33	5.609	1409	1421	1446	rBV	398478	813313	63.85%	8.133%
34	6.063	1549	1562	1593	rBV	311126	635699	49.90%	6.357%
35	6.333	1643	1646	1649	rBV3	1137	726	0.06%	0.007%
36	6.731	1767	1770	1771	rBV2	1107	636	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028034.D
 Acq On : 21 Sep 2022 23:24
 Operator : SY/MD
 Sample : N4659-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.796	1787	1790	1792	rVB3	702	407	0.03%	0.004%
38	6.812	1792	1795	1799	rBV4	528	453	0.04%	0.005%
39	6.889	1816	1819	1821	rBV3	712	459	0.04%	0.005%
40	6.982	1837	1848	1870	rBV	152014	279850	21.97%	2.798%
41	7.310	1937	1950	1971	rBV	544726	948246	74.44%	9.482%
42	7.545	2021	2023	2024	rBV2	793	362	0.03%	0.004%
43	7.619	2036	2046	2070	rBV	106424	189150	14.85%	1.891%
44	7.821	2101	2109	2113	rBV7	819	1145	0.09%	0.011%
45	8.040	2174	2177	2179	rBV2	350	226	0.02%	0.002%
46	8.085	2181	2191	2218	rBV	408889	749463	58.84%	7.494%
47	8.564	2337	2340	2344	rBV5	542	330	0.03%	0.003%
48	8.606	2351	2353	2358	rVB3	891	546	0.04%	0.005%
49	8.635	2360	2362	2365	rBV2	325	197	0.02%	0.002%
50	8.738	2390	2394	2398	rBV5	370	289	0.02%	0.003%
51	8.850	2416	2429	2449	rBV	577319	954265	74.91%	9.542%
52	9.050	2489	2491	2494	rVB2	1093	601	0.05%	0.006%
53	9.339	2578	2581	2582	rBV2	511	245	0.02%	0.002%
54	9.407	2600	2602	2605	rVB5	806	293	0.02%	0.003%
55	9.535	2640	2642	2645	rBV3	640	379	0.03%	0.004%
56	9.641	2673	2675	2678	rBV3	543	337	0.03%	0.003%
57	9.760	2709	2712	2715	rBV2	525	411	0.03%	0.004%
58	9.969	2776	2777	2780	rBV	871	378	0.03%	0.004%
59	9.985	2780	2782	2784	rBV2	422	200	0.02%	0.002%
60	10.214	2841	2853	2876	rBV	466441	743460	58.36%	7.434%
61	10.455	2926	2928	2929	rBV	647	264	0.02%	0.003%
62	10.497	2938	2941	2942	rBV	473	240	0.02%	0.002%
63	10.664	2990	2993	2994	rBV2	506	315	0.02%	0.003%
64	10.718	3009	3010	3013	rBV	465	239	0.02%	0.002%
65	10.731	3013	3014	3017	rVB2	549	243	0.02%	0.002%
66	10.805	3035	3037	3039	rVB2	590	196	0.02%	0.002%
67	10.966	3084	3087	3090	rBV3	463	223	0.02%	0.002%
68	11.008	3099	3100	3103	rBV2	579	222	0.02%	0.002%
69	11.062	3114	3117	3119	rBV3	367	203	0.02%	0.002%
70	11.108	3125	3131	3135	rVB5	982	1003	0.08%	0.010%
71	11.130	3136	3138	3140	rBV2	470	224	0.02%	0.002%
72	11.246	3163	3174	3195	rBV	538421	839363	65.89%	8.393%
73	11.538	3256	3265	3274	rBV9	5276	10605	0.83%	0.106%
74	11.622	3280	3291	3311	rBV	556389	864418	67.86%	8.644%
75	11.966	3394	3398	3402	rVB2	811	648	0.05%	0.006%
76	11.992	3403	3406	3410	rBV2	487	300	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028034.D
 Acq On : 21 Sep 2022 23:24
 Operator : SY/MD
 Sample : N4659-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	12.017	3412	3414	3416	rBV2	460	192	0.02%	0.002%
78	12.059	3425	3427	3428	rBV	568	259	0.02%	0.003%
79	12.204	3470	3472	3476	rBV3	461	264	0.02%	0.003%
80	12.284	3495	3497	3502	rVB	520	355	0.03%	0.004%
81	12.355	3517	3519	3522	rBV3	358	227	0.02%	0.002%
82	12.445	3543	3547	3549	rBV2	443	308	0.02%	0.003%
83	12.471	3549	3555	3558	rVV3	468	514	0.04%	0.005%
84	12.538	3574	3576	3580	rBV4	565	442	0.03%	0.004%
85	12.651	3608	3611	3615	rVB2	530	424	0.03%	0.004%
86	12.718	3630	3632	3634	rBV	524	256	0.02%	0.003%
87	12.770	3645	3648	3651	rVB2	408	277	0.02%	0.003%
88	12.892	3680	3686	3688	rBV5	962	918	0.07%	0.009%
89	12.908	3690	3691	3696	rBV3	505	335	0.03%	0.003%
90	12.947	3700	3703	3704	rBV2	406	203	0.02%	0.002%
91	12.992	3714	3717	3718	rBV2	577	225	0.02%	0.002%
92	13.127	3757	3759	3764	rVB3	496	317	0.02%	0.003%
93	13.300	3811	3813	3817	rBV2	710	457	0.04%	0.005%
94	13.416	3846	3849	3852	rVB2	720	411	0.03%	0.004%
95	13.574	3895	3898	3903	rVB	806	466	0.04%	0.005%
96	13.603	3904	3907	3911	rVB3	763	611	0.05%	0.006%
97	13.696	3933	3936	3937	rBV2	512	280	0.02%	0.003%
98	14.043	4042	4044	4050	rVB4	1021	916	0.07%	0.009%
99	14.069	4050	4052	4054	rBV2	1001	584	0.05%	0.006%
100	14.162	4078	4081	4084	rVB3	1018	545	0.04%	0.005%


Sum of corrected areas: 10000762

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028034.D
Acq On : 21 Sep 2022 23:24
Operator : SY/MD
Sample : N4659-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

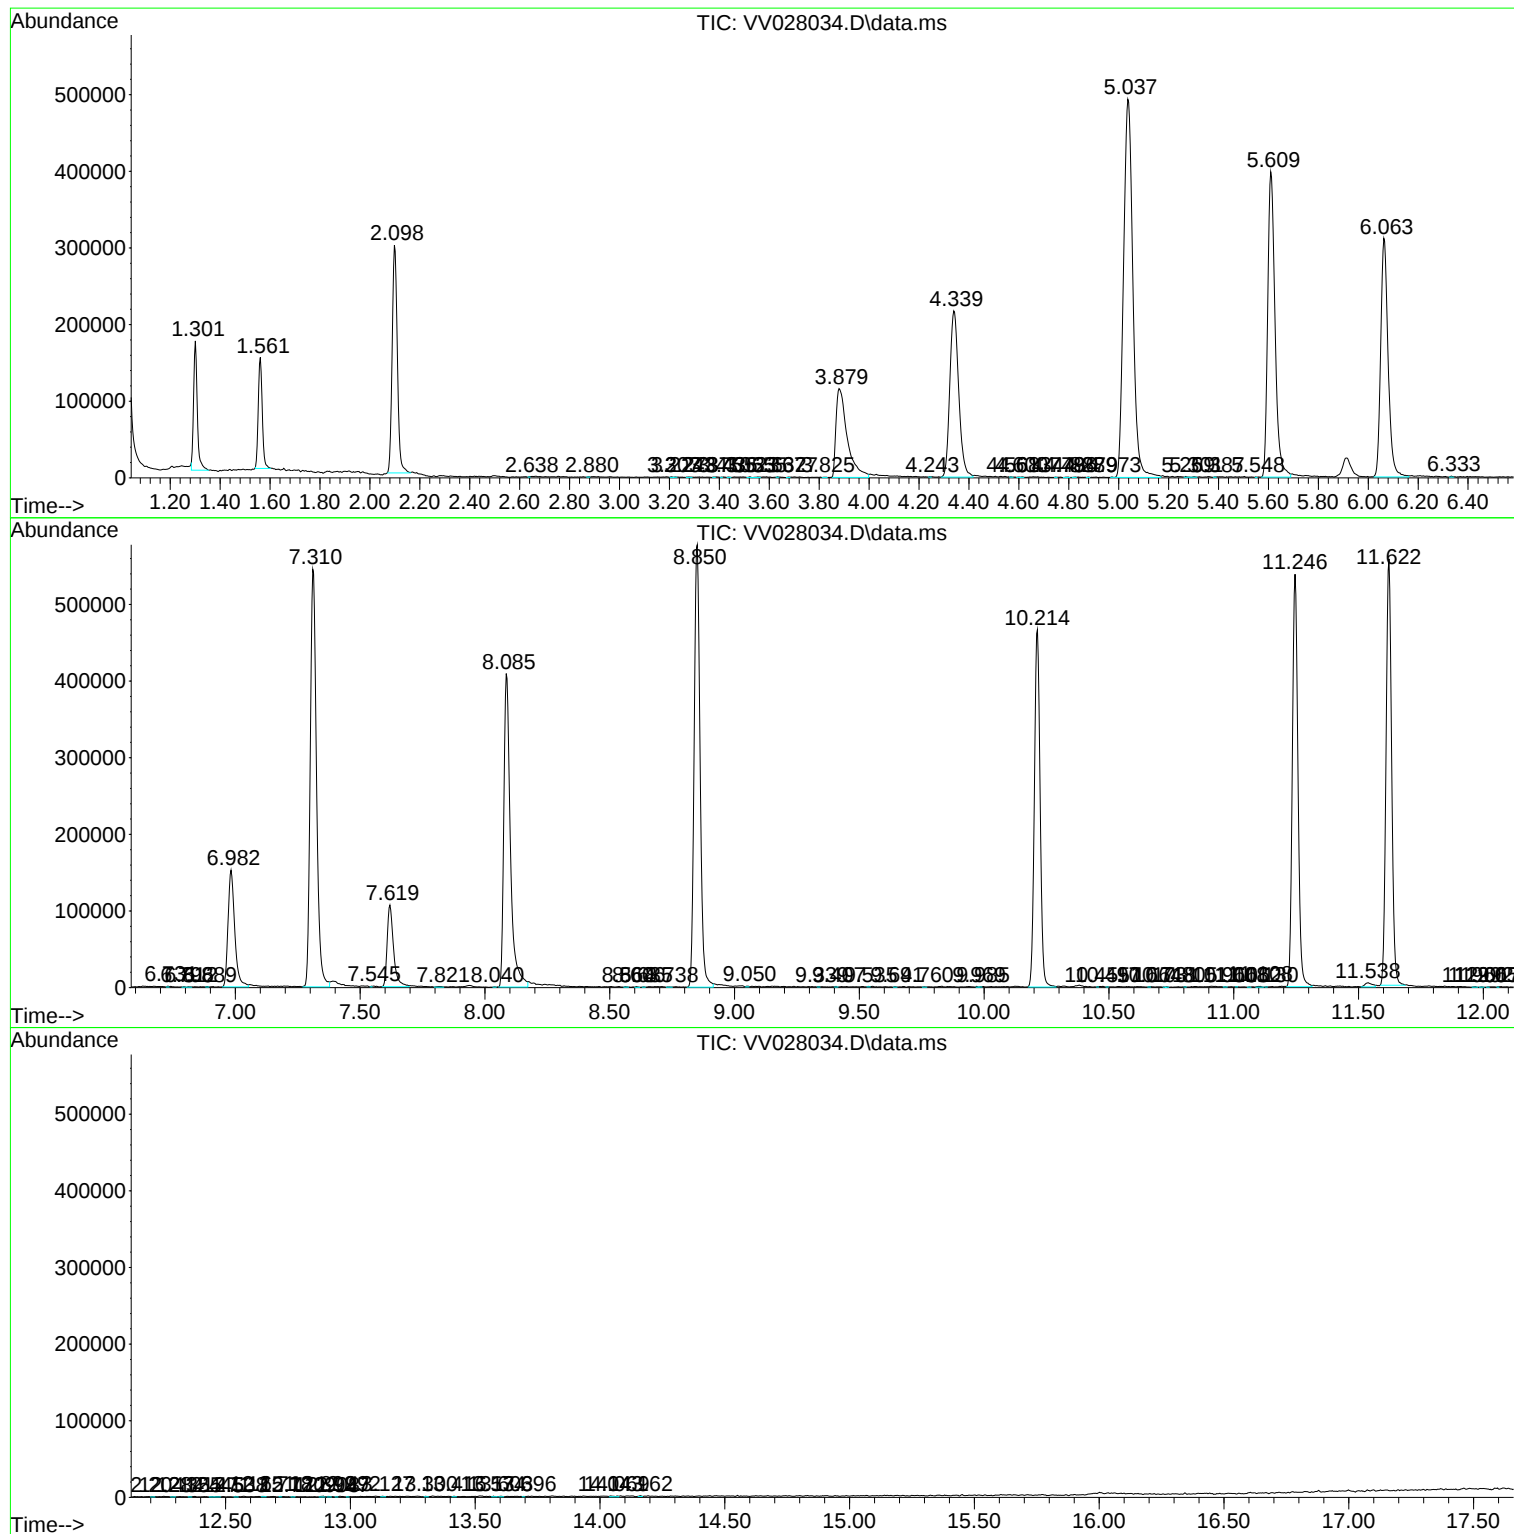

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028034.D
Acq On : 21 Sep 2022 23:24
Operator : SY/MD
Sample : N4659-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028034.D
Acq On : 21 Sep 2022 23:24
Operator : SY/MD
Sample : N4659-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc