

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028035.D
 Acq On : 21 Sep 2022 23:48
 Operator : SY/MD
 Sample : N4659-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	165525	175496	13.05%	1.712%
2	1.561	155	162	174	rBV	156378	168899	12.56%	1.648%
3	2.098	320	329	352	rVB	310115	456131	33.92%	4.451%
4	2.362	407	411	413	rBV3	843	640	0.05%	0.006%
5	2.561	468	473	479	rBV4	673	623	0.05%	0.006%
6	2.638	494	497	498	rVB3	594	319	0.02%	0.003%
7	2.767	534	537	538	rBV3	806	468	0.03%	0.005%
8	2.889	573	575	580	rVB	615	270	0.02%	0.003%
9	2.925	580	586	588	rBV3	769	784	0.06%	0.008%
10	3.063	625	629	632	rVB2	590	393	0.03%	0.004%
11	3.079	632	634	638	rVB3	612	302	0.02%	0.003%
12	3.101	638	641	642	rBV3	554	363	0.03%	0.004%
13	3.455	747	751	753	rBV3	385	247	0.02%	0.002%
14	3.468	753	755	757	rBV2	493	269	0.02%	0.003%
15	3.539	775	777	779	rBV3	575	272	0.02%	0.003%
16	3.674	817	819	822	rBV3	529	332	0.02%	0.003%
17	3.722	829	834	835	rBV	466	382	0.03%	0.004%
18	3.780	848	852	856	rVB4	738	548	0.04%	0.005%
19	3.838	866	870	871	rBV	594	448	0.03%	0.004%
20	3.883	873	884	913	rBV	128074	398129	29.61%	3.885%
21	4.339	1012	1026	1057	rVB	221707	549392	40.86%	5.361%
22	4.616	1110	1112	1116	rBV5	536	321	0.02%	0.003%
23	4.822	1172	1176	1178	rVB4	674	494	0.04%	0.005%
24	4.969	1220	1222	1226	rBV3	674	422	0.03%	0.004%
25	5.037	1226	1243	1270	rBV2	522822	1344623	100.00%	13.120%
26	5.288	1319	1321	1323	rBV2	890	444	0.03%	0.004%
27	5.539	1397	1399	1401	rBV2	533	291	0.02%	0.003%
28	5.609	1409	1421	1447	rBV	398981	807270	60.04%	7.877%
29	6.005	1541	1544	1546	rVB2	1085	577	0.04%	0.006%
30	6.063	1546	1562	1589	rBV	305568	636759	47.36%	6.213%
31	6.355	1649	1653	1654	rBV2	726	388	0.03%	0.004%
32	6.391	1662	1664	1667	rVB3	882	441	0.03%	0.004%
33	6.455	1680	1684	1685	rBV2	978	553	0.04%	0.005%
34	6.465	1685	1687	1689	rBV2	721	420	0.03%	0.004%
35	6.506	1696	1700	1702	rBV2	308	283	0.02%	0.003%
36	6.532	1706	1708	1714	rVB3	832	630	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028035.D
 Acq On : 21 Sep 2022 23:48
 Operator : SY/MD
 Sample : N4659-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.760	1776	1779	1783	rBV2	545	517	0.04%	0.005%
38	6.793	1787	1789	1794	rVV3	446	347	0.03%	0.003%
39	6.870	1809	1813	1820	rVB3	741	672	0.05%	0.007%
40	6.905	1820	1824	1826	rBV3	473	374	0.03%	0.004%
41	6.937	1830	1834	1835	rBV	509	245	0.02%	0.002%
42	6.982	1838	1848	1866	rBV	144819	264440	19.67%	2.580%
43	7.143	1895	1898	1899	rBV2	653	271	0.02%	0.003%
44	7.188	1907	1912	1913	rBV2	662	607	0.05%	0.006%
45	7.313	1939	1951	1971	rBV	542666	951865	70.79%	9.288%
46	7.619	2036	2046	2064	rBV	109558	193527	14.39%	1.888%
47	7.934	2138	2144	2148	rBV5	2410	3038	0.23%	0.030%
48	7.995	2161	2163	2165	rBV5	535	290	0.02%	0.003%
49	8.085	2182	2191	2225	rBV	459702	848169	63.08%	8.276%
50	8.622	2353	2358	2360	rBV5	802	680	0.05%	0.007%
51	8.850	2417	2429	2456	rBV	597078	984861	73.24%	9.610%
52	9.246	2548	2552	2555	rBV3	802	580	0.04%	0.006%
53	9.284	2562	2564	2571	rBV3	586	720	0.05%	0.007%
54	9.403	2597	2601	2604	rBV3	591	471	0.04%	0.005%
55	9.471	2619	2622	2624	rBV2	505	285	0.02%	0.003%
56	9.551	2640	2647	2649	rBV5	746	920	0.07%	0.009%
57	9.567	2649	2652	2654	rVV3	534	231	0.02%	0.002%
58	9.603	2661	2663	2670	rVB2	485	370	0.03%	0.004%
59	9.792	2720	2722	2727	rVB3	423	333	0.02%	0.003%
60	9.873	2744	2747	2750	rBV2	287	252	0.02%	0.002%
61	9.892	2750	2753	2756	rBV2	410	241	0.02%	0.002%
62	9.927	2761	2764	2767	rBV	343	244	0.02%	0.002%
63	10.021	2789	2793	2795	rBV2	384	340	0.03%	0.003%
64	10.091	2810	2815	2816	rBV2	359	266	0.02%	0.003%
65	10.114	2819	2822	2824	rBV	744	400	0.03%	0.004%
66	10.214	2841	2853	2873	rVV	449791	701762	52.19%	6.847%
67	10.381	2896	2905	2912	rBV6	2092	3391	0.25%	0.033%
68	10.432	2920	2921	2924	rVB	680	321	0.02%	0.003%
69	10.545	2951	2956	2957	rBV3	573	470	0.03%	0.005%
70	10.641	2984	2986	2989	rVB	446	255	0.02%	0.002%
71	10.664	2989	2993	2994	rBV2	364	253	0.02%	0.002%
72	10.751	3018	3020	3023	rBV2	490	284	0.02%	0.003%
73	10.796	3031	3034	3038	rBV3	713	414	0.03%	0.004%
74	10.837	3043	3047	3049	rVB4	405	232	0.02%	0.002%
75	10.911	3066	3070	3079	rBV6	1749	2412	0.18%	0.024%
76	11.005	3097	3099	3101	rBV	432	268	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028035.D
 Acq On : 21 Sep 2022 23:48
 Operator : SY/MD
 Sample : N4659-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.140	3139	3141	3143	rBV2	853	403	0.03%	0.004%
78	11.246	3163	3174	3192	rBV	546290	839348	62.42%	8.190%
79	11.497	3250	3252	3254	rBV2	718	299	0.02%	0.003%
80	11.509	3254	3256	3257	rBV	695	374	0.03%	0.004%
81	11.535	3257	3264	3273	rVV6	6236	10679	0.79%	0.104%
82	11.622	3280	3291	3311	rBV	552043	875098	65.08%	8.539%
83	11.873	3365	3369	3374	rBV4	769	696	0.05%	0.007%
84	12.095	3435	3438	3440	rBV2	790	446	0.03%	0.004%
85	12.124	3444	3447	3449	rBV2	1026	630	0.05%	0.006%
86	12.352	3515	3518	3521	rVB2	932	558	0.04%	0.005%
87	12.368	3521	3523	3524	rBV	821	367	0.03%	0.004%
88	12.628	3599	3604	3606	rBV2	962	744	0.06%	0.007%
89	12.670	3615	3617	3619	rBV	602	262	0.02%	0.003%
90	12.763	3642	3646	3650	rBV3	560	453	0.03%	0.004%
91	12.786	3650	3653	3655	rBV2	690	379	0.03%	0.004%
92	12.857	3672	3675	3677	rBV3	650	458	0.03%	0.004%
93	12.908	3689	3691	3694	rBV2	819	486	0.04%	0.005%
94	13.172	3769	3773	3774	rBV2	764	525	0.04%	0.005%
95	13.326	3819	3821	3826	rBV4	531	301	0.02%	0.003%
96	13.426	3849	3852	3855	rBV3	688	502	0.04%	0.005%
97	13.561	3890	3894	3897	rBV3	554	422	0.03%	0.004%
98	13.979	4021	4024	4026	rBV2	493	304	0.02%	0.003%
99	14.078	4053	4055	4056	rBV	853	376	0.03%	0.004%
100	15.210	4405	4407	4408	rBV3	848	288	0.02%	0.003%




Sum of corrected areas: 10248639

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028035.D
Acq On : 21 Sep 2022 23:48
Operator : SY/MD
Sample : N4659-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

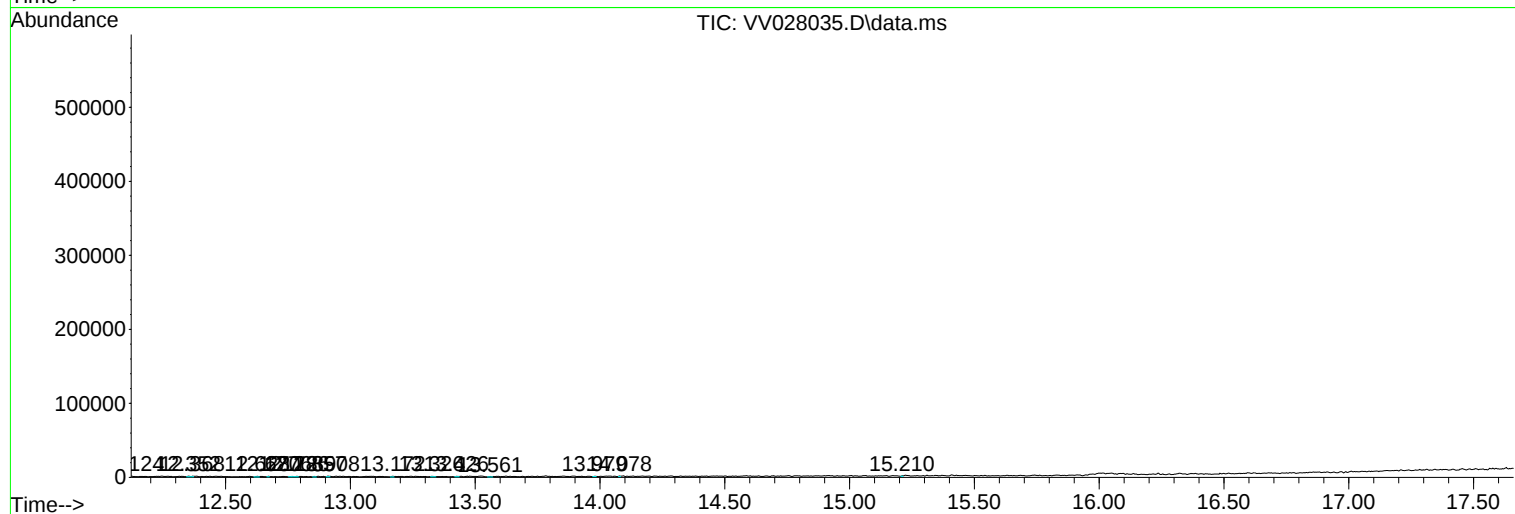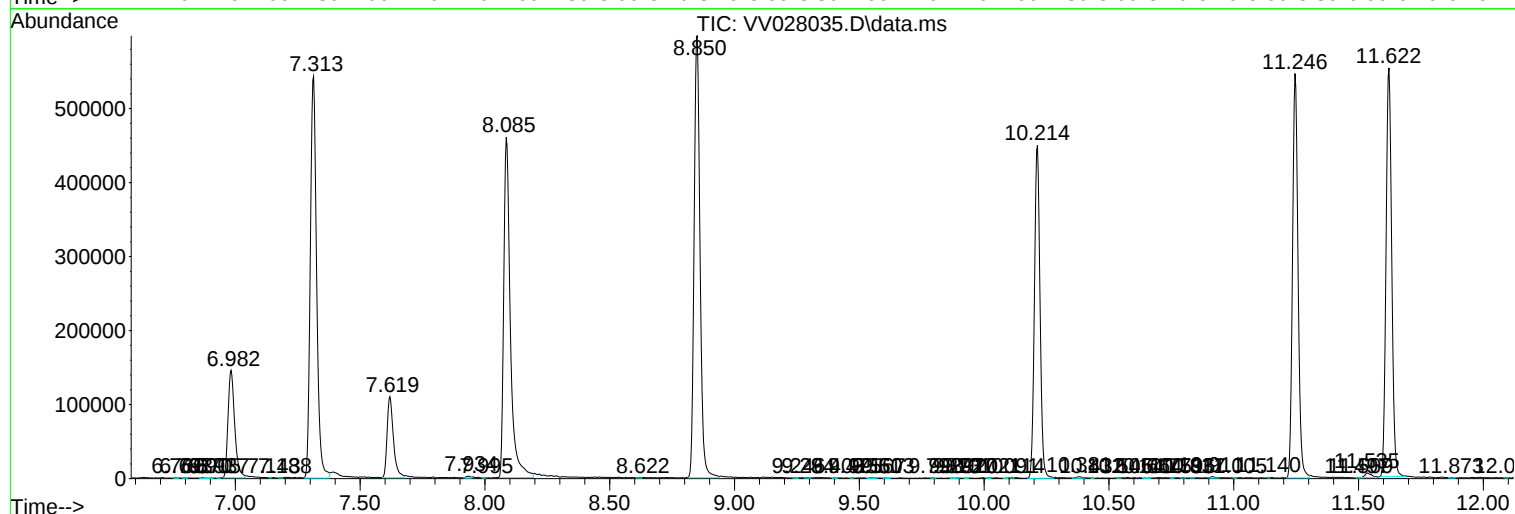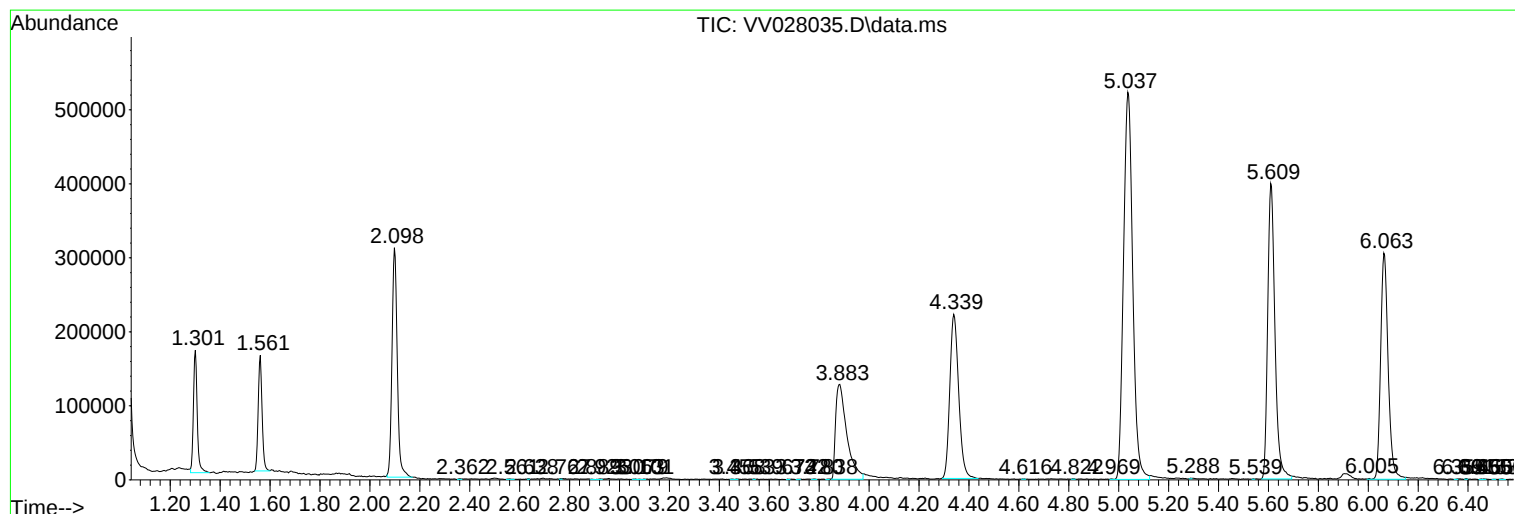

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028035.D
Acq On : 21 Sep 2022 23:48
Operator : SY/MD
Sample : N4659-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028035.D
Acq On : 21 Sep 2022 23:48
Operator : SY/MD
Sample : N4659-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc