

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028036.D
 Acq On : 22 Sep 2022 00:13
 Operator : SY/MD
 Sample : N4659-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	101	rVB	167623	175936	6.89%	1.356%
2	1.561	156	162	176	rVB	149983	168050	6.58%	1.295%
3	2.101	320	330	347	rBV3	362988	580959	22.75%	4.477%
4	2.490	447	451	452	rBV3	1800	1238	0.05%	0.010%
5	2.828	552	556	560	rBV5	608	623	0.02%	0.005%
6	2.908	579	581	585	rVB3	679	361	0.01%	0.003%
7	2.957	591	596	604	rVB4	756	1018	0.04%	0.008%
8	3.082	633	635	638	rBV3	618	363	0.01%	0.003%
9	3.188	659	668	675	rBV7	2466	4013	0.16%	0.031%
10	3.294	695	701	702	rBV2	502	398	0.02%	0.003%
11	3.336	712	714	718	rVB	693	372	0.01%	0.003%
12	3.388	727	730	734	rBV2	402	350	0.01%	0.003%
13	3.445	745	748	749	rBV3	791	401	0.02%	0.003%
14	3.654	810	813	818	rBV4	443	327	0.01%	0.003%
15	3.696	823	826	828	rBV2	534	328	0.01%	0.003%
16	3.886	873	885	926	rBV3	133156	457675	17.92%	3.527%
17	4.339	1011	1026	1050	rBV	218724	536104	20.99%	4.132%
18	4.603	1094	1108	1125	rVB3	36031	90514	3.54%	0.698%
19	4.683	1132	1133	1139	rVB5	724	485	0.02%	0.004%
20	4.738	1147	1150	1155	rVB5	735	652	0.03%	0.005%
21	4.767	1155	1159	1162	rBV3	890	545	0.02%	0.004%
22	4.828	1174	1178	1179	rBV2	457	312	0.01%	0.002%
23	4.924	1204	1208	1210	rBV3	714	436	0.02%	0.003%
24	4.944	1211	1214	1217	rVV4	785	496	0.02%	0.004%
25	5.037	1227	1243	1270	rBV2	516515	1330733	52.11%	10.256%
26	5.609	1410	1421	1452	rBV	394996	810890	31.76%	6.250%
27	5.905	1500	1513	1543	rBV	1319546	2553554	100.00%	19.680%
28	6.063	1551	1562	1592	rVB	310257	630663	24.70%	4.861%
29	6.516	1698	1703	1706	rBV4	1133	1101	0.04%	0.008%
30	6.551	1710	1714	1716	rVV3	694	461	0.02%	0.004%
31	6.641	1736	1742	1745	rBV3	945	924	0.04%	0.007%
32	6.863	1807	1811	1813	rBV	513	360	0.01%	0.003%
33	6.982	1837	1848	1866	rBV	145476	265191	10.39%	2.044%
34	7.204	1915	1917	1921	rVB5	1739	910	0.04%	0.007%
35	7.223	1921	1923	1927	rBV5	624	382	0.01%	0.003%
36	7.310	1939	1950	1969	rBV	520765	916907	35.91%	7.067%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028036.D
 Acq On : 22 Sep 2022 00:13
 Operator : SY/MD
 Sample : N4659-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	7.619	2036	2046	2062	rBV	107230	192106	7.52%	1.481%
38	7.937	2137	2145	2152	rBV5	3179	5169	0.20%	0.040%
39	8.014	2165	2169	2172	rBV3	810	877	0.03%	0.007%
40	8.085	2182	2191	2222	rBV	427002	797085	31.21%	6.143%
41	8.706	2382	2384	2386	rBV3	593	371	0.01%	0.003%
42	8.847	2417	2428	2455	rBV	604265	992135	38.85%	7.646%
43	9.146	2514	2521	2525	rBV8	1228	1725	0.07%	0.013%
44	9.201	2534	2538	2543	rBV4	792	919	0.04%	0.007%
45	9.246	2550	2552	2555	rVB2	664	342	0.01%	0.003%
46	9.310	2570	2572	2574	rBV	555	312	0.01%	0.002%
47	9.333	2577	2579	2582	rVB3	615	331	0.01%	0.003%
48	9.413	2602	2604	2608	rBV2	866	578	0.02%	0.004%
49	9.474	2622	2623	2627	rVB	644	344	0.01%	0.003%
50	9.493	2627	2629	2631	rBV2	618	308	0.01%	0.002%
51	9.596	2657	2661	2666	rVB6	854	724	0.03%	0.006%
52	9.644	2674	2676	2681	rBV3	441	363	0.01%	0.003%
53	9.725	2698	2701	2702	rBV3	698	412	0.02%	0.003%
54	9.751	2706	2709	2712	rVB3	978	598	0.02%	0.005%
55	9.792	2716	2722	2724	rBV3	627	609	0.02%	0.005%
56	9.808	2725	2727	2731	rVB	931	412	0.02%	0.003%
57	9.831	2731	2734	2735	rBV2	602	307	0.01%	0.002%
58	10.066	2802	2807	2812	rVV5	865	996	0.04%	0.008%
59	10.124	2818	2825	2834	rBV7	1923	2616	0.10%	0.020%
60	10.210	2841	2852	2872	rBV	461452	737363	28.88%	5.683%
61	10.384	2901	2906	2914	rVB6	3128	4042	0.16%	0.031%
62	10.490	2937	2939	2944	rBV4	839	450	0.02%	0.003%
63	10.570	2962	2964	2965	rBV	764	312	0.01%	0.002%
64	10.667	2985	2994	2997	rBV5	841	961	0.04%	0.007%
65	10.712	3007	3008	3013	rBV2	390	370	0.01%	0.003%
66	10.738	3014	3016	3019	rVB	801	416	0.02%	0.003%
67	10.767	3019	3025	3028	rVB2	715	556	0.02%	0.004%
68	10.831	3042	3045	3052	rBV6	572	652	0.03%	0.005%
69	10.873	3056	3058	3061	rBV3	497	374	0.01%	0.003%
70	11.021	3100	3104	3111	rBV4	514	525	0.02%	0.004%
71	11.146	3140	3143	3147	rVV4	627	514	0.02%	0.004%
72	11.191	3155	3157	3159	rVB2	735	373	0.01%	0.003%
73	11.246	3159	3174	3198	rBV	529411	822418	32.21%	6.338%
74	11.538	3256	3265	3278	rVV8	5544	11659	0.46%	0.090%
75	11.622	3280	3291	3313	rVV	548013	846520	33.15%	6.524%
76	11.776	3336	3339	3341	rVB2	842	402	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028036.D
 Acq On : 22 Sep 2022 00:13
 Operator : SY/MD
 Sample : N4659-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.792	3341	3344	3346	rBV3	577	333	0.01%	0.003%
78	11.853	3359	3363	3367	rBV5	600	456	0.02%	0.004%
79	11.934	3384	3388	3389	rBV3	535	361	0.01%	0.003%
80	12.014	3409	3413	3414	rBV	758	341	0.01%	0.003%
81	12.120	3443	3446	3448	rBV3	552	353	0.01%	0.003%
82	12.217	3474	3476	3479	rVB2	745	350	0.01%	0.003%
83	12.291	3493	3499	3505	rVB5	675	998	0.04%	0.008%
84	12.400	3531	3533	3538	rVB3	813	452	0.02%	0.003%
85	12.429	3538	3542	3544	rBV3	660	441	0.02%	0.003%
86	12.580	3586	3589	3590	rBV	506	328	0.01%	0.003%
87	12.747	3635	3641	3647	rBV6	802	1081	0.04%	0.008%
88	12.824	3663	3665	3668	rBV	606	398	0.02%	0.003%
89	12.927	3690	3697	3699	rBV2	787	854	0.03%	0.007%
90	13.017	3723	3725	3728	rVB3	1112	521	0.02%	0.004%
91	13.053	3730	3736	3738	rBV2	453	448	0.02%	0.003%
92	13.207	3782	3784	3787	rBV4	646	438	0.02%	0.003%
93	13.320	3817	3819	3822	rBV3	680	349	0.01%	0.003%
94	13.570	3895	3897	3901	rBV3	777	567	0.02%	0.004%
95	13.641	3916	3919	3923	rBV4	768	615	0.02%	0.005%
96	13.683	3930	3932	3938	rVB3	902	630	0.02%	0.005%
97	13.828	3973	3977	3978	rBV3	756	481	0.02%	0.004%
98	14.066	4049	4051	4053	rBV	958	604	0.02%	0.005%
99	14.310	4122	4127	4132	rBV7	963	1167	0.05%	0.009%
100	14.554	4200	4203	4208	rBV2	1128	1074	0.04%	0.008%




Sum of corrected areas: 12975218

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028036.D
Acq On : 22 Sep 2022 00:13
Operator : SY/MD
Sample : N4659-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

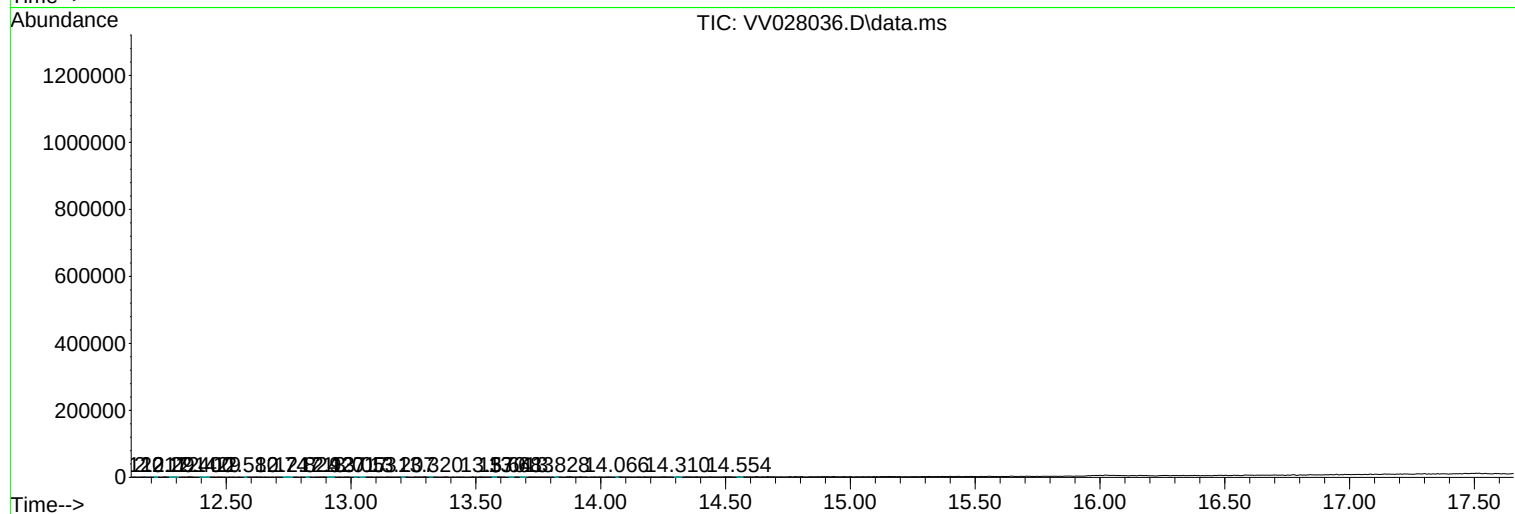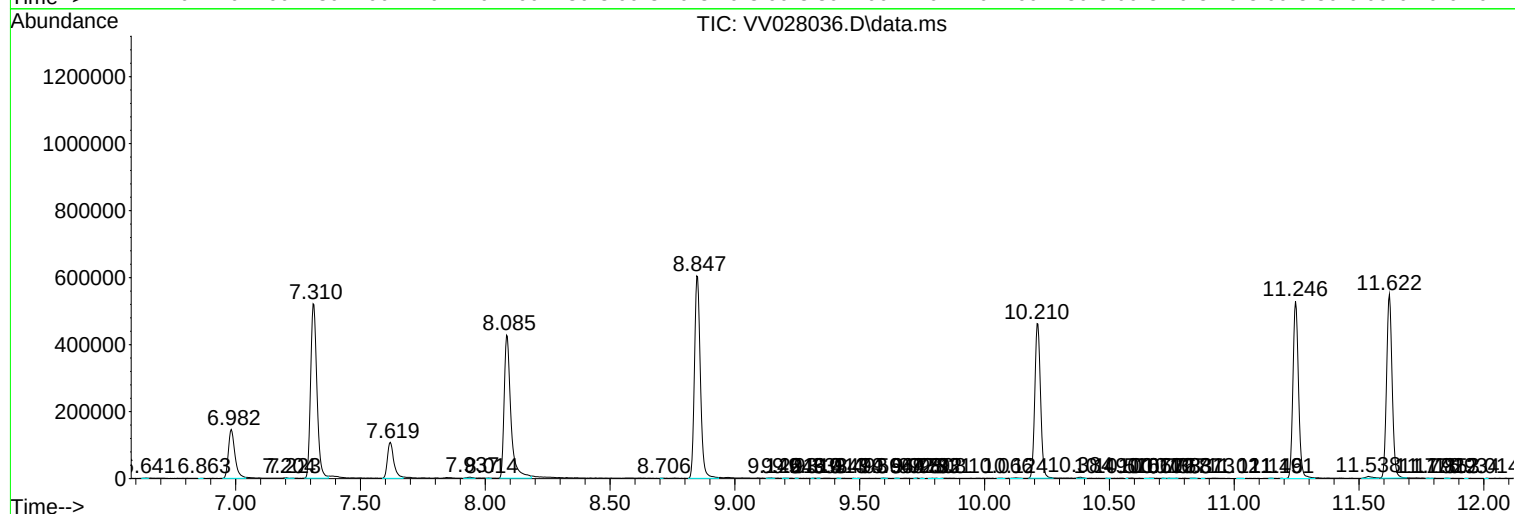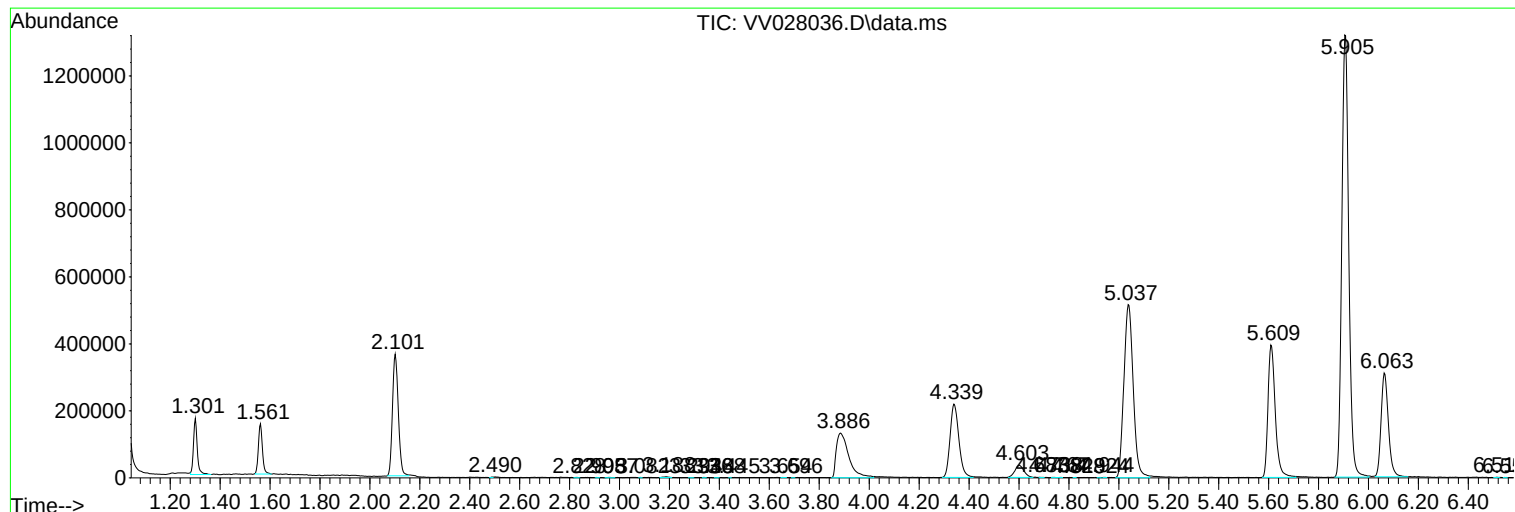

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028036.D
Acq On : 22 Sep 2022 00:13
Operator : SY/MD
Sample : N4659-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028036.D
Acq On : 22 Sep 2022 00:13
Operator : SY/MD
Sample : N4659-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc