

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028037.D
 Acq On : 22 Sep 2022 00:38
 Operator : SY/MD
 Sample : N4659-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	98	rVB	169413	180236	14.24%	1.806%
2	1.558	155	161	176	rVB	150283	171806	13.57%	1.722%
3	2.098	320	329	346	rBV	296102	432631	34.18%	4.335%
4	2.452	435	439	442	rBV4	643	488	0.04%	0.005%
5	2.500	446	454	461	rBV9	2331	3941	0.31%	0.039%
6	2.558	467	472	473	rBV	537	431	0.03%	0.004%
7	2.590	477	482	485	rBV5	549	511	0.04%	0.005%
8	2.844	557	561	563	rVV3	542	367	0.03%	0.004%
9	3.111	640	644	646	rVB2	474	241	0.02%	0.002%
10	3.166	657	661	662	rBV2	478	351	0.03%	0.004%
11	3.262	688	691	694	rVB2	582	279	0.02%	0.003%
12	3.285	694	698	702	rBV2	322	294	0.02%	0.003%
13	3.359	718	721	724	rBV2	487	304	0.02%	0.003%
14	3.375	724	726	729	rBV2	363	238	0.02%	0.002%
15	3.555	780	782	787	rVB3	443	332	0.03%	0.003%
16	3.600	794	796	799	rBV2	411	297	0.02%	0.003%
17	3.648	807	811	816	rVB3	417	493	0.04%	0.005%
18	3.680	816	821	822	rBV2	344	250	0.02%	0.003%
19	3.764	842	847	850	rBV3	489	340	0.03%	0.003%
20	3.828	862	867	869	rBV2	449	287	0.02%	0.003%
21	3.876	870	882	911	rBV	121678	346466	27.37%	3.472%
22	4.339	1011	1026	1052	rBV	218167	538673	42.56%	5.398%
23	4.648	1120	1122	1125	rVB2	536	299	0.02%	0.003%
24	4.728	1143	1147	1150	rVB3	553	408	0.03%	0.004%
25	4.802	1167	1170	1173	rBV	687	432	0.03%	0.004%
26	4.818	1173	1175	1178	rVB2	505	258	0.02%	0.003%
27	4.857	1184	1187	1189	rBV2	659	370	0.03%	0.004%
28	4.889	1193	1197	1200	rBV2	598	442	0.03%	0.004%
29	5.037	1226	1243	1271	rBV2	490500	1265748	100.00%	12.684%
30	5.301	1321	1325	1327	rBV2	498	352	0.03%	0.004%
31	5.355	1339	1342	1343	rBV	533	363	0.03%	0.004%
32	5.445	1366	1370	1371	rBV3	644	314	0.02%	0.003%
33	5.458	1372	1374	1376	rVB3	587	280	0.02%	0.003%
34	5.522	1390	1394	1398	rVB4	608	455	0.04%	0.005%
35	5.609	1409	1421	1449	rBV	390493	791012	62.49%	7.927%
36	5.905	1502	1513	1528	rVB	7525	18246	1.44%	0.183%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028037.D
 Acq On : 22 Sep 2022 00:38
 Operator : SY/MD
 Sample : N4659-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.998	1538	1542	1546	rBV3	734	770	0.06%	0.008%
38	6.063	1548	1562	1584	rBV	296379	600049	47.41%	6.013%
39	6.355	1650	1653	1656	rBV2	552	270	0.02%	0.003%
40	6.371	1656	1658	1660	rVV3	596	253	0.02%	0.003%
41	6.384	1660	1662	1664	rVV	710	265	0.02%	0.003%
42	6.420	1671	1673	1676	rVB2	855	426	0.03%	0.004%
43	6.442	1676	1680	1682	rBV2	756	532	0.04%	0.005%
44	6.455	1682	1684	1686	rVV2	631	358	0.03%	0.004%
45	6.484	1690	1693	1695	rBV	625	323	0.03%	0.003%
46	6.497	1695	1697	1700	rBV2	628	254	0.02%	0.003%
47	6.522	1700	1705	1710	rVB5	823	866	0.07%	0.009%
48	6.625	1733	1737	1741	rBV5	1206	1237	0.10%	0.012%
49	6.712	1760	1764	1767	rVB3	658	506	0.04%	0.005%
50	6.767	1779	1781	1785	rBV2	588	430	0.03%	0.004%
51	6.982	1836	1848	1875	rBV	149354	277120	21.89%	2.777%
52	7.310	1939	1950	1971	rBV	521322	920538	72.73%	9.225%
53	7.619	2036	2046	2077	rBV	104068	194013	15.33%	1.944%
54	8.027	2171	2173	2175	rVB3	874	334	0.03%	0.003%
55	8.043	2175	2178	2181	rBV2	948	838	0.07%	0.008%
56	8.085	2181	2191	2222	rBV	434947	808098	63.84%	8.098%
57	8.571	2339	2342	2344	rBV2	501	299	0.02%	0.003%
58	8.661	2369	2370	2373	rVB2	448	245	0.02%	0.002%
59	8.770	2402	2404	2406	rBV3	537	236	0.02%	0.002%
60	8.847	2416	2428	2450	rBV	593568	974789	77.01%	9.768%
61	9.223	2542	2545	2547	rBV3	1014	570	0.05%	0.006%
62	9.471	2620	2622	2625	rVB2	537	276	0.02%	0.003%
63	9.490	2626	2628	2630	rBV3	683	276	0.02%	0.003%
64	9.532	2639	2641	2645	rBV4	856	760	0.06%	0.008%
65	9.770	2713	2715	2720	rBV2	832	516	0.04%	0.005%
66	9.966	2773	2776	2778	rBV3	586	309	0.02%	0.003%
67	10.046	2799	2801	2802	rBV	492	234	0.02%	0.002%
68	10.072	2806	2809	2813	rBV3	536	394	0.03%	0.004%
69	10.165	2835	2838	2839	rBV2	538	313	0.02%	0.003%
70	10.214	2841	2853	2866	rBV	464377	733188	57.93%	7.347%
71	10.378	2898	2904	2912	rBV8	2346	3154	0.25%	0.032%
72	10.452	2923	2927	2928	rBV3	948	582	0.05%	0.006%
73	10.657	2984	2991	2993	rBV5	723	836	0.07%	0.008%
74	10.680	2996	2998	3002	rVB3	955	480	0.04%	0.005%
75	10.699	3002	3004	3007	rBV2	566	315	0.02%	0.003%
76	10.744	3015	3018	3021	rBV2	747	563	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028037.D
 Acq On : 22 Sep 2022 00:38
 Operator : SY/MD
 Sample : N4659-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.870	3055	3057	3061	rBV3	904	642	0.05%	0.006%
78	10.908	3066	3069	3070	rBV2	820	518	0.04%	0.005%
79	11.014	3100	3102	3105	rVB2	477	254	0.02%	0.003%
80	11.037	3105	3109	3112	rBV3	720	537	0.04%	0.005%
81	11.136	3137	3140	3141	rBV2	588	343	0.03%	0.003%
82	11.194	3155	3158	3162	rBV4	807	710	0.06%	0.007%
83	11.246	3163	3174	3196	rBV	527789	816107	64.48%	8.178%
84	11.535	3255	3264	3274	rBV3	11530	23174	1.83%	0.232%
85	11.622	3280	3291	3313	rVB	542241	845002	66.76%	8.468%
86	11.998	3406	3408	3411	rBV3	619	372	0.03%	0.004%
87	12.191	3465	3468	3470	rBV3	729	444	0.04%	0.004%
88	12.275	3491	3494	3496	rBV2	856	471	0.04%	0.005%
89	12.307	3502	3504	3507	rBV3	450	283	0.02%	0.003%
90	12.702	3624	3627	3628	rBV3	857	473	0.04%	0.005%
91	13.005	3718	3721	3723	rBV	766	471	0.04%	0.005%
92	13.033	3726	3730	3731	rBV	562	425	0.03%	0.004%
93	13.075	3736	3743	3746	rBV4	760	812	0.06%	0.008%
94	13.271	3802	3804	3808	rVB	690	402	0.03%	0.004%
95	13.490	3870	3872	3876	rBV3	789	470	0.04%	0.005%
96	13.564	3893	3895	3898	rBV3	585	420	0.03%	0.004%
97	13.889	3994	3996	3999	rBV2	770	476	0.04%	0.005%
98	14.101	4060	4062	4066	rBV2	643	433	0.03%	0.004%
99	14.660	4232	4236	4240	rBV5	1044	1171	0.09%	0.012%
100	14.956	4326	4328	4330	rBV2	908	519	0.04%	0.005%




Sum of corrected areas: 9978979

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028037.D
Acq On : 22 Sep 2022 00:38
Operator : SY/MD
Sample : N4659-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

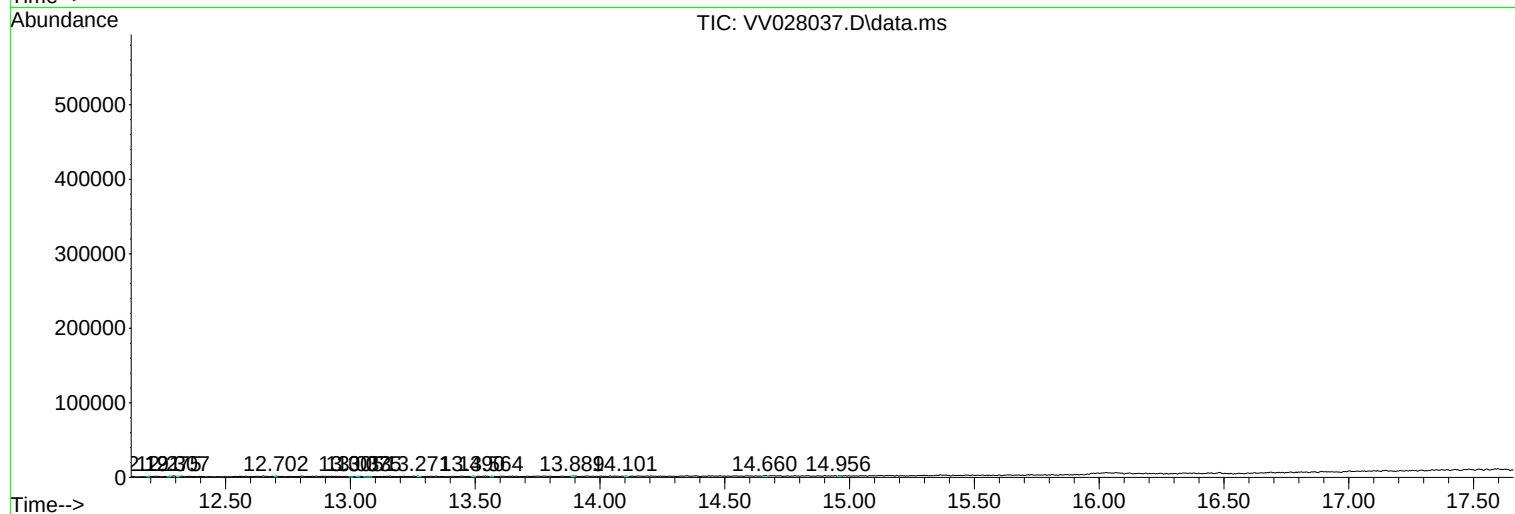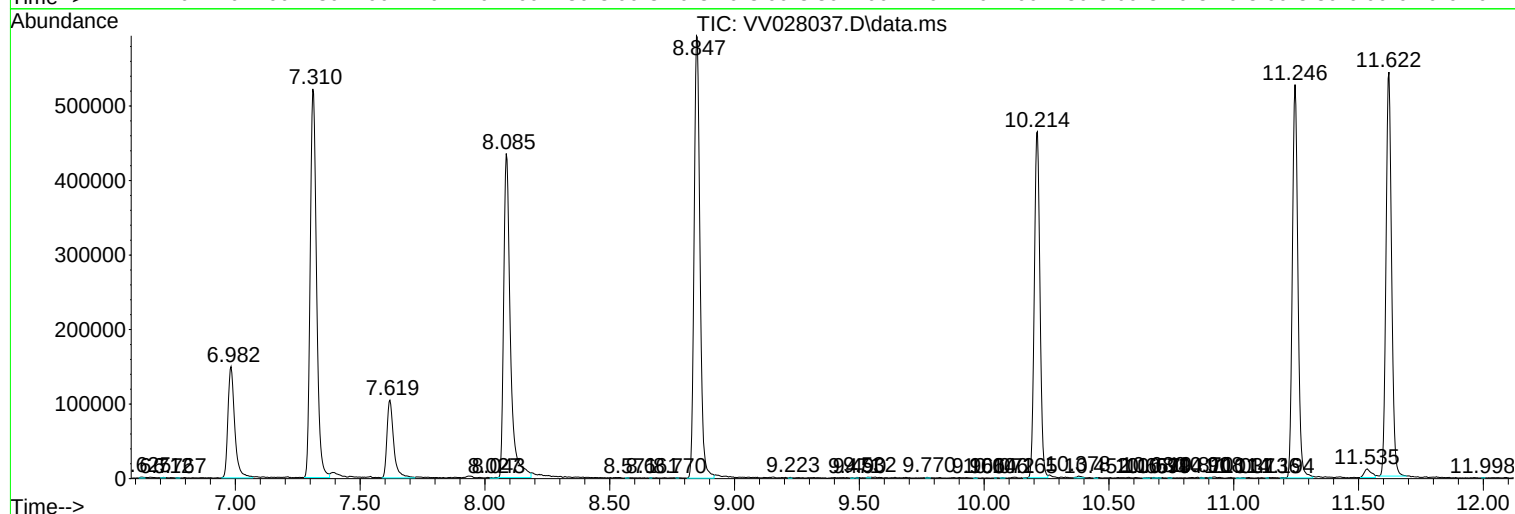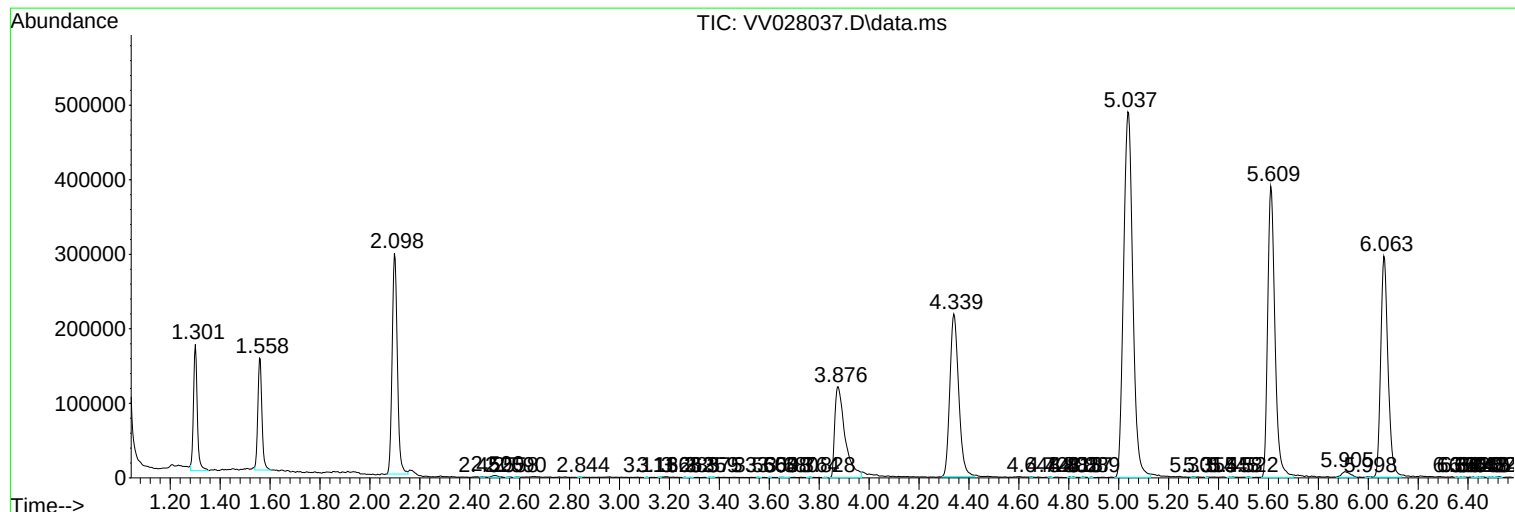

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028037.D
Acq On : 22 Sep 2022 00:38
Operator : SY/MD
Sample : N4659-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028037.D
Acq On : 22 Sep 2022 00:38
Operator : SY/MD
Sample : N4659-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc