

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028038.D
 Acq On : 22 Sep 2022 01:03
 Operator : SY/MD
 Sample : N4659-06DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E62DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	159653	168323	13.34%	1.608%
2	1.561	156	162	173	rVB	141005	154539	12.25%	1.477%
3	2.101	320	330	348	rBV2	291294	439456	34.82%	4.199%
4	2.355	407	409	412	rBV4	558	312	0.02%	0.003%
5	2.683	509	511	514	rBV3	522	203	0.02%	0.002%
6	2.902	577	579	582	rBV2	286	129	0.01%	0.001%
7	2.921	582	585	587	rBV2	983	590	0.05%	0.006%
8	3.024	614	617	620	rBV3	723	461	0.04%	0.004%
9	3.114	640	645	646	rBV3	498	373	0.03%	0.004%
10	3.150	654	656	657	rBV	405	130	0.01%	0.001%
11	3.182	661	666	671	rVV5	1154	1482	0.12%	0.014%
12	3.336	708	714	715	rBV3	556	468	0.04%	0.004%
13	3.346	715	717	718	rBV	387	118	0.01%	0.001%
14	3.355	718	720	721	rBV	538	200	0.02%	0.002%
15	3.426	740	742	744	rBV2	458	187	0.01%	0.002%
16	3.468	752	755	756	rBV	438	234	0.02%	0.002%
17	3.507	766	767	768	rBV	516	151	0.01%	0.001%
18	3.558	781	783	786	rBV3	360	156	0.01%	0.001%
19	3.577	786	789	793	rBV4	357	337	0.03%	0.003%
20	3.699	824	827	828	rVB2	396	143	0.01%	0.001%
21	3.754	843	844	845	rVB2	482	93	0.01%	0.001%
22	3.773	846	850	854	rBV4	597	531	0.04%	0.005%
23	3.809	859	861	864	rBV2	595	320	0.03%	0.003%
24	3.899	873	889	925	rBV3	281754	908720	72.01%	8.684%
25	4.339	1009	1026	1051	rBV2	221652	551432	43.70%	5.269%
26	4.600	1097	1107	1122	rVB3	9105	22390	1.77%	0.214%
27	4.744	1148	1152	1153	rBV2	978	534	0.04%	0.005%
28	4.950	1214	1216	1220	rBV2	535	255	0.02%	0.002%
29	5.040	1227	1244	1266	rBV2	491929	1261968	100.00%	12.059%
30	5.410	1357	1359	1360	rBV2	697	268	0.02%	0.003%
31	5.445	1368	1370	1374	rVB4	721	379	0.03%	0.004%
32	5.468	1374	1377	1378	rBV3	413	202	0.02%	0.002%
33	5.609	1407	1421	1442	rBV	408406	832529	65.97%	7.956%
34	5.860	1497	1499	1500	rBV2	870	348	0.03%	0.003%
35	5.992	1537	1540	1543	rBV5	1067	788	0.06%	0.008%
36	6.063	1549	1562	1589	rBV	290781	599112	47.47%	5.725%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028038.D
 Acq On : 22 Sep 2022 01:03
 Operator : SY/MD
 Sample : N4659-06DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E62DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.481	1691	1692	1695	rBB2	497	207	0.02%	0.002%
38	6.503	1695	1699	1703	rBV2	888	867	0.07%	0.008%
39	6.619	1733	1735	1736	rBV2	941	378	0.03%	0.004%
40	6.664	1747	1749	1753	rBV3	1341	955	0.08%	0.009%
41	6.805	1791	1793	1797	rVB2	715	374	0.03%	0.004%
42	6.831	1797	1801	1804	rBV4	659	606	0.05%	0.006%
43	6.889	1816	1819	1820	rBV2	303	106	0.01%	0.001%
44	6.902	1821	1823	1826	rBV4	587	371	0.03%	0.004%
45	6.982	1834	1848	1869	rBV2	133972	255087	20.21%	2.438%
46	7.162	1901	1904	1906	rBV2	610	374	0.03%	0.004%
47	7.252	1930	1932	1936	rBV4	744	600	0.05%	0.006%
48	7.310	1939	1950	1971	rBV	499980	872022	69.10%	8.333%
49	7.619	2036	2046	2071	rBV	100050	184055	14.58%	1.759%
50	7.812	2104	2106	2108	rBV2	699	262	0.02%	0.003%
51	7.863	2121	2122	2129	rVB4	927	998	0.08%	0.010%
52	7.924	2137	2141	2143	rBV5	1539	1293	0.10%	0.012%
53	8.085	2182	2191	2223	rBV	406978	766328	60.72%	7.323%
54	8.567	2339	2341	2343	rBV2	526	319	0.03%	0.003%
55	8.609	2352	2354	2357	rBV3	735	369	0.03%	0.004%
56	8.725	2388	2390	2392	rBV2	552	329	0.03%	0.003%
57	8.847	2417	2428	2461	rBV	628482	1031061	81.70%	9.853%
58	9.227	2544	2546	2548	rBV	396	173	0.01%	0.002%
59	9.339	2578	2581	2586	rBV5	825	742	0.06%	0.007%
60	9.381	2590	2594	2598	rBV3	792	777	0.06%	0.007%
61	9.516	2632	2636	2640	rBV5	662	629	0.05%	0.006%
62	9.654	2677	2679	2681	rBV2	324	173	0.01%	0.002%
63	9.706	2693	2695	2696	rBV2	401	112	0.01%	0.001%
64	9.841	2735	2737	2742	rVB3	1048	583	0.05%	0.006%
65	9.870	2742	2746	2751	rBV4	1178	1408	0.11%	0.013%
66	9.937	2764	2767	2769	rBV2	615	366	0.03%	0.003%
67	10.056	2802	2804	2805	rBV	431	189	0.01%	0.002%
68	10.214	2839	2853	2873	rBV	442126	703637	55.76%	6.724%
69	10.365	2897	2900	2901	rBV3	646	359	0.03%	0.003%
70	10.484	2933	2937	2941	rBV3	685	601	0.05%	0.006%
71	10.661	2988	2992	2996	rBV3	1242	1151	0.09%	0.011%
72	10.709	3006	3007	3011	rBV2	567	321	0.03%	0.003%
73	10.837	3044	3047	3050	rBV3	738	510	0.04%	0.005%
74	10.911	3066	3070	3071	rBV2	1565	1138	0.09%	0.011%
75	11.001	3096	3098	3101	rVB4	799	413	0.03%	0.004%
76	11.063	3114	3117	3118	rBV	357	220	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028038.D
 Acq On : 22 Sep 2022 01:03
 Operator : SY/MD
 Sample : N4659-06DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E62DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.178	3151	3153	3154	rVB	370	103	0.01%	0.001%
78	11.188	3154	3156	3158	rBV3	462	264	0.02%	0.003%
79	11.246	3162	3174	3197	rBV	561973	851241	67.45%	8.134%
80	11.535	3256	3264	3279	rBV5	7389	16161	1.28%	0.154%
81	11.622	3280	3291	3311	rVV	513096	811340	64.29%	7.753%
82	11.924	3381	3385	3387	rBV4	838	666	0.05%	0.006%
83	11.960	3395	3396	3398	rBV4	371	113	0.01%	0.001%
84	12.059	3423	3427	3429	rBV3	548	381	0.03%	0.004%
85	12.143	3450	3453	3455	rBV2	464	310	0.02%	0.003%
86	12.252	3484	3487	3492	rVB3	781	764	0.06%	0.007%
87	12.313	3504	3506	3509	rBV2	518	359	0.03%	0.003%
88	12.349	3515	3517	3519	rBV2	749	491	0.04%	0.005%
89	12.850	3671	3673	3676	rVB2	912	509	0.04%	0.005%
90	12.943	3700	3702	3703	rBV	587	197	0.02%	0.002%
91	13.188	3776	3778	3782	rVB5	893	572	0.05%	0.005%
92	13.210	3782	3785	3787	rBV2	944	638	0.05%	0.006%
93	13.458	3860	3862	3864	rBV2	621	250	0.02%	0.002%
94	13.506	3869	3877	3879	rBV4	1041	1094	0.09%	0.010%
95	13.699	3936	3937	3939	rBV4	534	247	0.02%	0.002%
96	13.927	4004	4008	4011	rBV4	764	772	0.06%	0.007%




Sum of corrected areas: 10464796

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028038.D
Acq On : 22 Sep 2022 01:03
Operator : SY/MD
Sample : N4659-06DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E62DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

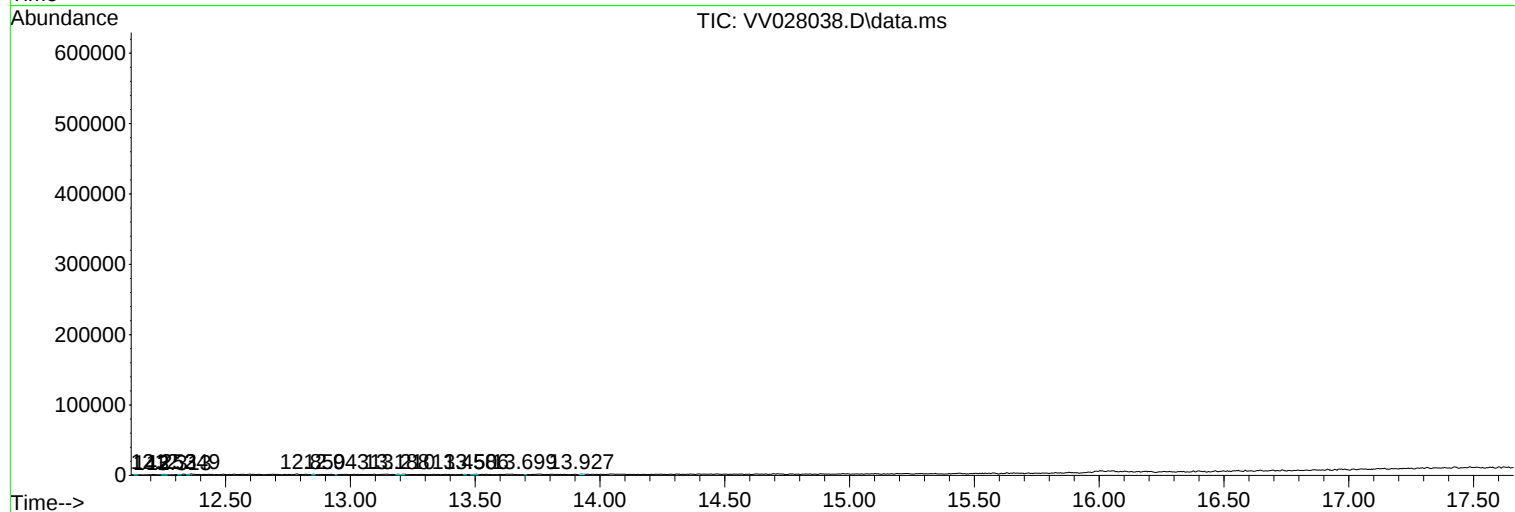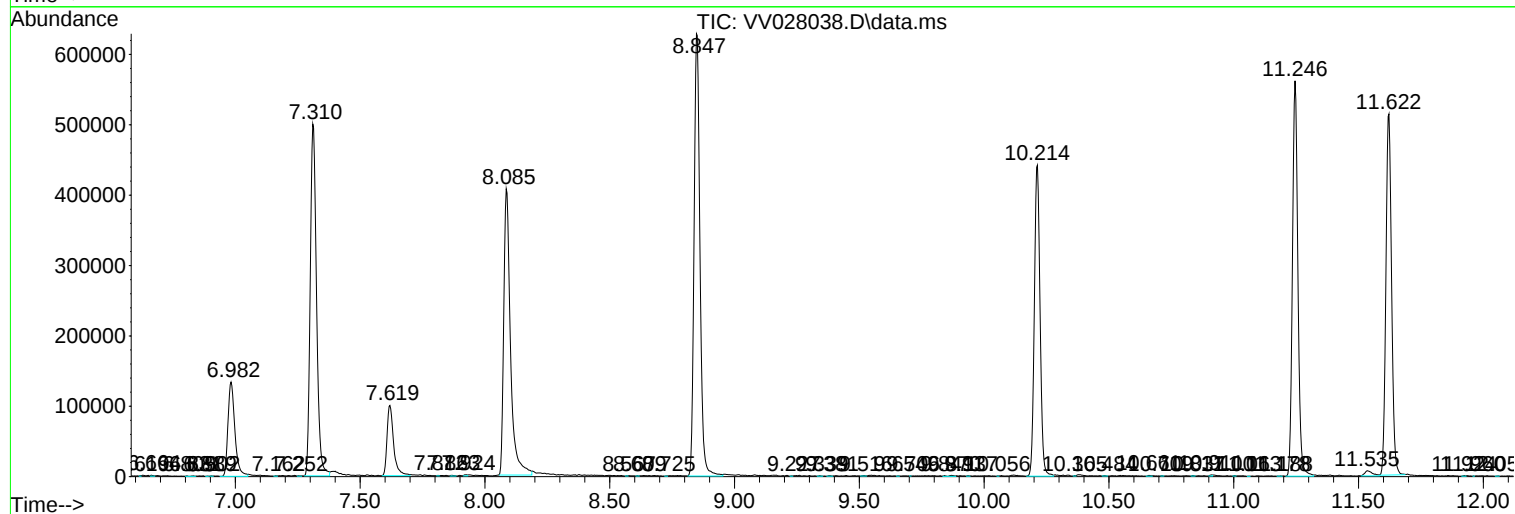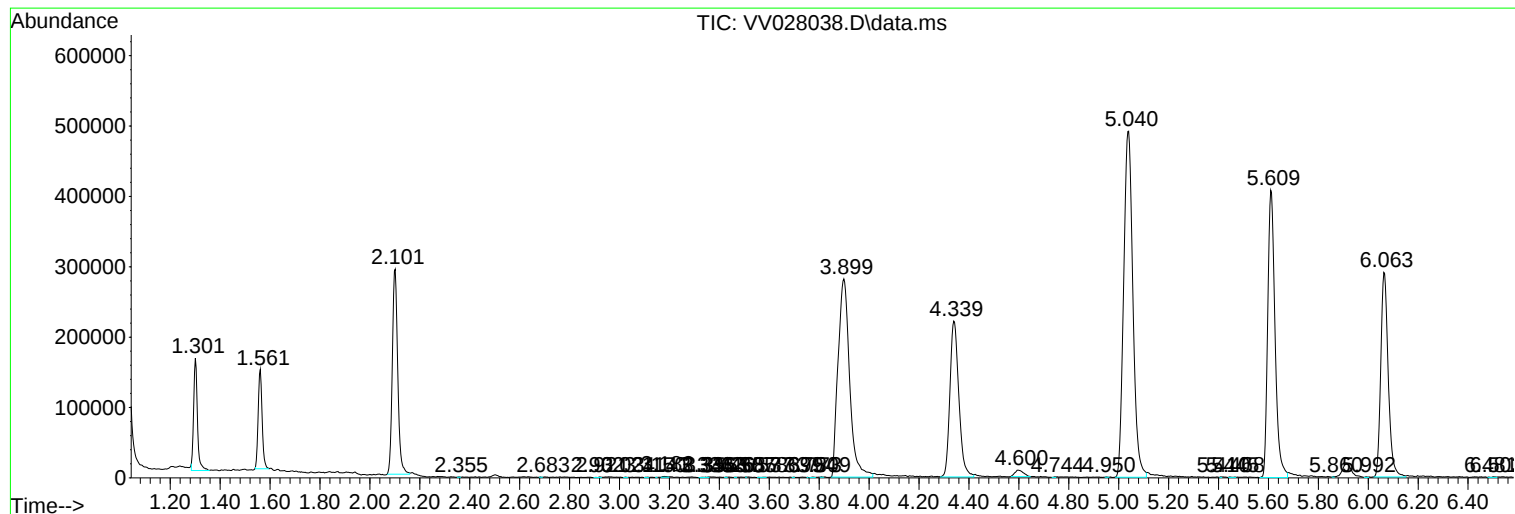

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028038.D
Acq On : 22 Sep 2022 01:03
Operator : SY/MD
Sample : N4659-06DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E62DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028038.D
Acq On : 22 Sep 2022 01:03
Operator : SY/MD
Sample : N4659-06DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E62DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc