

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028039.D
 Acq On : 22 Sep 2022 01:28
 Operator : SY/MD
 Sample : N4659-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	97	rVB	164120	168854	13.44%	1.692%
2	1.561	156	162	172	rVB	148414	163214	12.99%	1.635%
3	2.101	320	330	345	rBV	298284	438520	34.90%	4.393%
4	2.494	448	452	453	rBV3	1186	848	0.07%	0.008%
5	2.593	478	483	485	rBV2	669	471	0.04%	0.005%
6	2.635	489	496	497	rBV3	693	518	0.04%	0.005%
7	2.760	530	535	547	rVB6	804	1388	0.11%	0.014%
8	2.815	547	552	553	rBV2	447	273	0.02%	0.003%
9	2.876	568	571	576	rVB3	744	552	0.04%	0.006%
10	2.915	576	583	584	rBV3	557	359	0.03%	0.004%
11	2.937	588	590	592	rBV3	490	250	0.02%	0.003%
12	3.159	656	659	661	rBV	359	255	0.02%	0.003%
13	3.268	691	693	698	rBV3	315	313	0.02%	0.003%
14	3.378	724	727	731	rVB3	417	259	0.02%	0.003%
15	3.442	744	747	751	rBV2	393	274	0.02%	0.003%
16	3.699	825	827	832	rVV	370	364	0.03%	0.004%
17	3.754	841	844	850	rVB2	337	260	0.02%	0.003%
18	3.879	870	883	912	rBV	120486	354749	28.23%	3.554%
19	4.339	1011	1026	1056	rBV	213640	531167	42.27%	5.322%
20	4.645	1119	1121	1126	rVB3	678	497	0.04%	0.005%
21	4.674	1126	1130	1132	rBV3	436	314	0.02%	0.003%
22	4.719	1142	1144	1147	rBV3	464	305	0.02%	0.003%
23	4.738	1147	1150	1152	rVV	537	321	0.03%	0.003%
24	4.767	1156	1159	1163	rVV2	520	461	0.04%	0.005%
25	4.789	1164	1166	1171	rVV3	580	484	0.04%	0.005%
26	4.812	1171	1173	1177	rVV3	783	507	0.04%	0.005%
27	4.889	1195	1197	1201	rBV3	417	262	0.02%	0.003%
28	4.912	1201	1204	1208	rVB3	571	383	0.03%	0.004%
29	4.934	1208	1211	1214	rBV2	411	315	0.03%	0.003%
30	5.040	1226	1244	1269	rBV2	485961	1256668	100.00%	12.590%
31	5.339	1335	1337	1342	rVB2	841	411	0.03%	0.004%
32	5.358	1342	1343	1348	rVB4	479	309	0.02%	0.003%
33	5.609	1408	1421	1449	rBV	400748	811015	64.54%	8.125%
34	5.773	1470	1472	1473	rBV	852	301	0.02%	0.003%
35	5.908	1505	1514	1524	rBV10	5967	10574	0.84%	0.106%
36	5.973	1530	1534	1536	rBV3	638	466	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028039.D
 Acq On : 22 Sep 2022 01:28
 Operator : SY/MD
 Sample : N4659-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.008	1543	1545	1547	rBV2	494	256	0.02%	0.003%
38	6.063	1548	1562	1587	rVV	283722	586757	46.69%	5.879%
39	6.262	1622	1624	1631	rVB4	1180	990	0.08%	0.010%
40	6.310	1635	1639	1641	rBV2	547	410	0.03%	0.004%
41	6.355	1649	1653	1657	rBV4	928	723	0.06%	0.007%
42	6.407	1665	1669	1672	rBV5	361	378	0.03%	0.004%
43	6.448	1680	1682	1685	rVB2	485	250	0.02%	0.003%
44	6.474	1687	1690	1693	rVV3	356	240	0.02%	0.002%
45	6.564	1714	1718	1720	rBV	541	403	0.03%	0.004%
46	6.616	1732	1734	1735	rBV	447	248	0.02%	0.002%
47	6.789	1785	1788	1791	rBV3	445	278	0.02%	0.003%
48	6.809	1791	1794	1797	rVV	389	267	0.02%	0.003%
49	6.834	1800	1802	1806	rBV3	783	456	0.04%	0.005%
50	6.879	1813	1816	1819	rVB3	434	271	0.02%	0.003%
51	6.921	1827	1829	1832	rVB2	461	285	0.02%	0.003%
52	6.982	1833	1848	1868	rBV	143800	264928	21.08%	2.654%
53	7.165	1902	1905	1906	rBV2	568	305	0.02%	0.003%
54	7.191	1911	1913	1915	rBV2	993	561	0.04%	0.006%
55	7.243	1926	1929	1933	rBV3	890	921	0.07%	0.009%
56	7.310	1939	1950	1972	rBV	522459	919689	73.18%	9.214%
57	7.619	2036	2046	2072	rBV	105070	188632	15.01%	1.890%
58	7.854	2115	2119	2121	rBV4	825	586	0.05%	0.006%
59	7.889	2128	2130	2134	rBV4	721	521	0.04%	0.005%
60	7.937	2137	2145	2152	rBV8	2306	4195	0.33%	0.042%
61	8.085	2181	2191	2230	rBV	438259	815534	64.90%	8.171%
62	8.580	2341	2345	2346	rBV3	671	349	0.03%	0.003%
63	8.606	2350	2353	2356	rBV4	861	545	0.04%	0.005%
64	8.760	2399	2401	2407	rVB4	733	543	0.04%	0.005%
65	8.847	2416	2428	2451	rBV	604376	987272	78.56%	9.891%
66	9.249	2551	2553	2557	rVB3	626	416	0.03%	0.004%
67	9.275	2557	2561	2563	rBV5	782	644	0.05%	0.006%
68	9.333	2577	2579	2581	rBV2	666	308	0.02%	0.003%
69	9.426	2604	2608	2610	rVB4	917	635	0.05%	0.006%
70	9.596	2658	2661	2663	rBV	1023	446	0.04%	0.004%
71	9.702	2691	2694	2695	rBV2	576	368	0.03%	0.004%
72	9.763	2711	2713	2715	rBV	498	337	0.03%	0.003%
73	9.799	2719	2724	2726	rBV3	638	666	0.05%	0.007%
74	9.915	2756	2760	2763	rBV2	848	672	0.05%	0.007%
75	10.027	2792	2795	2798	rVV3	485	311	0.02%	0.003%
76	10.056	2802	2804	2807	rBV2	676	427	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028039.D
 Acq On : 22 Sep 2022 01:28
 Operator : SY/MD
 Sample : N4659-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.114	2819	2822	2824	rBV4	949	685	0.05%	0.007%
78	10.214	2841	2853	2869	rBV	472044	731215	58.19%	7.326%
79	10.567	2961	2963	2965	rBV	459	283	0.02%	0.003%
80	10.725	3009	3012	3014	rBV2	470	284	0.02%	0.003%
81	10.841	3044	3048	3049	rBV4	554	350	0.03%	0.004%
82	11.085	3122	3124	3129	rBV	679	427	0.03%	0.004%
83	11.172	3149	3151	3154	rBV4	569	307	0.02%	0.003%
84	11.246	3163	3174	3193	rBV	554634	856028	68.12%	8.576%
85	11.419	3227	3228	3230	rBV2	710	270	0.02%	0.003%
86	11.477	3242	3246	3247	rBV2	751	514	0.04%	0.005%
87	11.538	3258	3265	3277	rBV6	4463	8931	0.71%	0.089%
88	11.622	3280	3291	3313	rVB	541350	848051	67.48%	8.497%
89	12.053	3423	3425	3428	rVB2	640	329	0.03%	0.003%
90	12.075	3430	3432	3435	rBV2	590	323	0.03%	0.003%
91	12.721	3631	3633	3636	rBV3	701	399	0.03%	0.004%
92	12.853	3672	3674	3676	rBV	694	249	0.02%	0.002%
93	13.078	3741	3744	3745	rBV2	667	305	0.02%	0.003%
94	13.422	3848	3851	3854	rBV3	932	646	0.05%	0.006%
95	13.548	3888	3890	3893	rBV4	727	448	0.04%	0.004%
96	13.696	3934	3936	3939	rBV3	919	613	0.05%	0.006%
97	13.873	3988	3991	3992	rBV2	1040	581	0.05%	0.006%
98	13.995	4027	4029	4032	rBV2	721	383	0.03%	0.004%
99	14.377	4146	4148	4152	rBV3	796	523	0.04%	0.005%
100	14.667	4236	4238	4240	rBV2	887	477	0.04%	0.005%




Sum of corrected areas: 9981125

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028039.D
Acq On : 22 Sep 2022 01:28
Operator : SY/MD
Sample : N4659-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

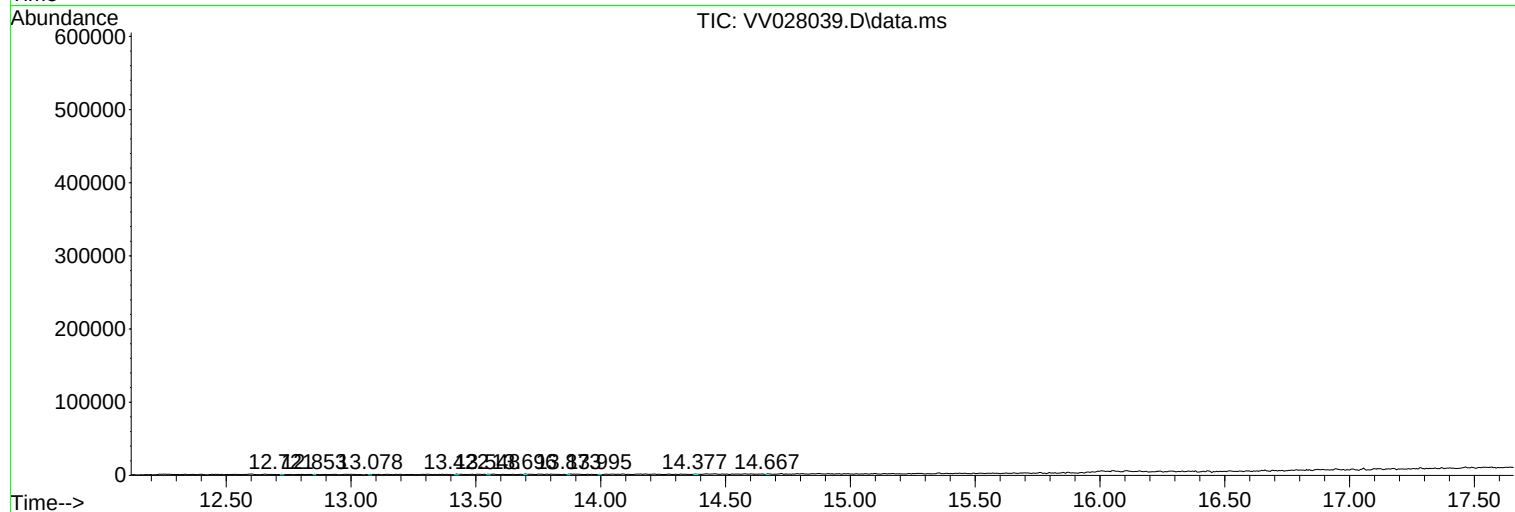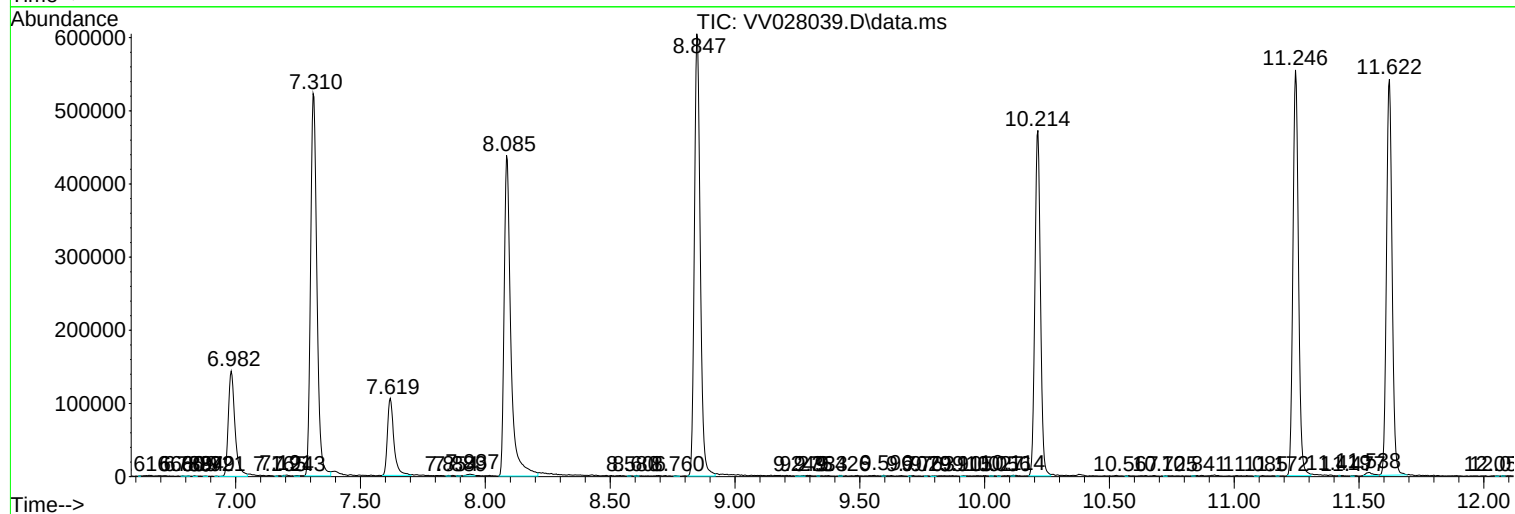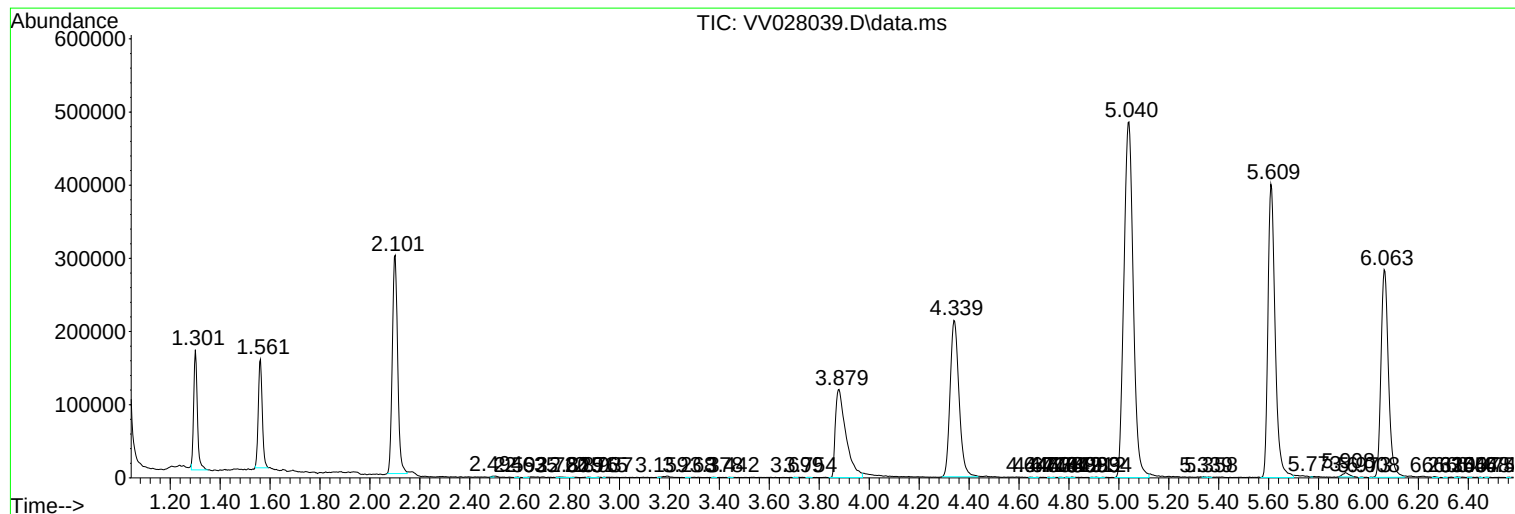

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028039.D
Acq On : 22 Sep 2022 01:28
Operator : SY/MD
Sample : N4659-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028039.D
Acq On : 22 Sep 2022 01:28
Operator : SY/MD
Sample : N4659-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc