

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028040.D
 Acq On : 22 Sep 2022 01:52
 Operator : SY/MD
 Sample : N4659-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	167715	180013	6.98%	1.352%
2	1.561	156	162	173	rVB	148563	161673	6.27%	1.214%
3	2.101	320	330	348	rBV3	357790	578402	22.42%	4.343%
4	2.278	381	385	386	rBV3	881	595	0.02%	0.004%
5	2.912	578	582	584	rBV	638	435	0.02%	0.003%
6	2.954	587	595	604	rVV6	2405	4664	0.18%	0.035%
7	3.037	619	621	629	rVB4	705	750	0.03%	0.006%
8	3.108	639	643	644	rBV2	378	261	0.01%	0.002%
9	3.182	655	666	667	rBV4	1899	2467	0.10%	0.019%
10	3.243	682	685	687	rVV3	579	315	0.01%	0.002%
11	3.278	693	696	699	rVB3	569	386	0.01%	0.003%
12	3.359	716	721	724	rVV3	527	487	0.02%	0.004%
13	3.436	743	745	749	rBV2	532	386	0.01%	0.003%
14	3.516	768	770	774	rVB3	588	262	0.01%	0.002%
15	3.751	840	843	845	rBV	412	242	0.01%	0.002%
16	3.883	873	884	917	rBV2	120901	417068	16.17%	3.131%
17	4.285	1006	1009	1010	rBV3	456	269	0.01%	0.002%
18	4.343	1010	1027	1048	rVV	218884	536600	20.80%	4.029%
19	4.600	1091	1107	1123	rBV2	37920	96545	3.74%	0.725%
20	4.786	1161	1165	1166	rBV2	422	283	0.01%	0.002%
21	4.825	1175	1177	1181	rBV3	697	501	0.02%	0.004%
22	4.854	1181	1186	1190	rVB3	790	718	0.03%	0.005%
23	5.037	1226	1243	1274	rBV2	513135	1327295	51.46%	9.966%
24	5.413	1357	1360	1365	rBV3	1091	877	0.03%	0.007%
25	5.539	1397	1399	1402	rBV4	577	370	0.01%	0.003%
26	5.609	1409	1421	1444	rBV	465646	944771	36.63%	7.094%
27	5.905	1499	1513	1549	rBV	1331044	2579314	100.00%	19.366%
28	6.063	1551	1562	1585	rVB	287855	583919	22.64%	4.384%
29	6.320	1640	1642	1645	rVV2	689	288	0.01%	0.002%
30	6.339	1645	1648	1652	rVB4	755	571	0.02%	0.004%
31	6.365	1654	1656	1661	rVB3	436	247	0.01%	0.002%
32	6.461	1684	1686	1689	rVB2	1140	507	0.02%	0.004%
33	6.522	1700	1705	1710	rBV6	955	1177	0.05%	0.009%
34	6.567	1714	1719	1726	rBV3	471	605	0.02%	0.005%
35	6.645	1735	1743	1744	rBV5	1091	1142	0.04%	0.009%
36	6.709	1761	1763	1765	rBV2	558	280	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028040.D
 Acq On : 22 Sep 2022 01:52
 Operator : SY/MD
 Sample : N4659-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.744	1771	1774	1777	rVB4	653	492	0.02%	0.004%
38	6.764	1777	1780	1783	rBV3	474	354	0.01%	0.003%
39	6.796	1789	1790	1793	rBV	463	260	0.01%	0.002%
40	6.818	1794	1797	1800	rVV3	617	368	0.01%	0.003%
41	6.886	1816	1818	1821	rBV3	389	339	0.01%	0.003%
42	6.982	1838	1848	1871	rBV	142286	259891	10.08%	1.951%
43	7.156	1900	1902	1903	rBV2	690	300	0.01%	0.002%
44	7.313	1939	1951	1970	rBV	528811	924761	35.85%	6.943%
45	7.619	2036	2046	2067	rBV	104354	190835	7.40%	1.433%
46	7.818	2104	2108	2110	rBV3	641	439	0.02%	0.003%
47	7.850	2113	2118	2124	rVV8	2127	2733	0.11%	0.021%
48	7.937	2139	2145	2153	rVB3	3304	5070	0.20%	0.038%
49	8.085	2181	2191	2228	rVV	412815	768989	29.81%	5.774%
50	8.661	2368	2370	2372	rBV	609	316	0.01%	0.002%
51	8.674	2372	2374	2377	rBV3	929	380	0.01%	0.003%
52	8.728	2389	2391	2394	rBV3	791	435	0.02%	0.003%
53	8.847	2417	2428	2449	rBV	703398	1138755	44.15%	8.550%
54	9.092	2501	2504	2508	rBV5	806	828	0.03%	0.006%
55	9.191	2533	2535	2538	rBV3	628	551	0.02%	0.004%
56	9.301	2567	2569	2572	rVB3	778	320	0.01%	0.002%
57	9.458	2617	2618	2620	rBV	439	246	0.01%	0.002%
58	9.513	2633	2635	2637	rBV2	418	247	0.01%	0.002%
59	9.609	2663	2665	2669	rBV3	509	263	0.01%	0.002%
60	9.638	2671	2674	2676	rBV3	462	279	0.01%	0.002%
61	9.651	2676	2678	2681	rVB3	679	250	0.01%	0.002%
62	9.731	2701	2703	2706	rBV3	444	251	0.01%	0.002%
63	9.863	2741	2744	2746	rBV4	635	447	0.02%	0.003%
64	9.895	2750	2754	2757	rVB4	892	560	0.02%	0.004%
65	9.940	2763	2768	2772	rVB4	1037	835	0.03%	0.006%
66	9.979	2778	2780	2785	rVB4	746	533	0.02%	0.004%
67	10.014	2785	2791	2792	rBV	962	718	0.03%	0.005%
68	10.108	2815	2820	2822	rBV5	1086	885	0.03%	0.007%
69	10.214	2840	2853	2876	rBV	459718	727442	28.20%	5.462%
70	10.513	2943	2946	2949	rBV3	786	618	0.02%	0.005%
71	10.670	2992	2995	2997	rVB2	563	357	0.01%	0.003%
72	10.850	3050	3051	3053	rBV2	570	294	0.01%	0.002%
73	10.899	3061	3066	3067	rBV4	687	508	0.02%	0.004%
74	10.915	3068	3071	3076	rVV3	1000	864	0.03%	0.006%
75	11.034	3106	3108	3111	rVB2	469	268	0.01%	0.002%
76	11.133	3137	3139	3140	rBV2	681	329	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028040.D
 Acq On : 22 Sep 2022 01:52
 Operator : SY/MD
 Sample : N4659-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.153	3143	3145	3148	rVV3	841	457	0.02%	0.003%
78	11.194	3154	3158	3159	rVB2	411	241	0.01%	0.002%
79	11.246	3162	3174	3194	rBV	641853	974443	37.78%	7.316%
80	11.538	3258	3265	3276	rBV6	5025	10326	0.40%	0.078%
81	11.622	3280	3291	3311	rVV	546570	864737	33.53%	6.493%
82	12.030	3417	3418	3421	rBV3	538	307	0.01%	0.002%
83	12.297	3500	3501	3504	rVB3	702	300	0.01%	0.002%
84	12.313	3504	3506	3509	rVB	886	385	0.01%	0.003%
85	12.329	3509	3511	3513	rBV2	768	484	0.02%	0.004%
86	12.484	3555	3559	3563	rBV6	1038	863	0.03%	0.006%
87	12.587	3587	3591	3592	rBV4	668	415	0.02%	0.003%
88	12.696	3622	3625	3626	rBV	402	286	0.01%	0.002%
89	12.767	3645	3647	3652	rBV4	634	614	0.02%	0.005%
90	12.918	3692	3694	3696	rBV2	735	341	0.01%	0.003%
91	13.030	3724	3729	3731	rBV3	768	706	0.03%	0.005%
92	13.249	3793	3797	3801	rBV3	1017	996	0.04%	0.007%
93	13.416	3846	3849	3853	rBV4	853	801	0.03%	0.006%
94	13.493	3871	3873	3876	rBV2	524	250	0.01%	0.002%
95	13.596	3903	3905	3908	rBV3	853	529	0.02%	0.004%
96	13.632	3912	3916	3921	rVB5	1012	933	0.04%	0.007%
97	13.747	3949	3952	3954	rBV3	967	598	0.02%	0.004%
98	14.197	4088	4092	4096	rBV6	809	866	0.03%	0.007%
99	14.596	4212	4216	4217	rBV3	1193	767	0.03%	0.006%
100	14.857	4295	4297	4302	rBV3	901	660	0.03%	0.005%




Sum of corrected areas: 13318600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028040.D
Acq On : 22 Sep 2022 01:52
Operator : SY/MD
Sample : N4659-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

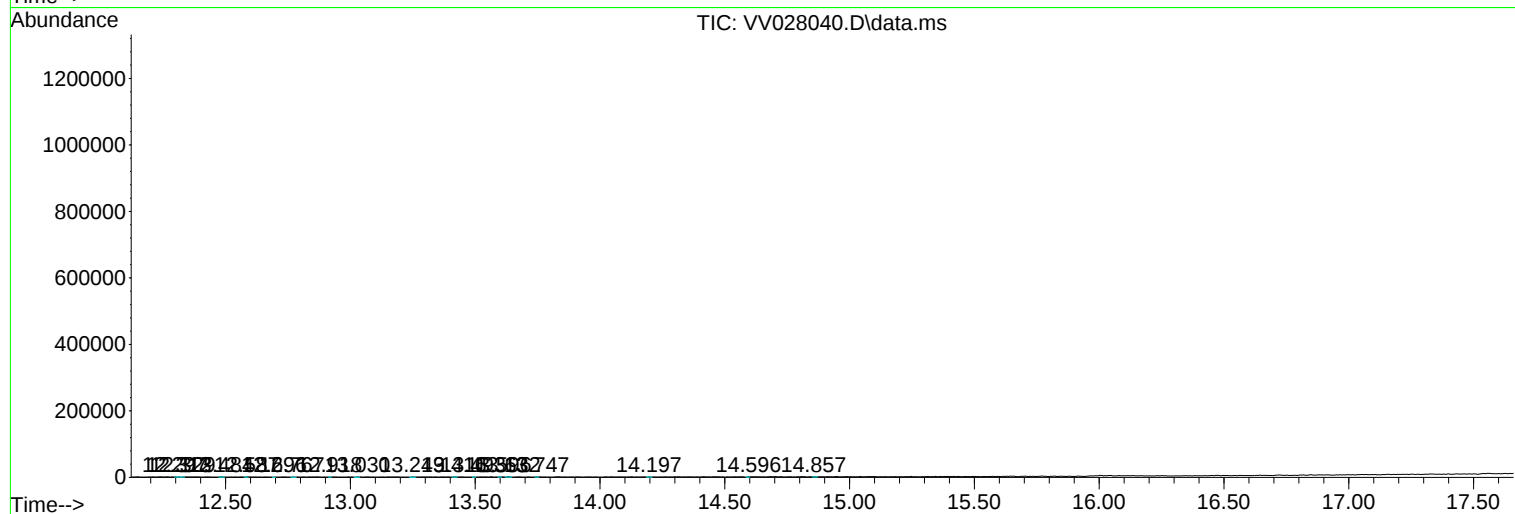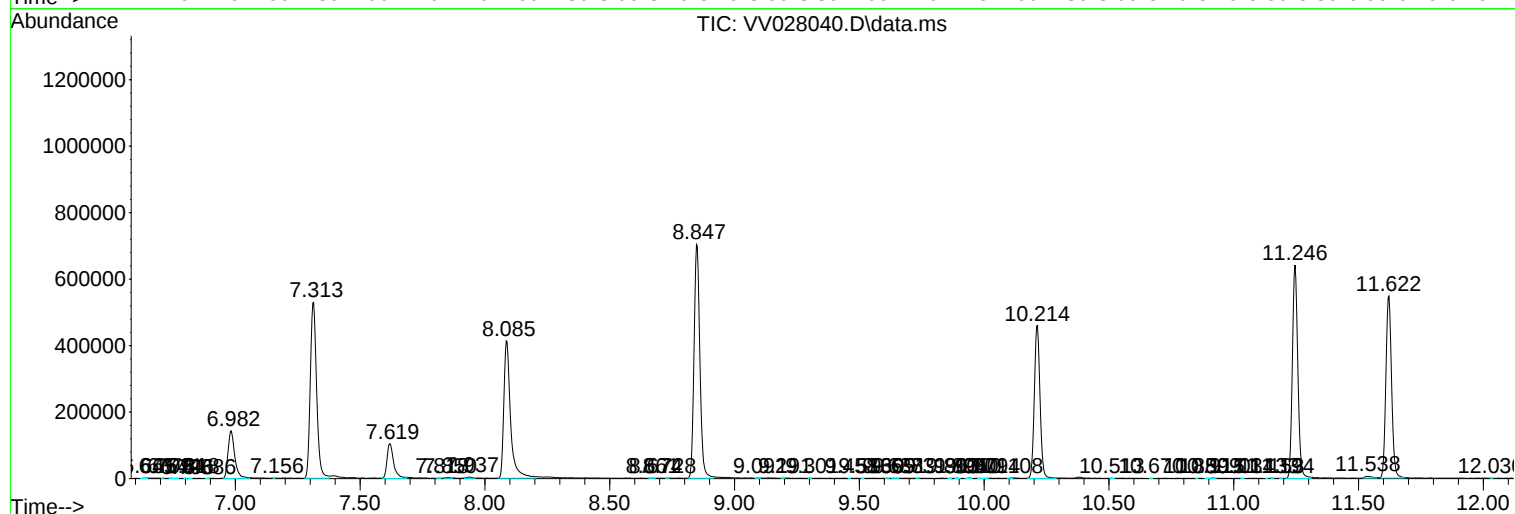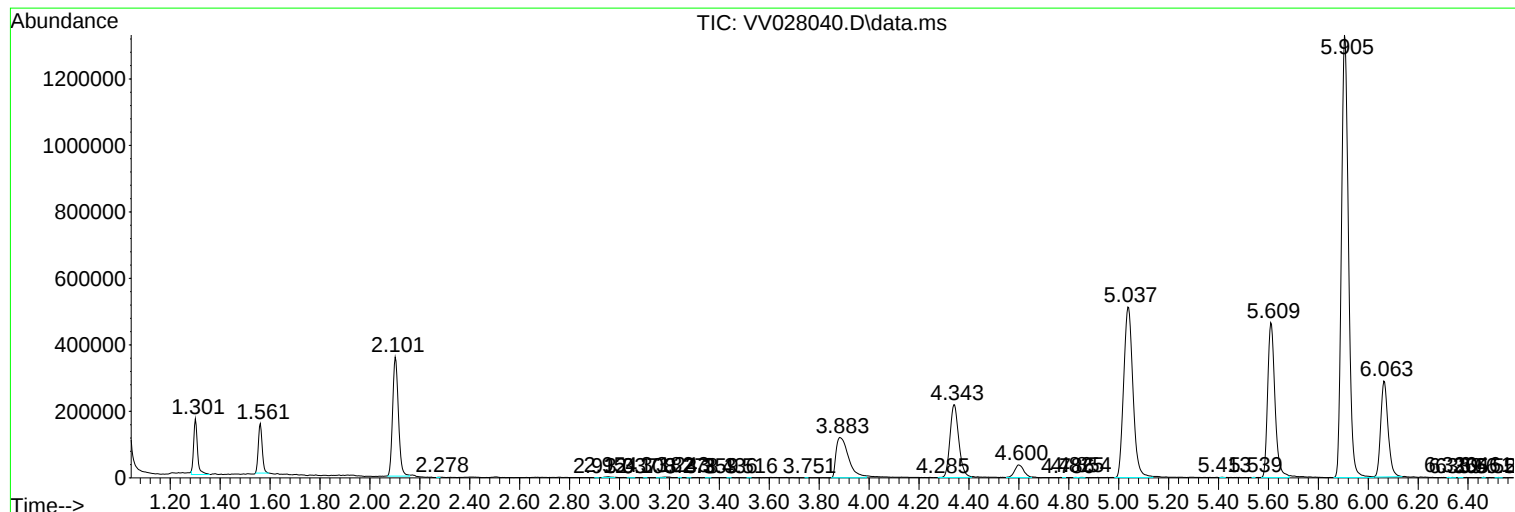

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028040.D
Acq On : 22 Sep 2022 01:52
Operator : SY/MD
Sample : N4659-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028040.D
Acq On : 22 Sep 2022 01:52
Operator : SY/MD
Sample : N4659-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
