

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028041.D
 Acq On : 22 Sep 2022 02:17
 Operator : SY/MD
 Sample : N4659-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	95	rVB	164007	167666	13.26%	1.682%
2	1.561	156	162	176	rVB	141827	161769	12.79%	1.623%
3	2.101	320	330	342	rBV	290754	418085	33.06%	4.194%
4	2.265	379	381	383	rBV2	615	268	0.02%	0.003%
5	2.413	424	427	428	rBV2	445	230	0.02%	0.002%
6	2.503	448	455	463	rVB5	1670	2655	0.21%	0.027%
7	2.613	485	489	492	rBV3	495	404	0.03%	0.004%
8	2.741	525	529	533	rBV2	512	404	0.03%	0.004%
9	2.764	533	536	541	rBV2	348	384	0.03%	0.004%
10	2.809	546	550	556	rVB3	627	507	0.04%	0.005%
11	2.886	572	574	576	rBV	542	229	0.02%	0.002%
12	2.937	587	590	591	rBV2	519	268	0.02%	0.003%
13	3.021	613	616	619	rVV2	398	266	0.02%	0.003%
14	3.076	631	633	637	rBV	372	278	0.02%	0.003%
15	3.092	637	638	642	rVV2	366	228	0.02%	0.002%
16	3.217	673	677	680	rBV4	528	349	0.03%	0.004%
17	3.288	695	699	702	rBV3	416	267	0.02%	0.003%
18	3.352	715	719	720	rBV	327	233	0.02%	0.002%
19	3.497	759	764	767	rBV3	780	601	0.05%	0.006%
20	3.519	767	771	773	rVV2	491	368	0.03%	0.004%
21	3.719	829	833	838	rVB3	369	328	0.03%	0.003%
22	3.886	874	885	929	rBV2	107821	361095	28.56%	3.622%
23	4.339	1008	1026	1051	rBV3	213437	533922	42.22%	5.356%
24	4.535	1085	1087	1089	rBV	507	258	0.02%	0.003%
25	4.715	1139	1143	1148	rBV4	902	929	0.07%	0.009%
26	4.741	1150	1151	1155	rVB3	503	327	0.03%	0.003%
27	4.812	1171	1173	1183	rVB2	844	997	0.08%	0.010%
28	4.854	1183	1186	1187	rBV2	520	364	0.03%	0.004%
29	4.876	1191	1193	1197	rVB3	513	317	0.03%	0.003%
30	4.895	1197	1199	1202	rBV3	521	336	0.03%	0.003%
31	4.928	1206	1209	1212	rBV	837	469	0.04%	0.005%
32	5.037	1226	1243	1269	rBV2	486603	1264479	100.00%	12.684%
33	5.333	1333	1335	1339	rBV2	821	596	0.05%	0.006%
34	5.522	1392	1394	1397	rVB2	500	247	0.02%	0.002%
35	5.538	1397	1399	1402	rBV4	690	492	0.04%	0.005%
36	5.609	1409	1421	1449	rBV	404408	826343	65.35%	8.289%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028041.D
 Acq On : 22 Sep 2022 02:17
 Operator : SY/MD
 Sample : N4659-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.905	1504	1513	1528	rBV9	8256	19652	1.55%	0.197%
38	6.011	1541	1546	1548	rBV3	677	502	0.04%	0.005%
39	6.063	1549	1562	1587	rVV	295270	608305	48.11%	6.102%
40	6.481	1690	1692	1693	rBV	627	259	0.02%	0.003%
41	6.555	1713	1715	1720	rBV4	715	715	0.06%	0.007%
42	6.780	1782	1785	1787	rBV2	816	601	0.05%	0.006%
43	6.828	1798	1800	1802	rBV	854	460	0.04%	0.005%
44	6.982	1838	1848	1873	rBV	141748	261793	20.70%	2.626%
45	7.310	1939	1950	1972	rBV	524770	921472	72.87%	9.244%
46	7.619	2037	2046	2064	rBV	102495	178544	14.12%	1.791%
47	7.757	2086	2089	2092	rBV3	641	567	0.04%	0.006%
48	7.853	2117	2119	2123	rVB4	1017	615	0.05%	0.006%
49	7.908	2131	2136	2138	rBV4	731	633	0.05%	0.006%
50	7.934	2139	2144	2155	rVB5	2748	4616	0.37%	0.046%
51	8.034	2172	2175	2181	rBV4	863	588	0.05%	0.006%
52	8.088	2181	2192	2223	rBV	403162	756775	59.85%	7.591%
53	8.593	2347	2349	2353	rBV2	689	373	0.03%	0.004%
54	8.847	2417	2428	2452	rBV	609875	993429	78.56%	9.965%
55	9.381	2592	2594	2596	rBV3	586	256	0.02%	0.003%
56	9.468	2619	2621	2624	rVB	601	241	0.02%	0.002%
57	9.632	2668	2672	2675	rBV2	997	674	0.05%	0.007%
58	9.677	2682	2686	2688	rBV3	962	599	0.05%	0.006%
59	9.689	2688	2690	2692	rBV	663	350	0.03%	0.004%
60	9.754	2707	2710	2714	rVB5	636	536	0.04%	0.005%
61	9.776	2714	2717	2722	rBV4	458	478	0.04%	0.005%
62	9.808	2724	2727	2735	rVB4	604	600	0.05%	0.006%
63	9.847	2736	2739	2742	rBV4	630	397	0.03%	0.004%
64	9.966	2772	2776	2779	rBV3	1001	855	0.07%	0.009%
65	10.214	2840	2853	2874	rBV	458342	734192	58.06%	7.365%
66	10.381	2898	2905	2915	rVV3	3431	5327	0.42%	0.053%
67	10.429	2919	2920	2924	rBV2	613	333	0.03%	0.003%
68	10.545	2951	2956	2958	rBV3	1068	761	0.06%	0.008%
69	10.561	2958	2961	2962	rBV2	730	423	0.03%	0.004%
70	10.590	2968	2970	2971	rBV	629	325	0.03%	0.003%
71	10.625	2979	2981	2985	rBV2	680	549	0.04%	0.006%
72	10.747	3017	3019	3021	rBV	640	363	0.03%	0.004%
73	10.847	3047	3050	3054	rBV2	945	844	0.07%	0.008%
74	11.024	3103	3105	3109	rBV3	574	560	0.04%	0.006%
75	11.091	3120	3126	3130	rVB4	760	817	0.06%	0.008%
76	11.143	3140	3142	3146	rVB4	1250	657	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028041.D
 Acq On : 22 Sep 2022 02:17
 Operator : SY/MD
 Sample : N4659-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.246	3162	3174	3193	rBV	552794	852555	67.42%	8.552%
78	11.535	3254	3264	3273	rBV9	5479	11618	0.92%	0.117%
79	11.622	3280	3291	3311	rBV	538141	849017	67.14%	8.517%
80	11.898	3374	3377	3378	rBV3	721	413	0.03%	0.004%
81	12.185	3462	3466	3467	rBV2	680	422	0.03%	0.004%
82	12.339	3511	3514	3516	rBV2	938	638	0.05%	0.006%
83	12.596	3590	3594	3597	rVB3	961	663	0.05%	0.007%
84	12.638	3604	3607	3608	rBV3	626	282	0.02%	0.003%
85	12.905	3688	3690	3692	rVB	821	344	0.03%	0.003%
86	12.930	3696	3698	3700	rVV2	647	275	0.02%	0.003%
87	12.982	3711	3714	3716	rBV2	858	509	0.04%	0.005%
88	13.082	3743	3745	3747	rBV2	834	377	0.03%	0.004%
89	13.201	3780	3782	3785	rVB4	711	328	0.03%	0.003%
90	13.217	3785	3787	3790	rVB	658	245	0.02%	0.002%
91	13.455	3859	3861	3862	rBV2	742	255	0.02%	0.003%
92	13.541	3885	3888	3894	rBV2	1144	886	0.07%	0.009%
93	13.676	3928	3930	3933	rVB3	720	368	0.03%	0.004%
94	13.795	3965	3967	3970	rBV	527	347	0.03%	0.003%
95	13.856	3984	3986	3988	rBV2	493	268	0.02%	0.003%
96	13.882	3992	3994	3998	rVB2	714	390	0.03%	0.004%
97	13.950	4010	4015	4018	rBV3	582	639	0.05%	0.006%
98	14.059	4046	4049	4051	rBV	553	338	0.03%	0.003%
99	14.155	4077	4079	4082	rVB	514	288	0.02%	0.003%
100	14.326	4130	4132	4135	rBV	463	341	0.03%	0.003%




Sum of corrected areas: 9968800

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028041.D
Acq On : 22 Sep 2022 02:17
Operator : SY/MD
Sample : N4659-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

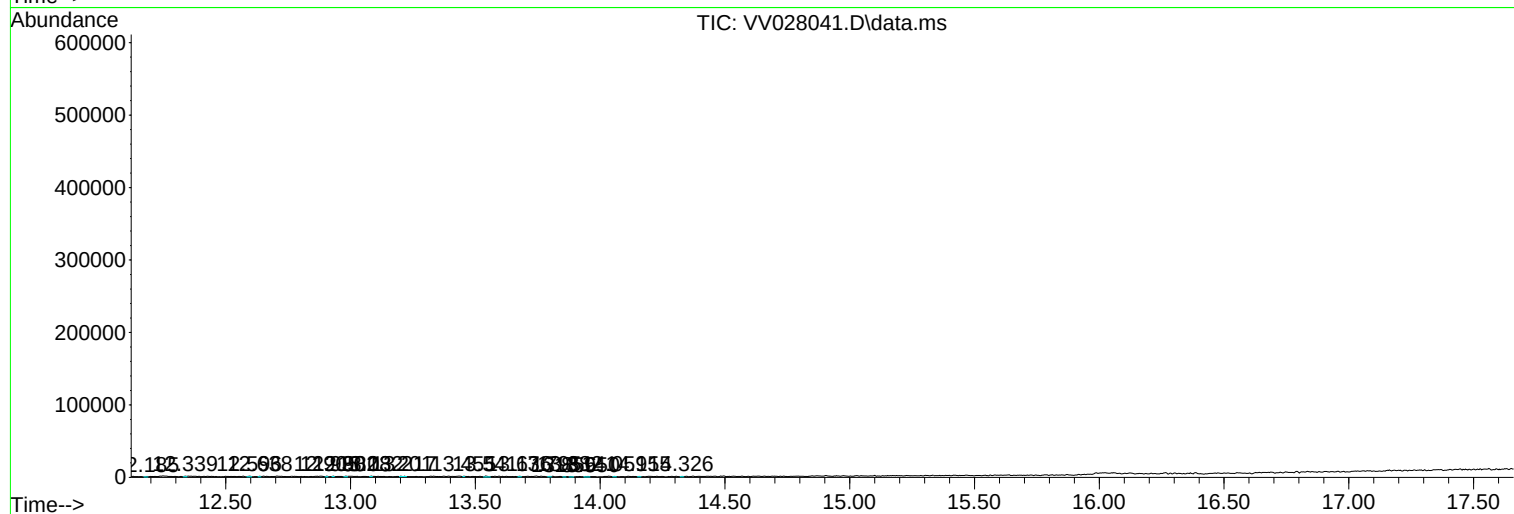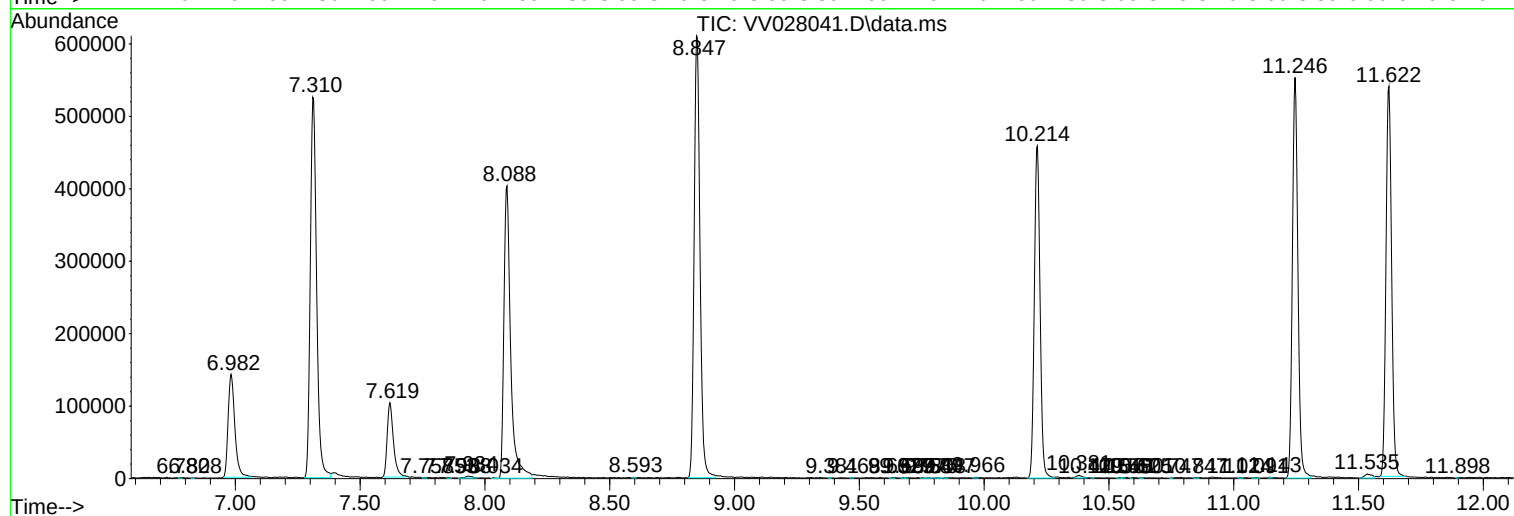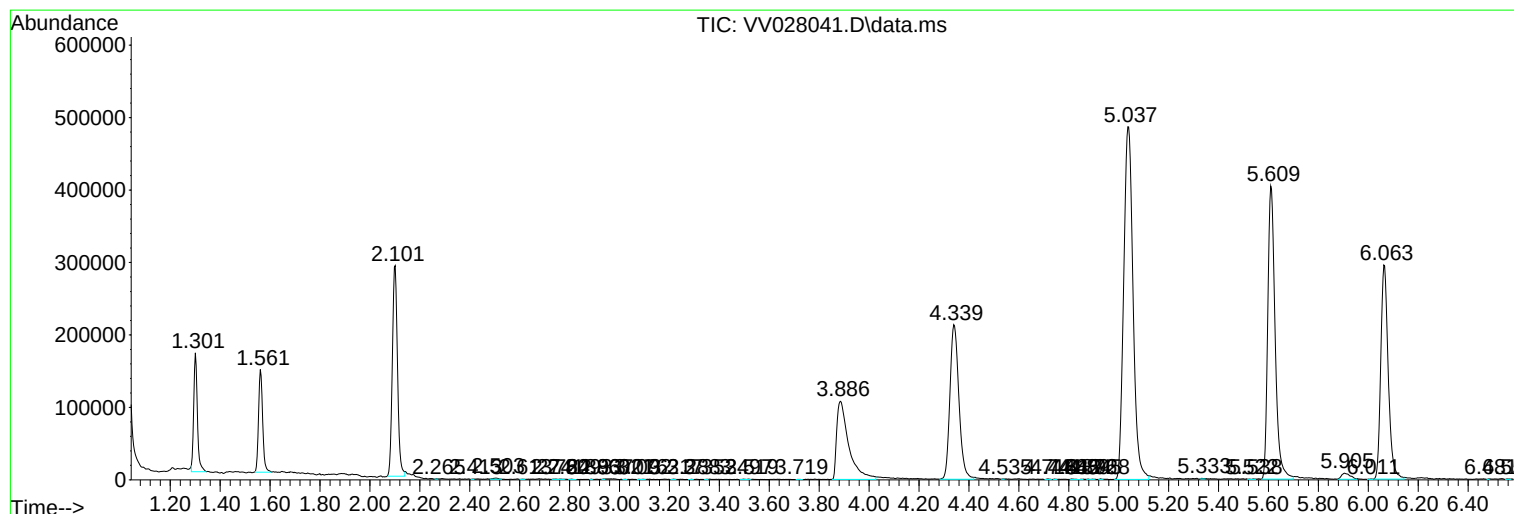

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028041.D
Acq On : 22 Sep 2022 02:17
Operator : SY/MD
Sample : N4659-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028041.D
Acq On : 22 Sep 2022 02:17
Operator : SY/MD
Sample : N4659-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc