

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028042.D
 Acq On : 22 Sep 2022 02:42
 Operator : SY/MD
 Sample : N4659-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	167010	176909	13.13%	1.728%
2	1.561	156	162	179	rVB	153340	173317	12.86%	1.693%
3	2.101	320	330	344	rBV	296715	435973	32.36%	4.258%
4	2.342	403	405	409	rBV3	676	334	0.02%	0.003%
5	2.770	535	538	540	rBV4	539	355	0.03%	0.003%
6	3.162	657	660	664	rVV3	426	338	0.03%	0.003%
7	3.262	686	691	692	rBV2	542	406	0.03%	0.004%
8	3.336	711	714	717	rBV3	511	353	0.03%	0.003%
9	3.397	729	733	736	rVB4	958	638	0.05%	0.006%
10	3.535	771	776	778	rBV3	731	576	0.04%	0.006%
11	3.571	784	787	794	rVB4	702	712	0.05%	0.007%
12	3.603	794	797	801	rBV	714	439	0.03%	0.004%
13	3.677	817	820	822	rBV2	725	366	0.03%	0.004%
14	3.876	869	882	918	rBV	123643	361860	26.86%	3.534%
15	4.339	1011	1026	1054	rBV	227112	564336	41.89%	5.512%
16	4.651	1120	1123	1127	rBV4	652	503	0.04%	0.005%
17	5.040	1228	1244	1270	rBV2	524490	1347344	100.00%	13.160%
18	5.291	1320	1322	1330	rVB3	917	770	0.06%	0.008%
19	5.358	1341	1343	1345	rBV3	709	352	0.03%	0.003%
20	5.468	1371	1377	1378	rBV2	915	628	0.05%	0.006%
21	5.609	1409	1421	1449	rBV	399466	819968	60.86%	8.009%
22	5.905	1504	1513	1528	rBV	8072	20794	1.54%	0.203%
23	6.001	1541	1543	1546	rBV4	745	404	0.03%	0.004%
24	6.063	1550	1562	1585	rVV	306829	631558	46.87%	6.168%
25	6.317	1638	1641	1643	rBV4	858	461	0.03%	0.005%
26	6.394	1662	1665	1668	rVB3	739	455	0.03%	0.004%
27	6.416	1668	1672	1673	rBV3	869	565	0.04%	0.006%
28	6.506	1697	1700	1702	rBV3	536	361	0.03%	0.004%
29	6.522	1702	1705	1708	rVB4	771	481	0.04%	0.005%
30	6.625	1734	1737	1738	rBV	646	380	0.03%	0.004%
31	6.879	1811	1816	1821	rBV5	1168	1132	0.08%	0.011%
32	6.982	1836	1848	1870	rBV	147741	275151	20.42%	2.687%
33	7.249	1929	1931	1936	rVB4	1112	814	0.06%	0.008%
34	7.310	1938	1950	1970	rBV	528273	923112	68.51%	9.016%
35	7.571	2028	2031	2035	rBV3	621	506	0.04%	0.005%
36	7.619	2035	2046	2066	rBV	102523	182613	13.55%	1.784%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028042.D
 Acq On : 22 Sep 2022 02:42
 Operator : SY/MD
 Sample : N4659-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	7.773	2092	2094	2097	rVB3	778	323	0.02%	0.003%
38	7.815	2104	2107	2112	rBV	4202	2576	0.19%	0.025%
39	7.870	2119	2124	2130	rBV6	734	764	0.06%	0.007%
40	7.934	2135	2144	2145	rBV3	3322	3410	0.25%	0.033%
41	8.001	2162	2165	2169	rBV4	643	392	0.03%	0.004%
42	8.085	2180	2191	2227	rBV	412073	779911	57.89%	7.617%
43	8.722	2387	2389	2392	rBV3	736	471	0.03%	0.005%
44	8.741	2392	2395	2399	rVB3	979	556	0.04%	0.005%
45	8.796	2407	2412	2413	rBV2	867	692	0.05%	0.007%
46	8.847	2417	2428	2457	rBV	598784	996160	73.94%	9.729%
47	9.291	2564	2566	2569	rVB2	795	499	0.04%	0.005%
48	9.310	2569	2572	2574	rBV2	754	558	0.04%	0.005%
49	9.378	2591	2593	2595	rVB2	770	339	0.03%	0.003%
50	9.429	2606	2609	2611	rBV4	739	421	0.03%	0.004%
51	9.641	2674	2675	2679	rVB4	713	373	0.03%	0.004%
52	9.660	2679	2681	2682	rBV4	876	384	0.03%	0.004%
53	9.702	2690	2694	2695	rBV3	797	482	0.04%	0.005%
54	9.725	2698	2701	2704	rVV3	526	374	0.03%	0.004%
55	9.831	2727	2734	2735	rBV4	633	701	0.05%	0.007%
56	9.850	2738	2740	2744	rVB3	781	465	0.03%	0.005%
57	9.950	2769	2771	2773	rVB3	742	330	0.02%	0.003%
58	10.053	2798	2803	2806	rBV6	752	562	0.04%	0.005%
59	10.120	2822	2824	2828	rBV5	1010	732	0.05%	0.007%
60	10.168	2836	2839	2841	rBV2	732	423	0.03%	0.004%
61	10.213	2841	2853	2873	rVV	477550	757670	56.23%	7.400%
62	10.458	2926	2929	2933	rVB2	711	480	0.04%	0.005%
63	10.480	2933	2936	2938	rBV2	896	592	0.04%	0.006%
64	10.590	2969	2970	2975	rBV2	568	538	0.04%	0.005%
65	10.696	2999	3003	3009	rBV2	511	691	0.05%	0.007%
66	10.738	3013	3016	3021	rVB2	580	451	0.03%	0.004%
67	10.792	3030	3033	3036	rBV4	794	470	0.03%	0.005%
68	10.821	3040	3042	3044	rBV3	909	321	0.02%	0.003%
69	10.847	3048	3050	3052	rBV2	664	389	0.03%	0.004%
70	10.902	3064	3067	3068	rBV2	782	319	0.02%	0.003%
71	10.963	3082	3086	3087	rBV3	525	319	0.02%	0.003%
72	11.088	3119	3125	3129	rBV4	835	927	0.07%	0.009%
73	11.133	3137	3139	3142	rBV	728	501	0.04%	0.005%
74	11.172	3149	3151	3157	rVB5	923	631	0.05%	0.006%
75	11.246	3162	3174	3198	rBV	544447	849690	63.06%	8.299%
76	11.471	3240	3244	3246	rBV2	746	486	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028042.D
 Acq On : 22 Sep 2022 02:42
 Operator : SY/MD
 Sample : N4659-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.535	3255	3264	3275	rBV6	6389	12456	0.92%	0.122%
78	11.622	3279	3291	3309	rVV	569017	884028	65.61%	8.634%
79	11.892	3373	3375	3379	rVB4	1115	575	0.04%	0.006%
80	12.152	3453	3456	3459	rBV3	630	353	0.03%	0.003%
81	12.207	3470	3473	3476	rVB4	910	497	0.04%	0.005%
82	12.300	3500	3502	3505	rVB4	931	478	0.04%	0.005%
83	12.323	3506	3509	3513	rVB3	495	368	0.03%	0.004%
84	12.419	3536	3539	3546	rVB3	869	712	0.05%	0.007%
85	12.483	3556	3559	3563	rVB3	689	533	0.04%	0.005%
86	12.519	3568	3570	3573	rVB3	1037	519	0.04%	0.005%
87	12.538	3573	3576	3579	rBV3	721	481	0.04%	0.005%
88	12.596	3592	3594	3598	rVB2	705	387	0.03%	0.004%
89	12.828	3664	3666	3669	rBV2	507	355	0.03%	0.003%
90	12.966	3707	3709	3712	rVB4	721	368	0.03%	0.004%
91	12.985	3712	3715	3718	rBV3	855	439	0.03%	0.004%
92	13.056	3734	3737	3742	rBV4	589	583	0.04%	0.006%
93	13.483	3868	3870	3871	rBV4	779	344	0.03%	0.003%
94	13.525	3881	3883	3886	rVB3	1089	525	0.04%	0.005%
95	13.551	3889	3891	3895	rVB2	611	361	0.03%	0.004%
96	13.715	3939	3942	3944	rBV3	718	391	0.03%	0.004%
97	13.901	3998	4000	4004	rVB3	853	393	0.03%	0.004%
98	13.921	4004	4006	4010	rVB2	904	534	0.04%	0.005%
99	14.078	4052	4055	4057	rBV2	953	407	0.03%	0.004%
100	14.294	4120	4122	4127	rBV4	894	831	0.06%	0.008%




Sum of corrected areas: 10238555

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028042.D
Acq On : 22 Sep 2022 02:42
Operator : SY/MD
Sample : N4659-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

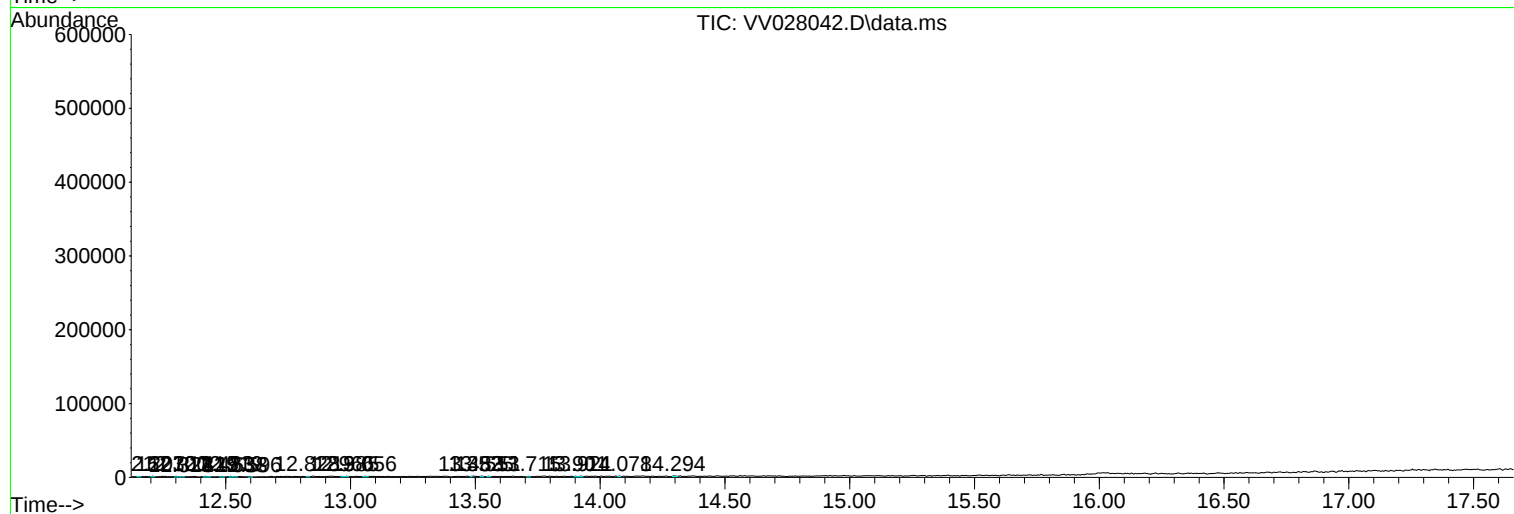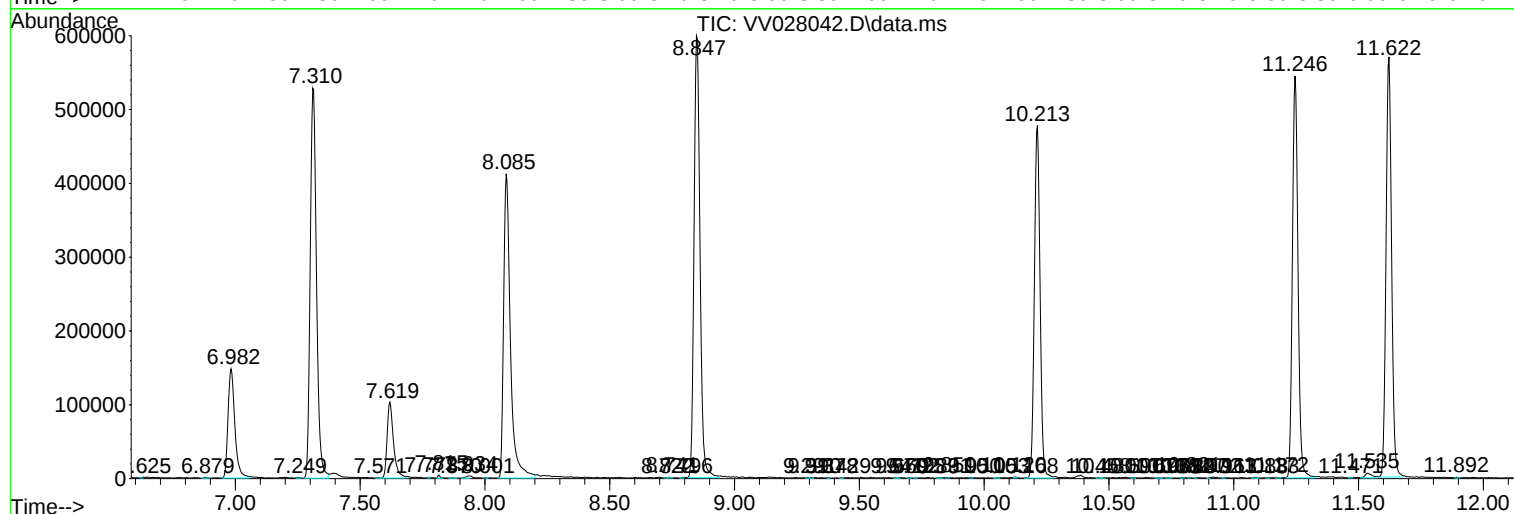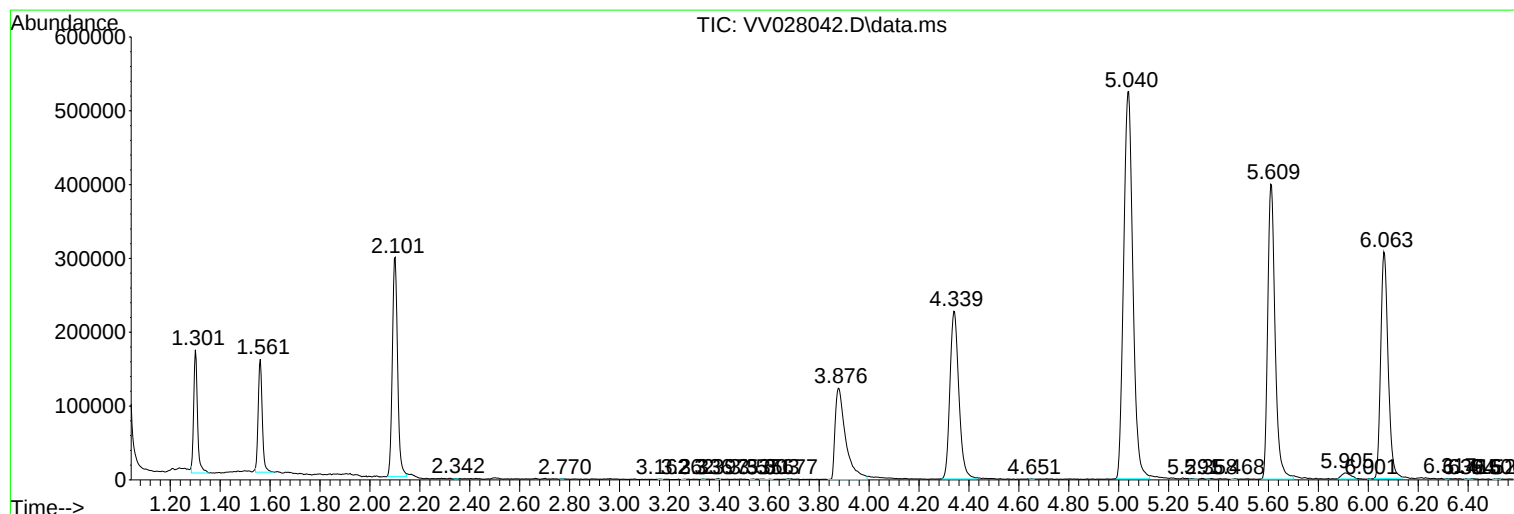

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028042.D
Acq On : 22 Sep 2022 02:42
Operator : SY/MD
Sample : N4659-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028042.D
Acq On : 22 Sep 2022 02:42
Operator : SY/MD
Sample : N4659-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc