

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028043.D
 Acq On : 22 Sep 2022 03:07
 Operator : SY/MD
 Sample : N4659-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	160648	164991	13.21%	1.679%
2	1.561	156	162	178	rVB	143347	163995	13.13%	1.669%
3	2.101	320	330	345	rBV	281605	412879	33.06%	4.202%
4	2.339	400	404	406	rBV3	731	572	0.05%	0.006%
5	2.555	465	471	472	rBV	949	578	0.05%	0.006%
6	2.658	501	503	507	rBV3	955	782	0.06%	0.008%
7	2.716	520	521	524	rVB	910	320	0.03%	0.003%
8	2.825	550	555	557	rVB	559	306	0.02%	0.003%
9	2.847	557	562	565	rBV2	435	414	0.03%	0.004%
10	3.034	617	620	621	rBV	578	255	0.02%	0.003%
11	3.098	637	640	641	rBV2	336	195	0.02%	0.002%
12	3.143	652	654	657	rVB2	397	196	0.02%	0.002%
13	3.195	667	670	672	rBV2	391	273	0.02%	0.003%
14	3.275	692	695	700	rBV3	608	486	0.04%	0.005%
15	3.320	704	709	711	rBV2	276	204	0.02%	0.002%
16	3.375	720	726	731	rVB3	465	322	0.03%	0.003%
17	3.471	753	756	759	rBV	359	263	0.02%	0.003%
18	3.487	759	761	764	rVB2	410	203	0.02%	0.002%
19	3.516	767	770	773	rBV	449	306	0.02%	0.003%
20	3.539	776	777	779	rBV	357	175	0.01%	0.002%
21	3.577	785	789	791	rBV3	418	336	0.03%	0.003%
22	3.603	795	797	799	rVV	463	218	0.02%	0.002%
23	3.616	799	801	802	rVV	592	192	0.02%	0.002%
24	3.651	809	812	815	rBV2	517	283	0.02%	0.003%
25	3.725	829	835	837	rBV4	953	840	0.07%	0.009%
26	3.773	848	850	852	rBV2	303	171	0.01%	0.002%
27	3.831	865	868	870	rBV	516	295	0.02%	0.003%
28	3.880	873	883	913	rBV	121292	364894	29.22%	3.713%
29	4.339	1012	1026	1056	rBV	207492	513474	41.11%	5.225%
30	4.587	1100	1103	1105	rBV3	494	342	0.03%	0.003%
31	4.722	1141	1145	1147	rBV2	816	528	0.04%	0.005%
32	4.757	1152	1156	1160	rBV3	775	614	0.05%	0.006%
33	4.828	1175	1178	1180	rVB2	956	455	0.04%	0.005%
34	4.841	1180	1182	1188	rBV3	340	318	0.03%	0.003%
35	5.040	1227	1244	1276	rBV2	476836	1248955	100.00%	12.710%
36	5.368	1345	1346	1354	rVB2	1346	979	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028043.D
 Acq On : 22 Sep 2022 03:07
 Operator : SY/MD
 Sample : N4659-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.407	1354	1358	1361	rBV4	915	718	0.06%	0.007%
38	5.432	1364	1366	1369	rBV	335	188	0.02%	0.002%
39	5.609	1409	1421	1444	rBV	394144	800786	64.12%	8.149%
40	5.905	1502	1513	1526	rBV6	10255	23843	1.91%	0.243%
41	5.976	1534	1535	1537	rBV2	781	237	0.02%	0.002%
42	6.063	1548	1562	1592	rBV	293841	615150	49.25%	6.260%
43	6.307	1629	1638	1641	rBV6	5481	9308	0.75%	0.095%
44	6.487	1692	1694	1696	rBV2	584	286	0.02%	0.003%
45	6.519	1700	1704	1707	rBV4	1042	1078	0.09%	0.011%
46	6.760	1776	1779	1782	rBV4	904	639	0.05%	0.007%
47	6.934	1831	1833	1835	rBV3	682	332	0.03%	0.003%
48	6.982	1837	1848	1869	rVV	136838	256340	20.52%	2.609%
49	7.310	1939	1950	1968	rBV	482293	846902	67.81%	8.618%
50	7.619	2036	2046	2069	rBV	99481	175295	14.04%	1.784%
51	7.799	2098	2102	2106	rBV4	531	606	0.05%	0.006%
52	7.870	2122	2124	2127	rBV2	592	371	0.03%	0.004%
53	7.918	2137	2139	2140	rBV2	653	277	0.02%	0.003%
54	8.085	2181	2191	2223	rBV	420186	797785	63.88%	8.119%
55	8.564	2336	2340	2342	rBV3	810	573	0.05%	0.006%
56	8.664	2369	2371	2375	rBV4	718	505	0.04%	0.005%
57	8.847	2417	2428	2450	rBV	606375	983144	78.72%	10.005%
58	9.008	2475	2478	2480	rBV2	1165	801	0.06%	0.008%
59	9.275	2559	2561	2562	rBV	531	243	0.02%	0.002%
60	9.477	2621	2624	2625	rBV2	666	368	0.03%	0.004%
61	9.741	2704	2706	2708	rBV2	495	208	0.02%	0.002%
62	9.818	2722	2730	2732	rBV5	2075	2219	0.18%	0.023%
63	9.915	2758	2760	2763	rBV2	503	364	0.03%	0.004%
64	9.953	2770	2772	2776	rVB3	357	232	0.02%	0.002%
65	9.979	2777	2780	2782	rBV2	761	404	0.03%	0.004%
66	10.114	2820	2822	2826	rBV3	955	690	0.06%	0.007%
67	10.149	2831	2833	2835	rVB	612	222	0.02%	0.002%
68	10.214	2841	2853	2872	rBV	454297	724257	57.99%	7.370%
69	10.464	2926	2931	2934	rBV4	722	843	0.07%	0.009%
70	10.490	2937	2939	2942	rBV2	402	260	0.02%	0.003%
71	10.526	2948	2950	2951	rBV2	620	280	0.02%	0.003%
72	10.574	2963	2965	2967	rBV3	824	493	0.04%	0.005%
73	10.735	3013	3015	3018	rVB2	561	220	0.02%	0.002%
74	10.892	3059	3064	3065	rBV	407	374	0.03%	0.004%
75	11.053	3110	3114	3116	rBV3	641	369	0.03%	0.004%
76	11.246	3163	3174	3196	rBV	547087	844662	67.63%	8.596%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028043.D
 Acq On : 22 Sep 2022 03:07
 Operator : SY/MD
 Sample : N4659-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.538	3257	3265	3279	rBV5	6333	13418	1.07%	0.137%
78	11.622	3279	3291	3313	rVV	530335	831580	66.58%	8.462%
79	11.892	3372	3375	3376	rBV2	548	287	0.02%	0.003%
80	12.181	3464	3465	3469	rBV3	600	387	0.03%	0.004%
81	12.204	3469	3472	3477	rVB3	999	705	0.06%	0.007%
82	12.291	3497	3499	3502	rBV	527	345	0.03%	0.004%
83	12.307	3502	3504	3505	rVV2	594	171	0.01%	0.002%
84	12.500	3561	3564	3565	rBV2	583	328	0.03%	0.003%
85	12.744	3638	3640	3643	rBV	691	494	0.04%	0.005%
86	12.760	3643	3645	3649	rVV3	568	444	0.04%	0.005%
87	12.799	3654	3657	3658	rVB2	634	255	0.02%	0.003%
88	12.927	3692	3697	3699	rBV4	1052	818	0.07%	0.008%
89	12.960	3705	3707	3708	rBV	420	202	0.02%	0.002%
90	13.194	3777	3780	3782	rBV2	995	403	0.03%	0.004%
91	13.226	3787	3790	3794	rBV3	485	391	0.03%	0.004%
92	13.291	3808	3810	3814	rBV3	480	296	0.02%	0.003%
93	13.313	3814	3817	3821	rBV2	1085	699	0.06%	0.007%
94	13.451	3858	3860	3864	rBV3	650	416	0.03%	0.004%
95	13.686	3931	3933	3937	rBV4	507	261	0.02%	0.003%
96	14.008	4031	4033	4036	rBV	640	473	0.04%	0.005%
97	14.185	4086	4088	4093	rBV2	890	477	0.04%	0.005%
98	14.435	4164	4166	4168	rBV3	827	415	0.03%	0.004%
99	14.676	4238	4241	4242	rBV2	678	394	0.03%	0.004%
100	15.374	4456	4458	4459	rBV	1395	529	0.04%	0.005%




Sum of corrected areas: 9826669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028043.D
Acq On : 22 Sep 2022 03:07
Operator : SY/MD
Sample : N4659-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

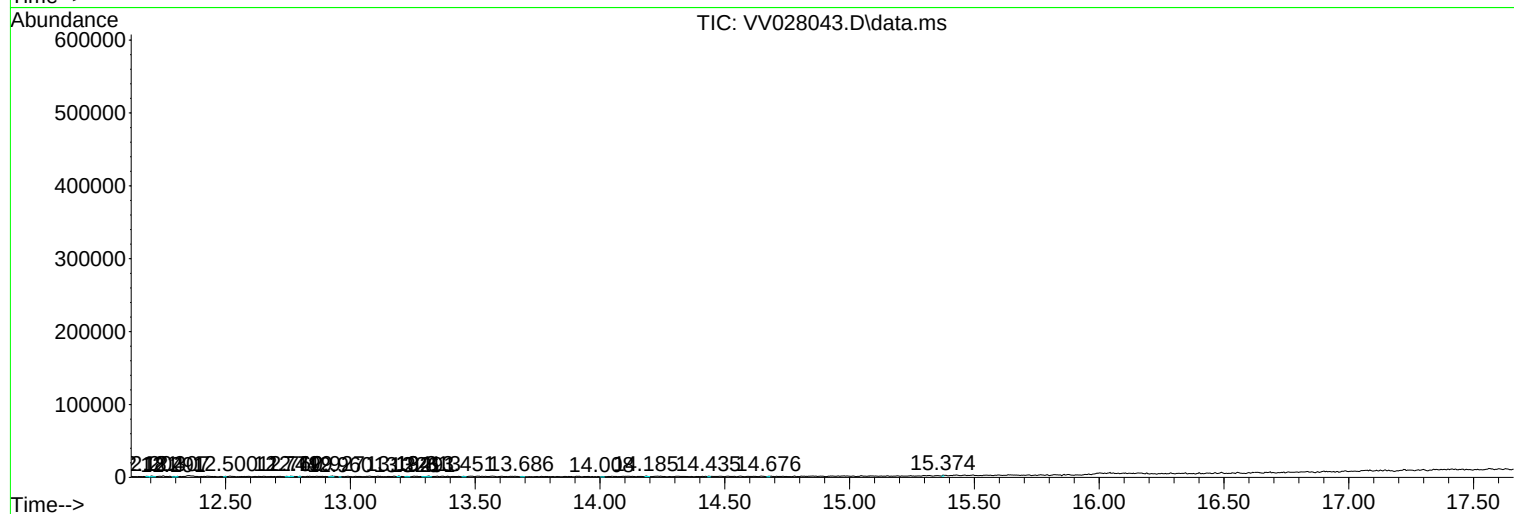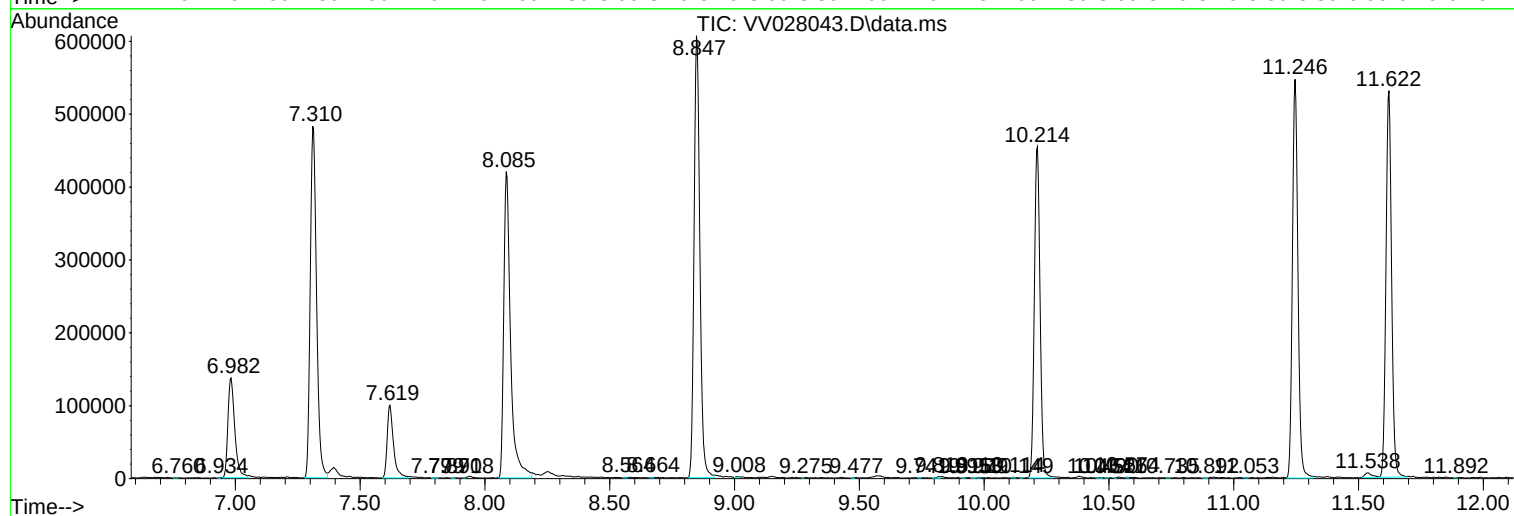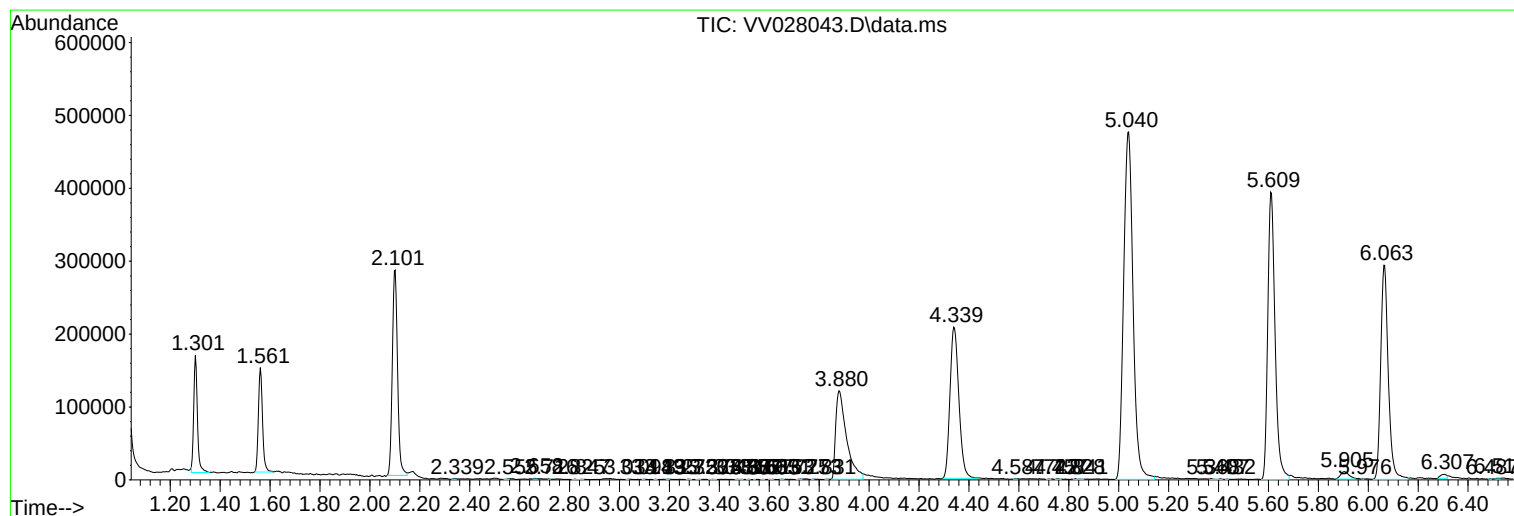

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028043.D
Acq On : 22 Sep 2022 03:07
Operator : SY/MD
Sample : N4659-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028043.D
Acq On : 22 Sep 2022 03:07
Operator : SY/MD
Sample : N4659-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc