

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028044.D
 Acq On : 22 Sep 2022 03:32
 Operator : SY/MD
 Sample : N4659-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	101	rVB	230567	244906	16.61%	2.197%
2	1.561	156	162	177	rVB	184093	205484	13.93%	1.844%
3	2.101	320	330	346	rBV	392512	563645	38.22%	5.057%
4	2.423	427	430	431	rBV2	544	332	0.02%	0.003%
5	2.651	494	501	502	rBV4	1076	1168	0.08%	0.010%
6	2.712	518	520	523	rBV3	657	415	0.03%	0.004%
7	2.831	555	557	559	rBV3	458	240	0.02%	0.002%
8	2.844	559	561	564	rVV3	461	260	0.02%	0.002%
9	2.876	569	571	573	rBV	501	254	0.02%	0.002%
10	2.909	579	581	583	rBV	433	208	0.01%	0.002%
11	3.050	621	625	626	rBV2	414	262	0.02%	0.002%
12	3.069	629	631	638	rVB4	528	506	0.03%	0.005%
13	3.130	644	650	653	rBV5	476	517	0.04%	0.005%
14	3.246	682	686	687	rBV2	313	187	0.01%	0.002%
15	3.355	717	720	722	rBV2	344	207	0.01%	0.002%
16	3.519	769	771	774	rBV2	456	206	0.01%	0.002%
17	3.642	807	809	814	rVB3	727	331	0.02%	0.003%
18	3.699	824	827	830	rVB3	482	233	0.02%	0.002%
19	3.757	841	845	847	rVB2	665	348	0.02%	0.003%
20	3.780	847	852	854	rBV	552	454	0.03%	0.004%
21	3.883	874	884	919	rBV	117412	366611	24.86%	3.289%
22	4.275	1004	1006	1008	rBV2	851	411	0.03%	0.004%
23	4.339	1011	1026	1058	rVV	247387	621421	42.14%	5.575%
24	4.590	1102	1104	1108	rVB4	1382	725	0.05%	0.007%
25	4.780	1158	1163	1164	rBV2	656	404	0.03%	0.004%
26	4.793	1164	1167	1170	rVB2	579	410	0.03%	0.004%
27	4.815	1170	1174	1175	rBV3	459	218	0.01%	0.002%
28	4.825	1175	1177	1179	rBV	560	304	0.02%	0.003%
29	4.892	1193	1198	1199	rBV3	661	444	0.03%	0.004%
30	4.979	1220	1225	1226	rBV2	608	396	0.03%	0.004%
31	5.040	1226	1244	1270	rBV2	576874	1474802	100.00%	13.231%
32	5.481	1378	1381	1384	rBV3	619	466	0.03%	0.004%
33	5.516	1389	1392	1396	rVB3	553	347	0.02%	0.003%
34	5.539	1396	1399	1401	rVB2	703	360	0.02%	0.003%
35	5.551	1401	1403	1405	rBV	662	389	0.03%	0.003%
36	5.609	1408	1421	1448	rBV	389430	795310	53.93%	7.135%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028044.D
 Acq On : 22 Sep 2022 03:32
 Operator : SY/MD
 Sample : N4659-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.912	1503	1515	1527	rBV	8269	19032	1.29%	0.171%
38	5.982	1535	1537	1541	rVB3	592	389	0.03%	0.003%
39	6.063	1547	1562	1586	rBV	324866	675082	45.77%	6.057%
40	6.301	1631	1636	1638	rBV2	982	925	0.06%	0.008%
41	6.413	1668	1671	1675	rBV3	566	397	0.03%	0.004%
42	6.461	1684	1686	1688	rBV	482	185	0.01%	0.002%
43	6.603	1727	1730	1731	rBV2	737	411	0.03%	0.004%
44	6.715	1762	1765	1766	rBV2	717	364	0.02%	0.003%
45	6.899	1819	1822	1824	rBV2	596	356	0.02%	0.003%
46	6.915	1824	1827	1830	rVB2	969	564	0.04%	0.005%
47	6.982	1834	1848	1873	rBV	169131	318260	21.58%	2.855%
48	7.310	1939	1950	1970	rBV	665667	1165097	79.00%	10.453%
49	7.619	2036	2046	2070	rBV	121869	218700	14.83%	1.962%
50	8.085	2181	2191	2223	rBV	434264	821304	55.69%	7.368%
51	8.494	2314	2318	2320	rBV3	1214	1036	0.07%	0.009%
52	8.703	2381	2383	2386	rBV	661	491	0.03%	0.004%
53	8.725	2388	2390	2392	rVB	818	344	0.02%	0.003%
54	8.738	2392	2394	2397	rBV3	448	258	0.02%	0.002%
55	8.754	2397	2399	2403	rBV2	604	447	0.03%	0.004%
56	8.847	2417	2428	2450	rBV	603727	989185	67.07%	8.875%
57	9.066	2494	2496	2498	rBV2	640	362	0.02%	0.003%
58	9.092	2501	2504	2507	rVV3	598	382	0.03%	0.003%
59	9.140	2516	2519	2520	rBV2	608	397	0.03%	0.004%
60	9.243	2546	2551	2554	rVB3	427	392	0.03%	0.004%
61	9.291	2563	2566	2568	rBV3	360	228	0.02%	0.002%
62	9.342	2578	2582	2584	rBV2	640	419	0.03%	0.004%
63	9.381	2591	2594	2598	rBV	690	490	0.03%	0.004%
64	9.426	2604	2608	2610	rBV2	509	336	0.02%	0.003%
65	9.526	2636	2639	2641	rBV2	397	246	0.02%	0.002%
66	9.731	2700	2703	2709	rBV4	543	497	0.03%	0.004%
67	9.773	2713	2716	2717	rBV2	396	226	0.02%	0.002%
68	9.850	2738	2740	2741	rBV2	778	310	0.02%	0.003%
69	9.899	2753	2755	2757	rBV2	604	298	0.02%	0.003%
70	10.011	2787	2790	2793	rBV3	877	533	0.04%	0.005%
71	10.053	2801	2803	2804	rBV	553	182	0.01%	0.002%
72	10.214	2839	2853	2878	rBV	488694	768908	52.14%	6.898%
73	10.445	2923	2925	2929	rVB3	1004	724	0.05%	0.006%
74	10.464	2929	2931	2934	rBV2	682	509	0.03%	0.005%
75	10.481	2934	2936	2938	rVB	609	238	0.02%	0.002%
76	10.497	2938	2941	2944	rBV3	836	460	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028044.D
 Acq On : 22 Sep 2022 03:32
 Operator : SY/MD
 Sample : N4659-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.638	2983	2985	2987	rBV2	423	248	0.02%	0.002%
78	10.696	2998	3003	3004	rBV3	909	478	0.03%	0.004%
79	10.757	3020	3022	3026	rBV4	674	534	0.04%	0.005%
80	10.805	3034	3037	3040	rBV3	532	401	0.03%	0.004%
81	11.005	3097	3099	3101	rBV2	486	273	0.02%	0.002%
82	11.136	3137	3140	3142	rBV3	1095	675	0.05%	0.006%
83	11.185	3154	3155	3162	rVB3	844	693	0.05%	0.006%
84	11.246	3162	3174	3196	rBV	558248	849942	57.63%	7.625%
85	11.622	3279	3291	3322	rVB	630875	999351	67.76%	8.966%
86	11.895	3373	3376	3380	rBV3	654	745	0.05%	0.007%
87	12.326	3505	3510	3513	rBV4	785	816	0.06%	0.007%
88	12.455	3548	3550	3554	rBV4	676	524	0.04%	0.005%
89	12.564	3582	3584	3586	rBV2	663	239	0.02%	0.002%
90	12.590	3590	3592	3594	rBV2	585	319	0.02%	0.003%
91	12.628	3602	3604	3607	rVB	725	438	0.03%	0.004%
92	12.786	3651	3653	3656	rVB2	740	421	0.03%	0.004%
93	12.841	3667	3670	3674	rBV3	631	450	0.03%	0.004%
94	12.995	3715	3718	3722	rVB2	718	529	0.04%	0.005%
95	13.021	3722	3726	3729	rBV3	619	505	0.03%	0.005%
96	13.207	3782	3784	3786	rBV2	563	219	0.01%	0.002%
97	13.275	3803	3805	3807	rBV2	637	304	0.02%	0.003%
98	13.445	3854	3858	3861	rBV2	658	422	0.03%	0.004%
99	13.706	3936	3939	3941	rBV2	509	293	0.02%	0.003%
100	14.397	4147	4154	4163	rVB4	10597	15361	1.04%	0.138%




Sum of corrected areas: 11146325

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028044.D
Acq On : 22 Sep 2022 03:32
Operator : SY/MD
Sample : N4659-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

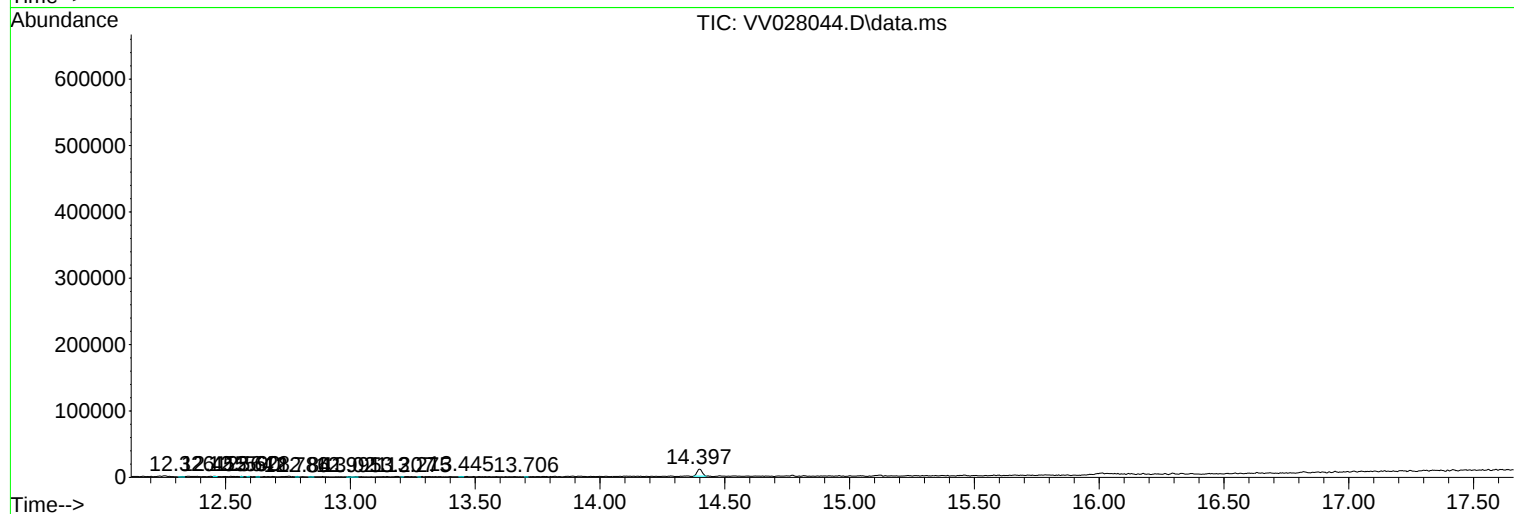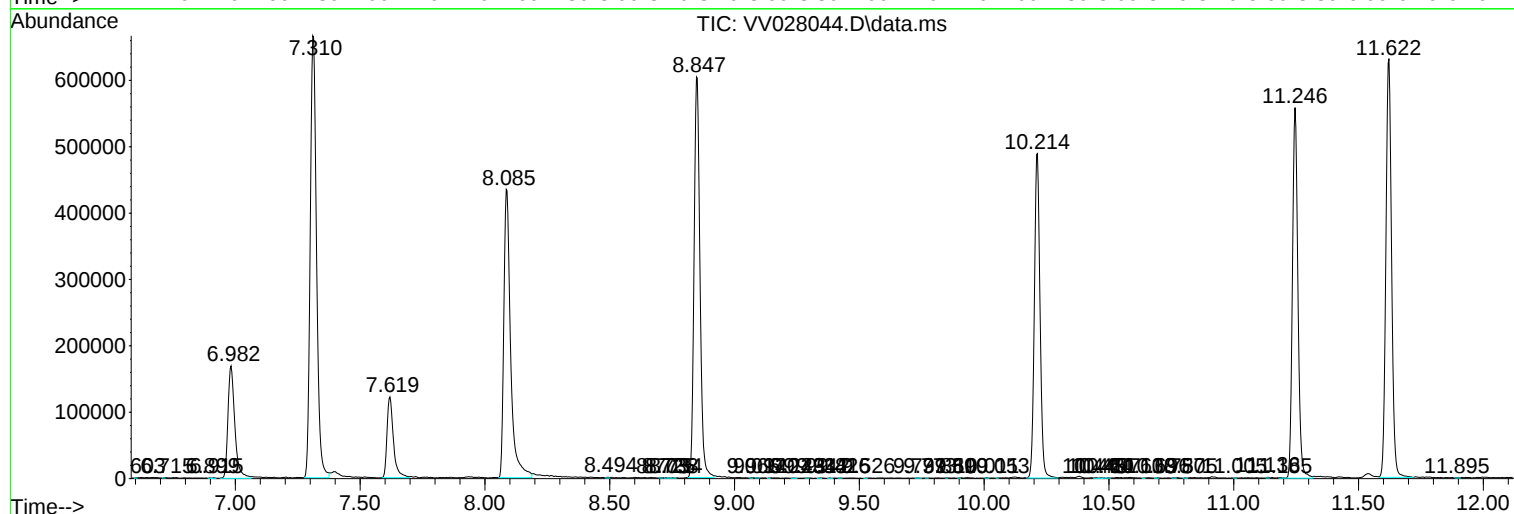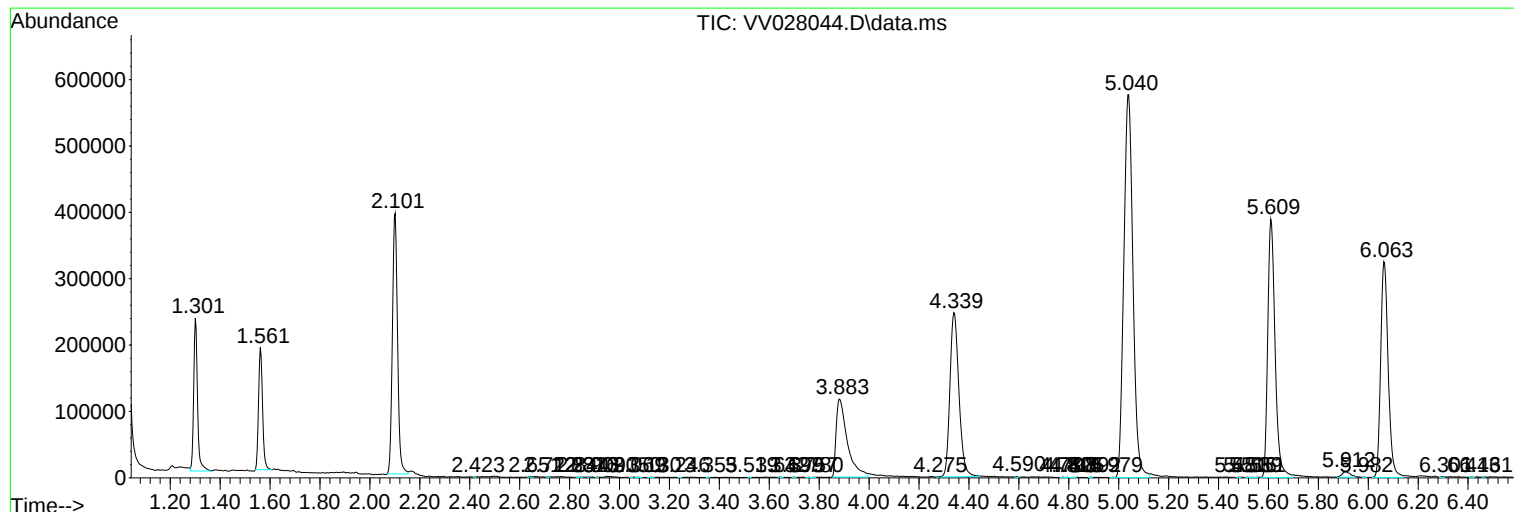

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028044.D
Acq On : 22 Sep 2022 03:32
Operator : SY/MD
Sample : N4659-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028044.D
Acq On : 22 Sep 2022 03:32
Operator : SY/MD
Sample : N4659-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------