

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028045.D
 Acq On : 22 Sep 2022 03:56
 Operator : SY/MD
 Sample : N4659-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	101	rVB	233831	248310	16.63%	2.251%
2	1.561	156	162	177	rVB	180254	203904	13.66%	1.849%
3	2.101	320	330	356	rVB	386082	565346	37.86%	5.125%
4	2.670	504	507	510	rBV3	466	325	0.02%	0.003%
5	2.693	510	514	517	rBV3	597	537	0.04%	0.005%
6	2.748	527	531	535	rBV3	869	648	0.04%	0.006%
7	2.847	559	562	563	rBV2	324	195	0.01%	0.002%
8	2.953	587	595	600	rBV4	1060	1902	0.13%	0.017%
9	3.021	610	616	617	rBV2	702	404	0.03%	0.004%
10	3.050	622	625	627	rBV2	407	249	0.02%	0.002%
11	3.085	634	636	638	rBV2	473	207	0.01%	0.002%
12	3.182	664	666	670	rBV2	416	346	0.02%	0.003%
13	3.214	674	676	679	rVB3	779	425	0.03%	0.004%
14	3.236	679	683	684	rBV	489	313	0.02%	0.003%
15	3.268	691	693	697	rVB4	511	207	0.01%	0.002%
16	3.307	700	705	706	rBV3	502	428	0.03%	0.004%
17	3.375	724	726	732	rBV3	337	235	0.02%	0.002%
18	3.413	735	738	740	rBV	453	278	0.02%	0.003%
19	3.449	747	749	752	rVB3	502	293	0.02%	0.003%
20	3.561	782	784	786	rVB2	486	248	0.02%	0.002%
21	3.600	792	796	797	rBV	307	221	0.01%	0.002%
22	3.680	819	821	826	rVB2	415	236	0.02%	0.002%
23	3.725	833	835	836	rBV2	560	254	0.02%	0.002%
24	3.802	853	859	863	rVB5	551	600	0.04%	0.005%
25	3.886	874	885	919	rBV	105593	348958	23.37%	3.164%
26	4.339	1012	1026	1059	rVB	239376	597903	40.04%	5.421%
27	4.773	1159	1161	1166	rBV2	488	396	0.03%	0.004%
28	4.883	1188	1195	1196	rBV2	499	358	0.02%	0.003%
29	4.911	1200	1204	1207	rVV2	393	375	0.03%	0.003%
30	4.976	1219	1224	1225	rBV2	399	316	0.02%	0.003%
31	5.040	1227	1244	1275	rBV2	584342	1493216	100.00%	13.538%
32	5.442	1367	1369	1375	rVB2	640	411	0.03%	0.004%
33	5.609	1409	1421	1449	rBV	381562	783350	52.46%	7.102%
34	5.915	1504	1516	1531	rBV8	12501	30042	2.01%	0.272%
35	6.063	1548	1562	1587	rBV	337568	694182	46.49%	6.293%
36	6.410	1667	1670	1672	rBV3	525	283	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028045.D
 Acq On : 22 Sep 2022 03:56
 Operator : SY/MD
 Sample : N4659-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.796	1788	1790	1792	rBV2	625	357	0.02%	0.003%
38	6.844	1803	1805	1807	rVB2	563	181	0.01%	0.002%
39	6.882	1815	1817	1821	rBV3	422	325	0.02%	0.003%
40	6.918	1824	1828	1829	rBV2	570	296	0.02%	0.003%
41	6.982	1836	1848	1875	rBV	165641	309924	20.76%	2.810%
42	7.198	1913	1915	1919	rBV6	900	562	0.04%	0.005%
43	7.310	1938	1950	1970	rBV	658387	1150784	77.07%	10.433%
44	7.619	2037	2046	2064	rBV	120837	204540	13.70%	1.854%
45	7.882	2124	2128	2130	rBV3	724	630	0.04%	0.006%
46	8.085	2181	2191	2225	rBV	435630	825354	55.27%	7.483%
47	8.538	2326	2332	2337	rBV5	770	929	0.06%	0.008%
48	8.593	2345	2349	2351	rBV5	494	426	0.03%	0.004%
49	8.657	2365	2369	2372	rBV4	590	435	0.03%	0.004%
50	8.847	2417	2428	2451	rBV	576255	948235	63.50%	8.597%
51	9.185	2530	2533	2534	rBV2	663	335	0.02%	0.003%
52	9.294	2565	2567	2570	rVB2	501	253	0.02%	0.002%
53	9.313	2570	2573	2580	rVB4	836	805	0.05%	0.007%
54	9.368	2588	2590	2592	rBV	466	193	0.01%	0.002%
55	9.432	2607	2610	2611	rBV	875	417	0.03%	0.004%
56	9.471	2620	2622	2625	rVB2	871	502	0.03%	0.005%
57	9.487	2625	2627	2629	rBV2	599	295	0.02%	0.003%
58	9.545	2643	2645	2648	rBV3	767	346	0.02%	0.003%
59	9.657	2678	2680	2683	rBV2	615	259	0.02%	0.002%
60	9.815	2725	2729	2733	rBV4	912	745	0.05%	0.007%
61	9.908	2756	2758	2761	rBV3	284	195	0.01%	0.002%
62	9.931	2762	2765	2766	rBV2	625	317	0.02%	0.003%
63	10.037	2796	2798	2802	rVB2	702	481	0.03%	0.004%
64	10.059	2803	2805	2809	rBV2	797	653	0.04%	0.006%
65	10.104	2816	2819	2820	rBV2	1373	721	0.05%	0.007%
66	10.214	2840	2853	2871	rVV	480754	768303	51.45%	6.965%
67	10.509	2943	2945	2948	rBV	518	230	0.02%	0.002%
68	10.599	2969	2973	2979	rBV6	1143	1153	0.08%	0.010%
69	10.722	3009	3011	3013	rBV2	452	221	0.01%	0.002%
70	10.767	3022	3025	3026	rBV2	533	320	0.02%	0.003%
71	10.818	3038	3041	3043	rBV2	792	516	0.03%	0.005%
72	10.853	3050	3052	3054	rBV3	974	573	0.04%	0.005%
73	10.905	3065	3068	3069	rBV3	1108	648	0.04%	0.006%
74	10.959	3081	3085	3087	rBV	573	392	0.03%	0.004%
75	10.972	3087	3089	3092	rVV2	748	400	0.03%	0.004%
76	11.033	3103	3108	3113	rBV5	649	867	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028045.D
 Acq On : 22 Sep 2022 03:56
 Operator : SY/MD
 Sample : N4659-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.101	3126	3129	3132	rBV2	683	562	0.04%	0.005%
78	11.143	3137	3142	3144	rBV4	1653	1527	0.10%	0.014%
79	11.168	3148	3150	3153	rBV2	675	381	0.03%	0.003%
80	11.246	3163	3174	3192	rBV	546027	832176	55.73%	7.545%
81	11.474	3243	3245	3247	rBV2	648	271	0.02%	0.002%
82	11.622	3280	3291	3310	rBV	641411	987516	66.13%	8.953%
83	12.066	3426	3429	3434	rVB4	781	764	0.05%	0.007%
84	12.146	3452	3454	3457	rBV4	647	430	0.03%	0.004%
85	12.310	3501	3505	3506	rBV2	784	548	0.04%	0.005%
86	12.336	3511	3513	3516	rBV2	667	332	0.02%	0.003%
87	12.368	3521	3523	3525	rBV2	678	364	0.02%	0.003%
88	12.432	3541	3543	3546	rVB2	913	377	0.03%	0.003%
89	12.651	3609	3611	3613	rBV	642	395	0.03%	0.004%
90	12.686	3620	3622	3626	rBV2	636	330	0.02%	0.003%
91	12.940	3697	3701	3702	rBV3	544	288	0.02%	0.003%
92	13.204	3781	3783	3784	rBV	697	357	0.02%	0.003%
93	13.445	3856	3858	3860	rVB2	708	263	0.02%	0.002%
94	13.754	3952	3954	3959	rVB3	644	352	0.02%	0.003%
95	13.786	3962	3964	3965	rBV	623	234	0.02%	0.002%
96	14.001	4029	4031	4035	rVB2	629	421	0.03%	0.004%
97	14.030	4038	4040	4043	rVV2	458	272	0.02%	0.002%
98	14.397	4151	4154	4155	rBV2	2212	1476	0.10%	0.013%
99	14.545	4196	4200	4203	rBV5	894	880	0.06%	0.008%
100	14.705	4248	4250	4254	rVB4	797	639	0.04%	0.006%




Sum of corrected areas: 11030174

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028045.D
Acq On : 22 Sep 2022 03:56
Operator : SY/MD
Sample : N4659-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

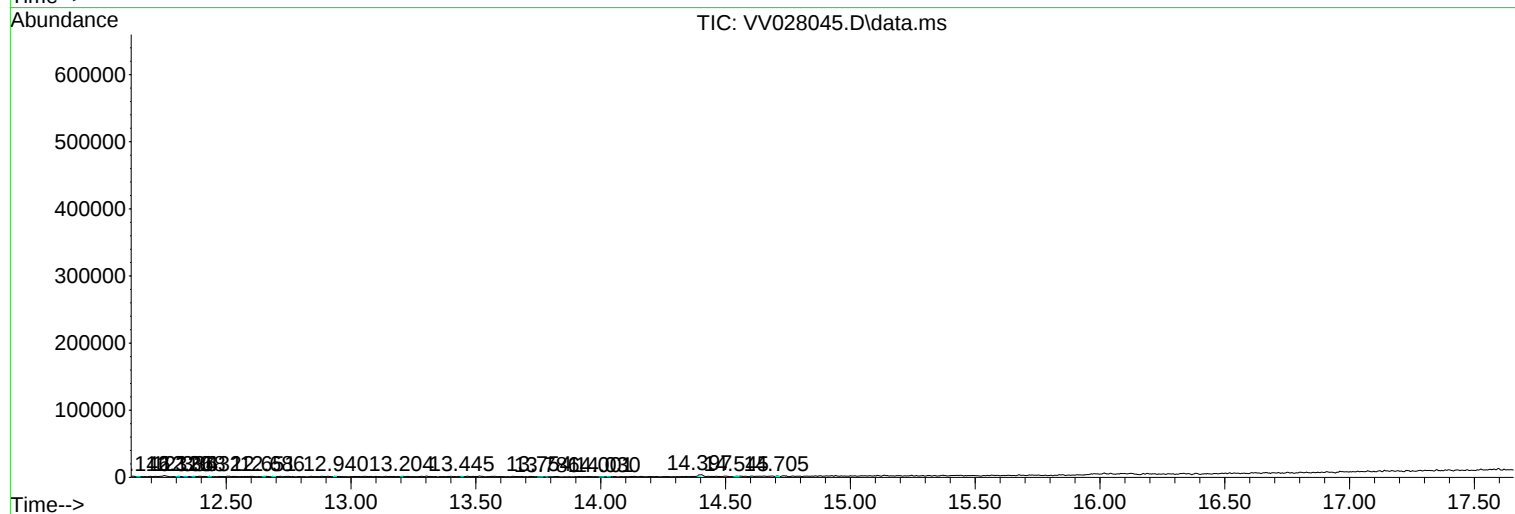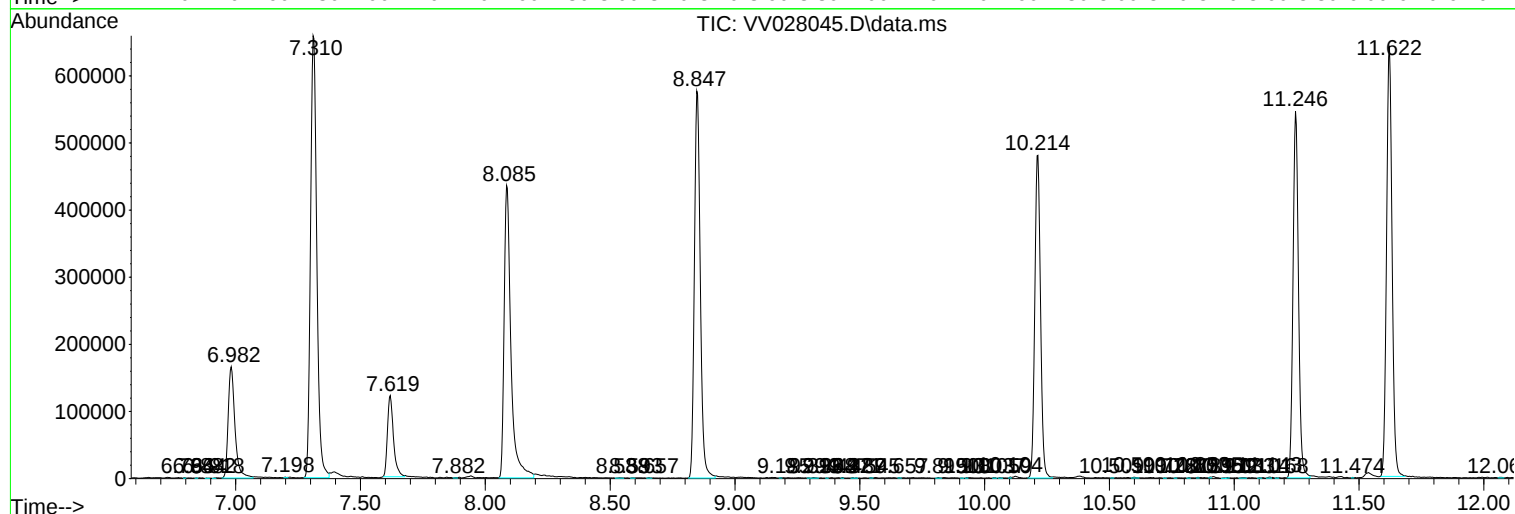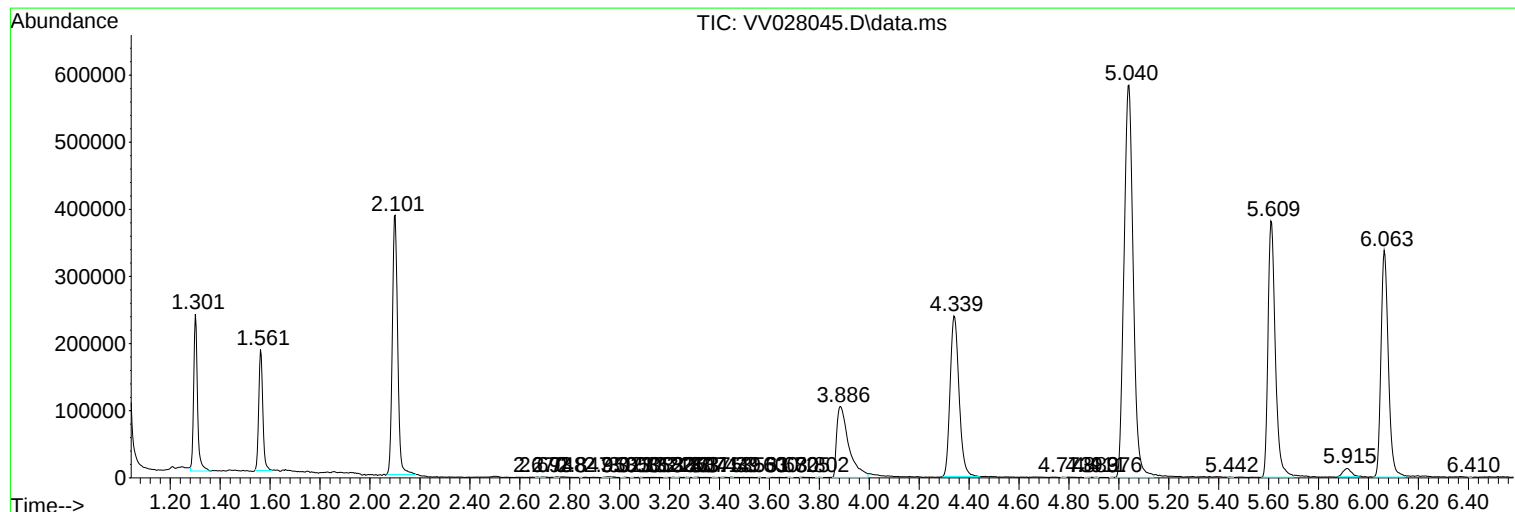

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028045.D
Acq On : 22 Sep 2022 03:56
Operator : SY/MD
Sample : N4659-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028045.D
Acq On : 22 Sep 2022 03:56
Operator : SY/MD
Sample : N4659-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------