

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028046.D
 Acq On : 22 Sep 2022 04:21
 Operator : SY/MD
 Sample : N4659-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV028046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	98	rVB	232607	238612	15.44%	2.093%
2	1.561	156	162	174	rVB	185105	204517	13.23%	1.794%
3	2.098	320	329	356	rVB	391888	572708	37.06%	5.024%
4	2.497	448	453	454	rBV3	1119	919	0.06%	0.008%
5	2.532	461	464	466	rBV3	581	336	0.02%	0.003%
6	2.635	492	496	498	rVB2	465	333	0.02%	0.003%
7	2.655	498	502	508	rBV4	978	1066	0.07%	0.009%
8	2.716	517	521	522	rBV2	397	309	0.02%	0.003%
9	3.114	639	645	649	rVB4	664	646	0.04%	0.006%
10	3.150	649	656	657	rBV3	583	412	0.03%	0.004%
11	3.169	658	662	666	rBV2	681	672	0.04%	0.006%
12	3.355	715	720	724	rVB3	797	663	0.04%	0.006%
13	3.381	725	728	729	rBV2	763	307	0.02%	0.003%
14	3.478	756	758	761	rBV	434	280	0.02%	0.002%
15	3.732	835	837	840	rBV2	404	305	0.02%	0.003%
16	3.822	861	865	867	rBV2	377	223	0.01%	0.002%
17	3.883	873	884	919	rBV	113677	364751	23.60%	3.200%
18	4.153	964	968	973	rBV5	1025	1115	0.07%	0.010%
19	4.339	1011	1026	1056	rBV	239218	589290	38.13%	5.170%
20	4.500	1074	1076	1083	rVB3	1069	734	0.05%	0.006%
21	4.561	1094	1095	1097	rBV2	624	258	0.02%	0.002%
22	4.664	1125	1127	1131	rBV3	719	376	0.02%	0.003%
23	4.786	1161	1165	1167	rBV2	561	399	0.03%	0.004%
24	4.802	1167	1170	1172	rBV2	567	245	0.02%	0.002%
25	4.815	1172	1174	1175	rBV	480	253	0.02%	0.002%
26	4.880	1188	1194	1196	rBV4	520	603	0.04%	0.005%
27	5.040	1227	1244	1276	rVV2	605108	1545364	100.00%	13.557%
28	5.310	1326	1328	1329	rBV2	779	330	0.02%	0.003%
29	5.416	1359	1361	1363	rBV2	565	290	0.02%	0.003%
30	5.609	1409	1421	1448	rBV	403316	824448	53.35%	7.232%
31	5.912	1503	1515	1532	rBV3	92870	191478	12.39%	1.680%
32	6.063	1549	1562	1583	rBV	344659	702681	45.47%	6.164%
33	6.294	1632	1634	1635	rBV3	536	218	0.01%	0.002%
34	6.362	1653	1655	1657	rBV2	663	295	0.02%	0.003%
35	6.413	1668	1671	1674	rVB2	672	361	0.02%	0.003%
36	6.452	1680	1683	1689	rBV5	806	769	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028046.D
 Acq On : 22 Sep 2022 04:21
 Operator : SY/MD
 Sample : N4659-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.497	1694	1697	1699	rBV4	592	389	0.03%	0.003%
38	6.645	1734	1743	1746	rBV6	1033	1210	0.08%	0.011%
39	6.661	1746	1748	1754	rVB3	610	597	0.04%	0.005%
40	6.892	1815	1820	1821	rBV3	261	244	0.02%	0.002%
41	6.982	1837	1848	1874	rBV	156667	297003	19.22%	2.605%
42	7.188	1908	1912	1914	rBV3	845	547	0.04%	0.005%
43	7.310	1936	1950	1971	rBV	643470	1131866	73.24%	9.929%
44	7.619	2036	2046	2062	rBV	119802	210705	13.63%	1.848%
45	7.924	2139	2141	2143	rBV2	1266	717	0.05%	0.006%
46	8.002	2162	2165	2166	rBV3	1117	475	0.03%	0.004%
47	8.085	2181	2191	2228	rBV	444798	845202	54.69%	7.414%
48	8.477	2310	2313	2314	rBV2	823	561	0.04%	0.005%
49	8.703	2381	2383	2384	rBV2	600	210	0.01%	0.002%
50	8.780	2406	2407	2411	rBV3	494	321	0.02%	0.003%
51	8.847	2417	2428	2449	rBV	622308	1006038	65.10%	8.825%
52	9.095	2503	2505	2507	rBV3	1041	542	0.04%	0.005%
53	9.246	2548	2552	2553	rBV3	848	625	0.04%	0.005%
54	9.420	2604	2606	2608	rBV	750	413	0.03%	0.004%
55	9.545	2638	2645	2647	rBV5	1309	1286	0.08%	0.011%
56	9.706	2693	2695	2698	rVB2	666	259	0.02%	0.002%
57	9.802	2721	2725	2728	rBV4	765	535	0.03%	0.005%
58	9.828	2730	2733	2736	rBV	1016	653	0.04%	0.006%
59	9.863	2741	2744	2745	rBV	469	207	0.01%	0.002%
60	9.905	2755	2757	2760	rBV3	914	554	0.04%	0.005%
61	9.960	2771	2774	2777	rBV2	655	463	0.03%	0.004%
62	10.059	2801	2805	2807	rBV	569	422	0.03%	0.004%
63	10.120	2816	2824	2830	rBV9	2192	3753	0.24%	0.033%
64	10.214	2841	2853	2872	rVV	497694	777469	50.31%	6.820%
65	10.374	2899	2903	2906	rBV7	1604	1547	0.10%	0.014%
66	10.474	2931	2934	2938	rBV3	352	281	0.02%	0.002%
67	10.693	2999	3002	3005	rBV3	646	497	0.03%	0.004%
68	10.744	3016	3018	3020	rBV2	569	248	0.02%	0.002%
69	10.915	3062	3071	3073	rBV6	2215	2862	0.19%	0.025%
70	10.976	3086	3090	3092	rBV3	756	530	0.03%	0.005%
71	11.072	3117	3120	3122	rVB3	837	394	0.03%	0.003%
72	11.088	3122	3125	3127	rBV3	845	565	0.04%	0.005%
73	11.101	3127	3129	3131	rBV2	544	293	0.02%	0.003%
74	11.137	3137	3140	3141	rBV3	830	455	0.03%	0.004%
75	11.246	3163	3174	3198	rBV	551390	859402	55.61%	7.539%
76	11.503	3252	3254	3256	rBV2	1044	460	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028046.D
 Acq On : 22 Sep 2022 04:21
 Operator : SY/MD
 Sample : N4659-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.622	3279	3291	3312	rBV	621992	991695	64.17%	8.700%
78	11.783	3336	3341	3342	rBV3	1074	852	0.06%	0.007%
79	11.821	3351	3353	3357	rBV4	504	410	0.03%	0.004%
80	11.937	3386	3389	3391	rBV2	435	264	0.02%	0.002%
81	12.030	3416	3418	3421	rVB3	466	251	0.02%	0.002%
82	12.059	3421	3427	3430	rBV3	625	693	0.04%	0.006%
83	12.091	3435	3437	3441	rVB	788	478	0.03%	0.004%
84	12.146	3452	3454	3458	rBV2	435	323	0.02%	0.003%
85	12.358	3516	3520	3530	rVB4	937	1191	0.08%	0.010%
86	12.461	3549	3552	3554	rBV	415	286	0.02%	0.003%
87	12.474	3554	3556	3560	rVB3	419	249	0.02%	0.002%
88	12.529	3571	3573	3575	rVB2	600	256	0.02%	0.002%
89	12.593	3590	3593	3597	rBV	444	434	0.03%	0.004%
90	12.686	3620	3622	3631	rVB2	417	436	0.03%	0.004%
91	12.834	3666	3668	3671	rBV2	489	245	0.02%	0.002%
92	12.870	3677	3679	3682	rVB2	1012	466	0.03%	0.004%
93	12.886	3682	3684	3686	rBV	825	509	0.03%	0.004%
94	12.934	3697	3699	3701	rBV	770	434	0.03%	0.004%
95	13.140	3761	3763	3765	rBV2	582	232	0.02%	0.002%
96	13.326	3819	3821	3824	rBV2	862	358	0.02%	0.003%
97	13.519	3878	3881	3882	rBV2	603	361	0.02%	0.003%
98	13.583	3899	3901	3903	rBV	789	323	0.02%	0.003%
99	14.320	4128	4130	4132	rBV2	800	488	0.03%	0.004%
100	15.046	4352	4356	4358	rBV2	1064	740	0.05%	0.006%




Sum of corrected areas: 11399340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028046.D
Acq On : 22 Sep 2022 04:21
Operator : SY/MD
Sample : N4659-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

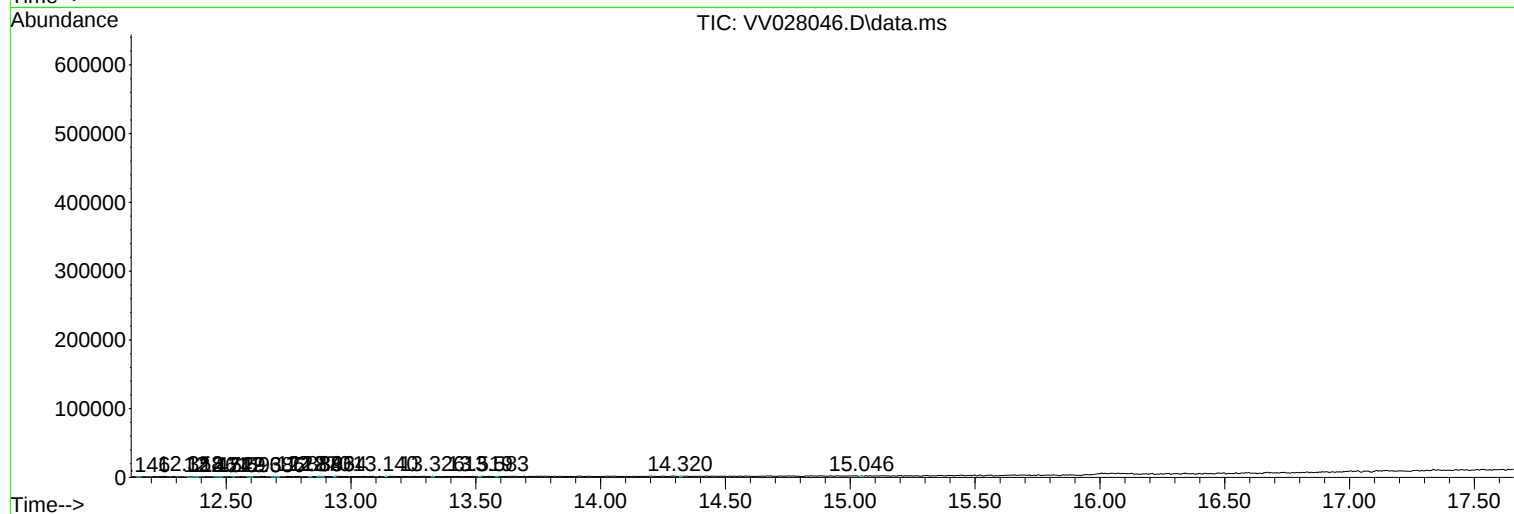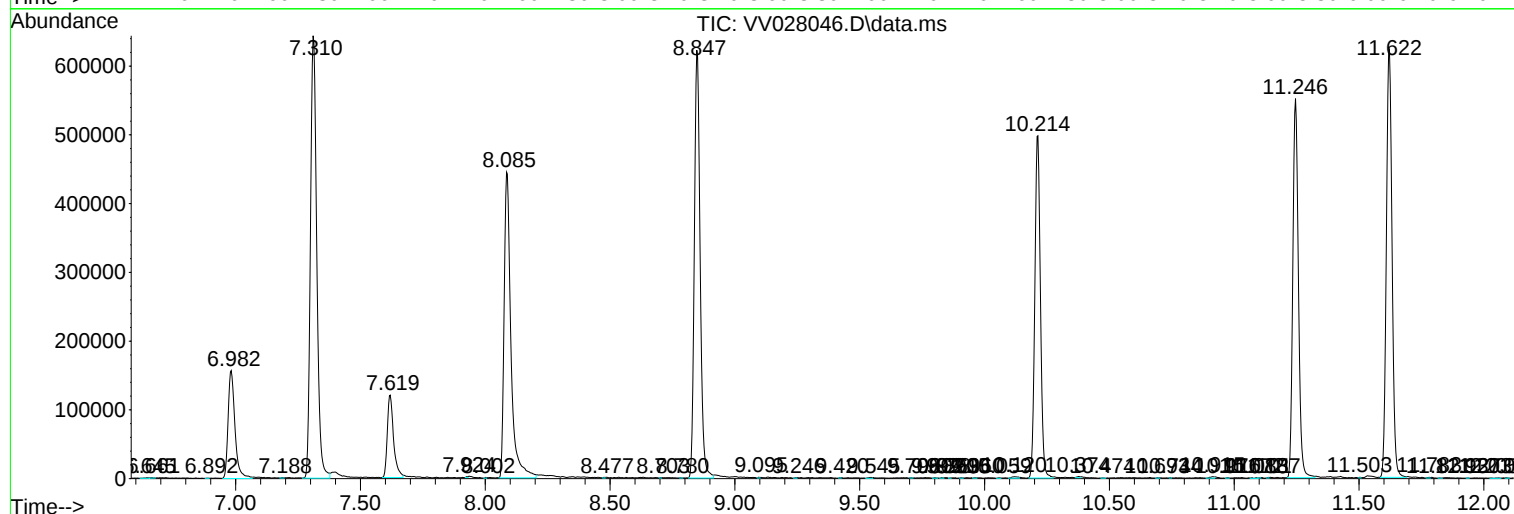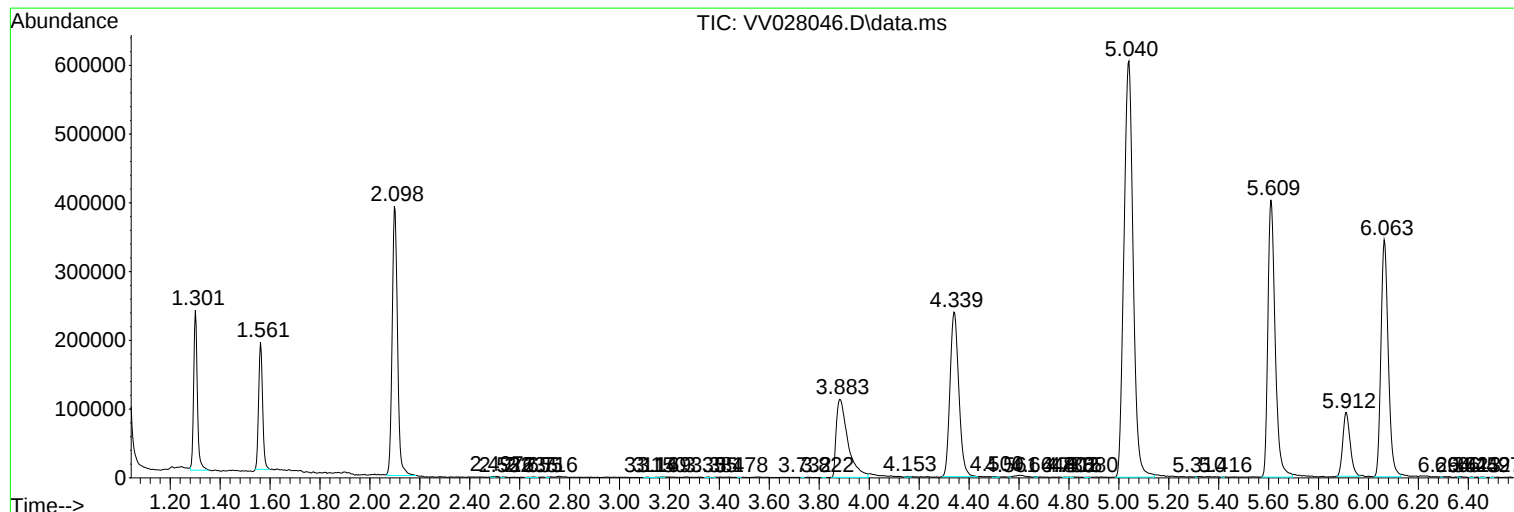

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028046.D
Acq On : 22 Sep 2022 04:21
Operator : SY/MD
Sample : N4659-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028046.D
Acq On : 22 Sep 2022 04:21
Operator : SY/MD
Sample : N4659-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc