

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028047.D
 Acq On : 22 Sep 2022 04:46
 Operator : SY/MD
 Sample : N4659-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV028047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	96	rVB	228461	234505	15.75%	2.135%
2	1.561	156	162	180	rVB	182989	207858	13.96%	1.892%
3	2.101	320	330	346	rBV	390815	564442	37.91%	5.139%
4	2.433	430	433	436	rBV2	792	503	0.03%	0.005%
5	2.494	449	452	463	rVB6	1655	2834	0.19%	0.026%
6	2.651	499	501	504	rBV3	550	336	0.02%	0.003%
7	2.937	586	590	591	rBV	557	396	0.03%	0.004%
8	2.979	601	603	608	rVB2	515	390	0.03%	0.004%
9	3.008	608	612	614	rBV2	382	343	0.02%	0.003%
10	3.092	635	638	642	rVB3	552	411	0.03%	0.004%
11	3.179	663	665	671	rVB4	566	443	0.03%	0.004%
12	3.298	698	702	704	rBV2	229	208	0.01%	0.002%
13	3.310	704	706	711	rVB2	582	394	0.03%	0.004%
14	3.397	731	733	736	rVB2	578	236	0.02%	0.002%
15	3.426	736	742	746	rBV4	576	637	0.04%	0.006%
16	3.532	773	775	778	rVB2	378	196	0.01%	0.002%
17	3.603	795	797	802	rVB	372	203	0.01%	0.002%
18	3.773	846	850	853	rBV2	500	485	0.03%	0.004%
19	3.844	869	872	874	rBV2	484	318	0.02%	0.003%
20	3.886	874	885	917	rBV2	105178	338618	22.74%	3.083%
21	4.339	1009	1026	1055	rBV2	236803	593693	39.87%	5.405%
22	4.561	1091	1095	1097	rBV	255	213	0.01%	0.002%
23	4.654	1123	1124	1126	rBV	485	212	0.01%	0.002%
24	4.693	1134	1136	1138	rBV2	531	207	0.01%	0.002%
25	4.706	1138	1140	1142	rVB2	569	207	0.01%	0.002%
26	4.802	1168	1170	1172	rBV2	612	270	0.02%	0.002%
27	4.921	1205	1207	1210	rBV2	407	226	0.02%	0.002%
28	5.040	1226	1244	1276	rBV2	582131	1489018	100.00%	13.556%
29	5.359	1341	1343	1345	rBV3	483	263	0.02%	0.002%
30	5.423	1360	1363	1367	rBV3	856	547	0.04%	0.005%
31	5.542	1395	1400	1405	rVB6	806	837	0.06%	0.008%
32	5.564	1405	1407	1409	rBV3	529	266	0.02%	0.002%
33	5.609	1409	1421	1457	rBV	384213	785943	52.78%	7.155%
34	5.822	1485	1487	1488	rBV2	775	317	0.02%	0.003%
35	5.908	1502	1514	1532	rVB2	7865	19044	1.28%	0.173%
36	5.973	1532	1534	1538	rBV3	671	529	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028047.D
 Acq On : 22 Sep 2022 04:46
 Operator : SY/MD
 Sample : N4659-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.998	1538	1542	1547	rBV7	1129	839	0.06%	0.008%
38	6.063	1549	1562	1591	rBV2	342989	695962	46.74%	6.336%
39	6.333	1642	1646	1648	rBV3	888	598	0.04%	0.005%
40	6.429	1675	1676	1678	rBV2	407	195	0.01%	0.002%
41	6.461	1684	1686	1690	rVB2	789	390	0.03%	0.004%
42	6.484	1690	1693	1694	rBV2	429	216	0.01%	0.002%
43	6.506	1697	1700	1701	rBV2	581	242	0.02%	0.002%
44	6.590	1722	1726	1728	rBV2	372	261	0.02%	0.002%
45	6.738	1769	1772	1773	rBV3	547	322	0.02%	0.003%
46	6.802	1788	1792	1795	rVV3	847	533	0.04%	0.005%
47	6.921	1825	1829	1832	rBV4	682	572	0.04%	0.005%
48	6.982	1838	1848	1867	rBV	164394	298629	20.06%	2.719%
49	7.310	1939	1950	1969	rBV	666048	1157131	77.71%	10.535%
50	7.619	2037	2046	2061	rBV	115646	199523	13.40%	1.816%
51	7.776	2093	2095	2099	rBV4	632	507	0.03%	0.005%
52	8.085	2177	2191	2231	rBV	419504	808313	54.28%	7.359%
53	8.567	2337	2341	2343	rBV3	1026	726	0.05%	0.007%
54	8.629	2357	2360	2361	rBV3	787	406	0.03%	0.004%
55	8.645	2361	2365	2367	rBV4	858	602	0.04%	0.005%
56	8.847	2417	2428	2453	rBV	585463	969175	65.09%	8.823%
57	9.108	2506	2509	2510	rBV3	1243	727	0.05%	0.007%
58	9.227	2544	2546	2554	rVB6	1047	1134	0.08%	0.010%
59	9.301	2567	2569	2572	rBV2	1061	556	0.04%	0.005%
60	9.391	2595	2597	2600	rVB3	890	372	0.02%	0.003%
61	9.474	2621	2623	2626	rBV2	747	510	0.03%	0.005%
62	9.519	2635	2637	2640	rVB	717	315	0.02%	0.003%
63	9.603	2660	2663	2665	rBV	705	522	0.04%	0.005%
64	9.715	2695	2698	2701	rBV2	769	571	0.04%	0.005%
65	9.825	2730	2732	2736	rVB3	513	340	0.02%	0.003%
66	9.854	2737	2741	2742	rBV	556	334	0.02%	0.003%
67	9.937	2765	2767	2769	rBV2	555	217	0.01%	0.002%
68	9.963	2774	2775	2778	rBV2	353	218	0.01%	0.002%
69	10.108	2817	2820	2821	rBV2	1039	606	0.04%	0.006%
70	10.214	2841	2853	2870	rBV	479950	764876	51.37%	6.963%
71	10.381	2900	2905	2912	rVB6	3141	4240	0.28%	0.039%
72	10.410	2912	2914	2918	rVB4	692	407	0.03%	0.004%
73	10.429	2918	2920	2923	rBV	398	197	0.01%	0.002%
74	10.442	2923	2924	2927	rVB	780	254	0.02%	0.002%
75	10.461	2927	2930	2931	rBV2	577	376	0.03%	0.003%
76	10.593	2969	2971	2973	rBV2	500	238	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028047.D
 Acq On : 22 Sep 2022 04:46
 Operator : SY/MD
 Sample : N4659-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.657	2989	2991	2995	rBV2	626	422	0.03%	0.004%
78	10.728	3008	3013	3017	rBV2	340	349	0.02%	0.003%
79	10.776	3026	3028	3030	rBV	433	254	0.02%	0.002%
80	10.876	3056	3059	3060	rBV2	321	204	0.01%	0.002%
81	11.008	3096	3100	3101	rBV	408	215	0.01%	0.002%
82	11.117	3129	3134	3135	rBV	351	232	0.02%	0.002%
83	11.133	3136	3139	3140	rBV2	1081	580	0.04%	0.005%
84	11.246	3163	3174	3197	rBV	534179	823354	55.30%	7.496%
85	11.500	3249	3253	3255	rBV4	986	714	0.05%	0.007%
86	11.532	3255	3263	3278	rBV10	5173	11389	0.76%	0.104%
87	11.622	3279	3291	3312	rVV	618600	981845	65.94%	8.939%
88	12.175	3461	3463	3467	rVB	650	289	0.02%	0.003%
89	12.201	3467	3471	3473	rBV2	796	700	0.05%	0.006%
90	12.484	3553	3559	3562	rBV5	1188	1215	0.08%	0.011%
91	12.641	3606	3608	3610	rBV	474	201	0.01%	0.002%
92	13.291	3809	3810	3816	rVB5	983	762	0.05%	0.007%
93	13.320	3816	3819	3820	rBV2	542	305	0.02%	0.003%
94	13.677	3926	3930	3932	rBV3	836	713	0.05%	0.006%
95	13.879	3989	3993	3996	rVB4	788	732	0.05%	0.007%
96	13.911	4001	4003	4005	rBV2	600	234	0.02%	0.002%
97	14.072	4050	4053	4055	rBV3	806	585	0.04%	0.005%
98	14.111	4063	4065	4067	rBV2	706	389	0.03%	0.004%
99	14.181	4085	4087	4092	rVB4	715	367	0.02%	0.003%
100	14.345	4136	4138	4141	rBV2	643	379	0.03%	0.003%




Sum of corrected areas: 10984129

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028047.D
Acq On : 22 Sep 2022 04:46
Operator : SY/MD
Sample : N4659-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

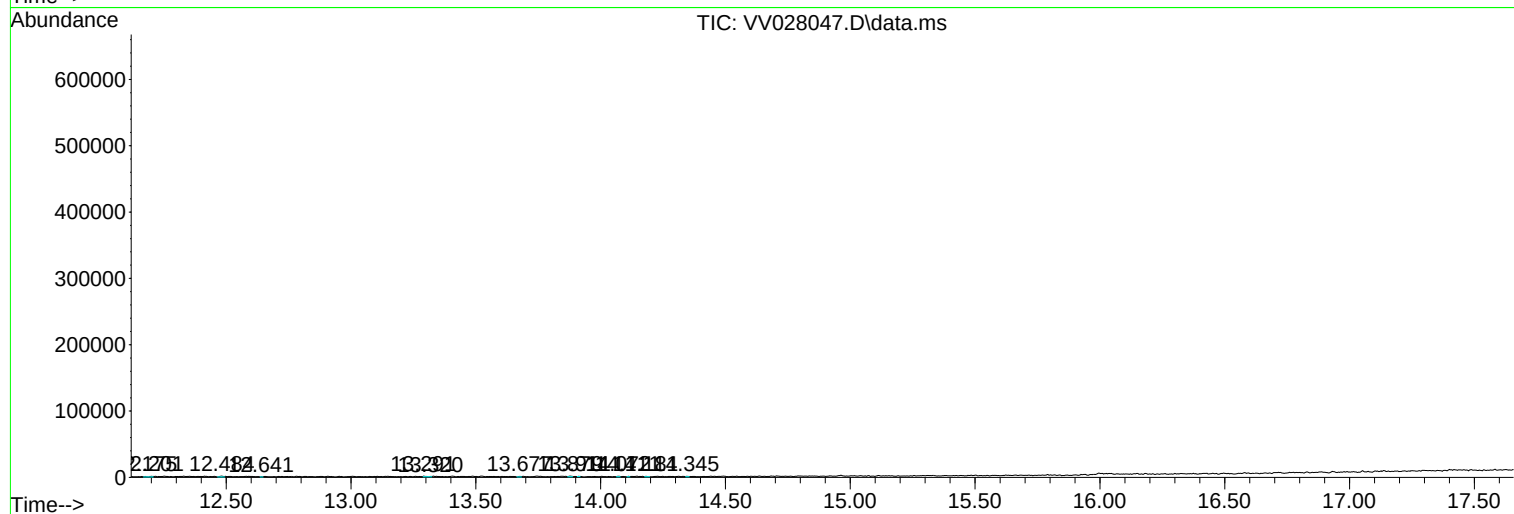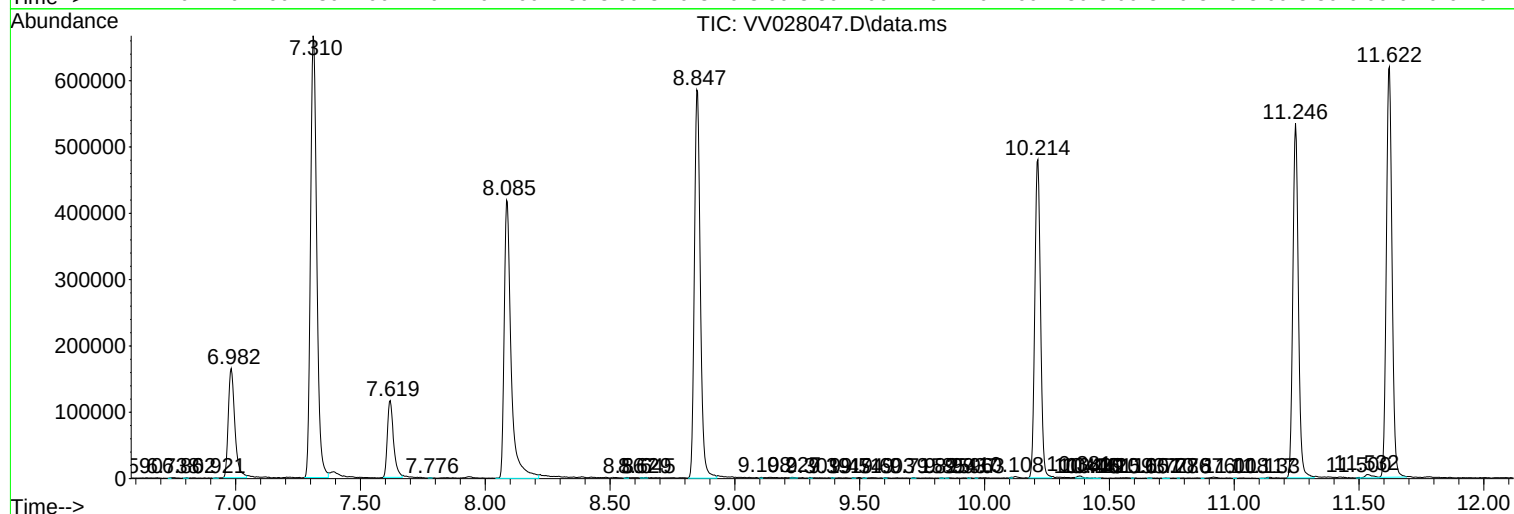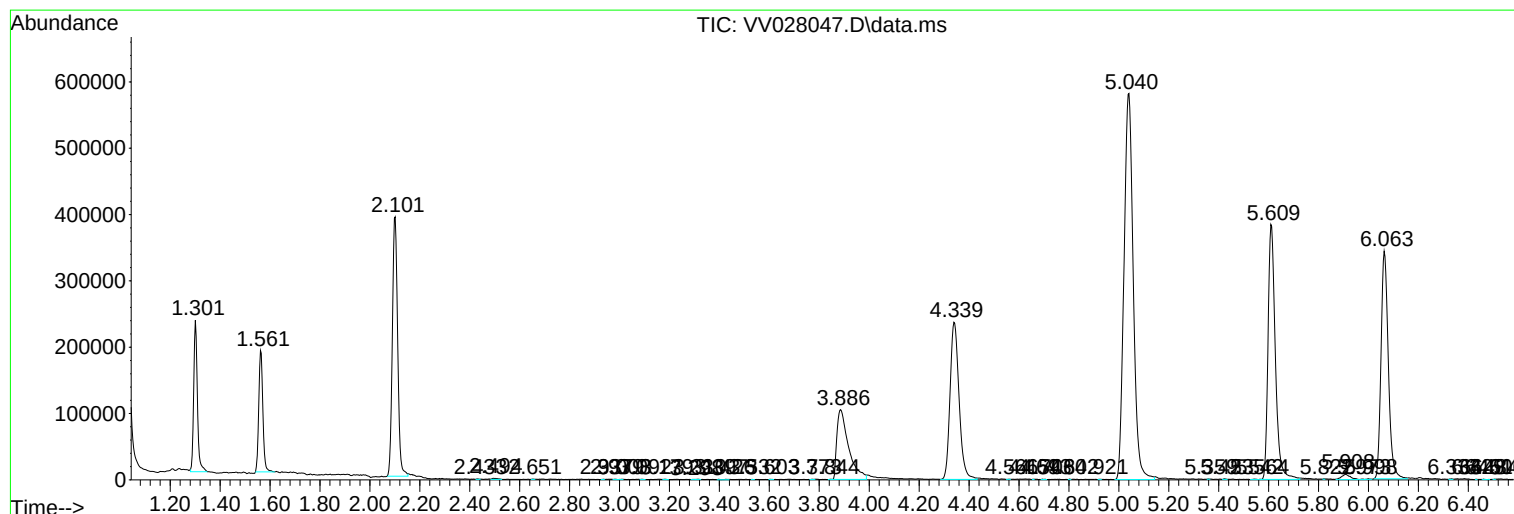

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028047.D
Acq On : 22 Sep 2022 04:46
Operator : SY/MD
Sample : N4659-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028047.D
Acq On : 22 Sep 2022 04:46
Operator : SY/MD
Sample : N4659-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc