

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028048.D
 Acq On : 22 Sep 2022 05:11
 Operator : SY/MD
 Sample : N4659-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV028048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	103	rVB	234692	245523	16.87%	2.257%
2	1.561	156	162	173	rBV	176095	198598	13.64%	1.826%
3	2.101	320	330	348	rBV	380342	549763	37.76%	5.055%
4	2.352	404	408	409	rBV2	733	455	0.03%	0.004%
5	2.580	476	479	480	rBV	749	419	0.03%	0.004%
6	2.667	502	506	508	rBV3	805	503	0.03%	0.005%
7	2.950	587	594	596	rBV4	2212	2299	0.16%	0.021%
8	2.998	607	609	612	rBV3	486	332	0.02%	0.003%
9	3.072	628	632	634	rBV2	476	389	0.03%	0.004%
10	3.104	639	642	647	rVB4	628	487	0.03%	0.004%
11	3.291	698	700	706	rVB3	790	594	0.04%	0.005%
12	3.320	706	709	711	rBV2	430	178	0.01%	0.002%
13	3.342	711	716	719	rBV4	449	437	0.03%	0.004%
14	3.400	731	734	736	rBV2	498	223	0.02%	0.002%
15	3.500	761	765	768	rBV3	388	319	0.02%	0.003%
16	3.580	787	790	792	rBV3	522	289	0.02%	0.003%
17	3.674	816	819	821	rBV	397	276	0.02%	0.003%
18	3.744	838	841	842	rBV	478	268	0.02%	0.002%
19	3.786	851	854	855	rBV	312	184	0.01%	0.002%
20	3.821	862	865	870	rBV3	414	313	0.02%	0.003%
21	3.850	870	874	875	rBV	511	330	0.02%	0.003%
22	3.886	875	885	915	rBV	105214	340182	23.37%	3.128%
23	4.339	1008	1026	1051	rBV	236346	584324	40.14%	5.373%
24	4.558	1092	1094	1095	rVB	622	180	0.01%	0.002%
25	4.571	1095	1098	1100	rBV3	985	728	0.05%	0.007%
26	4.651	1121	1123	1126	rVB2	785	469	0.03%	0.004%
27	4.667	1126	1128	1130	rBV2	546	330	0.02%	0.003%
28	4.767	1157	1159	1165	rVB3	792	580	0.04%	0.005%
29	4.796	1165	1168	1169	rBV2	839	433	0.03%	0.004%
30	4.873	1190	1192	1195	rBV4	449	250	0.02%	0.002%
31	4.918	1202	1206	1210	rBV4	485	468	0.03%	0.004%
32	4.960	1217	1219	1222	rBV3	515	282	0.02%	0.003%
33	5.040	1226	1244	1281	rBV2	567616	1455803	100.00%	13.386%
34	5.506	1387	1389	1390	rBV2	613	201	0.01%	0.002%
35	5.555	1402	1404	1406	rBV2	383	188	0.01%	0.002%
36	5.609	1410	1421	1451	rVV	390340	795659	54.65%	7.316%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028048.D
 Acq On : 22 Sep 2022 05:11
 Operator : SY/MD
 Sample : N4659-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.908	1504	1514	1523	rBV10	6326	13820	0.95%	0.127%
38	5.982	1536	1537	1540	rVB	823	250	0.02%	0.002%
39	6.063	1548	1562	1593	rBV	332321	688461	47.29%	6.330%
40	6.384	1660	1662	1666	rVB2	917	414	0.03%	0.004%
41	6.410	1666	1670	1672	rBV4	1295	918	0.06%	0.008%
42	6.490	1693	1695	1698	rBV2	686	355	0.02%	0.003%
43	6.542	1709	1711	1713	rBV2	698	336	0.02%	0.003%
44	6.651	1743	1745	1747	rBV	842	523	0.04%	0.005%
45	6.747	1772	1775	1777	rBV3	823	525	0.04%	0.005%
46	6.879	1814	1816	1818	rBV	404	229	0.02%	0.002%
47	6.895	1818	1821	1824	rVV2	974	549	0.04%	0.005%
48	6.934	1831	1833	1835	rBV2	631	333	0.02%	0.003%
49	6.982	1837	1848	1873	rVV	160209	296350	20.36%	2.725%
50	7.259	1931	1934	1936	rBV3	944	549	0.04%	0.005%
51	7.310	1939	1950	1970	rBV	644090	1128968	77.55%	10.380%
52	7.619	2036	2046	2069	rBV	111443	197059	13.54%	1.812%
53	7.853	2117	2119	2124	rVB4	1339	706	0.05%	0.006%
54	8.088	2181	2192	2225	rBV	403589	779144	53.52%	7.164%
55	8.644	2361	2365	2367	rBV3	677	661	0.05%	0.006%
56	8.677	2372	2375	2377	rVB3	662	394	0.03%	0.004%
57	8.847	2417	2428	2453	rBV	611080	1005222	69.05%	9.243%
58	9.021	2479	2482	2484	rBV3	1490	970	0.07%	0.009%
59	9.265	2554	2558	2560	rBV3	596	395	0.03%	0.004%
60	9.342	2580	2582	2588	rVB3	616	467	0.03%	0.004%
61	9.381	2588	2594	2600	rBV5	1046	1273	0.09%	0.012%
62	9.426	2607	2608	2613	rVB3	650	294	0.02%	0.003%
63	9.448	2613	2615	2618	rBV	483	252	0.02%	0.002%
64	9.484	2624	2626	2628	rBV2	658	341	0.02%	0.003%
65	9.532	2638	2641	2643	rBV	590	257	0.02%	0.002%
66	9.632	2670	2672	2674	rVB2	713	233	0.02%	0.002%
67	9.796	2722	2723	2725	rBV2	533	206	0.01%	0.002%
68	9.818	2728	2730	2731	rBV	421	231	0.02%	0.002%
69	9.837	2735	2736	2740	rVB2	698	342	0.02%	0.003%
70	9.860	2740	2743	2745	rBV3	669	519	0.04%	0.005%
71	10.120	2819	2824	2834	rVB6	2023	2685	0.18%	0.025%
72	10.213	2841	2853	2872	rBV	459747	726346	49.89%	6.678%
73	10.361	2896	2899	2900	rBV2	1125	634	0.04%	0.006%
74	10.426	2917	2919	2923	rBV3	566	399	0.03%	0.004%
75	10.458	2926	2929	2931	rBV	260	201	0.01%	0.002%
76	10.538	2952	2954	2958	rBV	445	308	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028048.D
 Acq On : 22 Sep 2022 05:11
 Operator : SY/MD
 Sample : N4659-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.567	2961	2963	2967	rBV2	468	289	0.02%	0.003%
78	10.754	3019	3021	3024	rBV3	299	188	0.01%	0.002%
79	10.914	3064	3071	3073	rBV3	1536	1470	0.10%	0.014%
80	10.982	3089	3092	3093	rBV	414	183	0.01%	0.002%
81	11.030	3103	3107	3108	rBV	546	381	0.03%	0.004%
82	11.246	3163	3174	3195	rBV	559335	860568	59.11%	7.913%
83	11.496	3250	3252	3255	rBV2	770	425	0.03%	0.004%
84	11.622	3280	3291	3316	rBV	617651	970712	66.68%	8.925%
85	12.066	3427	3429	3431	rBV2	516	279	0.02%	0.003%
86	12.217	3473	3476	3479	rBV2	735	554	0.04%	0.005%
87	12.529	3569	3573	3576	rBV3	1135	904	0.06%	0.008%
88	12.625	3601	3603	3604	rBV2	717	252	0.02%	0.002%
89	12.670	3615	3617	3621	rBV2	689	418	0.03%	0.004%
90	12.699	3624	3626	3632	rVB2	826	563	0.04%	0.005%
91	12.824	3662	3665	3668	rBV3	563	494	0.03%	0.005%
92	13.101	3749	3751	3756	rVB3	1066	694	0.05%	0.006%
93	13.123	3756	3758	3759	rBV	706	344	0.02%	0.003%
94	13.246	3794	3796	3798	rVB	617	237	0.02%	0.002%
95	13.307	3813	3815	3818	rBV4	751	490	0.03%	0.005%
96	13.371	3832	3835	3837	rBV	659	462	0.03%	0.004%
97	14.065	4049	4051	4052	rBV	867	375	0.03%	0.003%
98	14.262	4110	4112	4113	rBV	865	356	0.02%	0.003%
99	14.364	4143	4144	4146	rBV	825	372	0.03%	0.003%
100	14.461	4172	4174	4176	rBV3	855	530	0.04%	0.005%




Sum of corrected areas: 10875915

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028048.D
Acq On : 22 Sep 2022 05:11
Operator : SY/MD
Sample : N4659-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

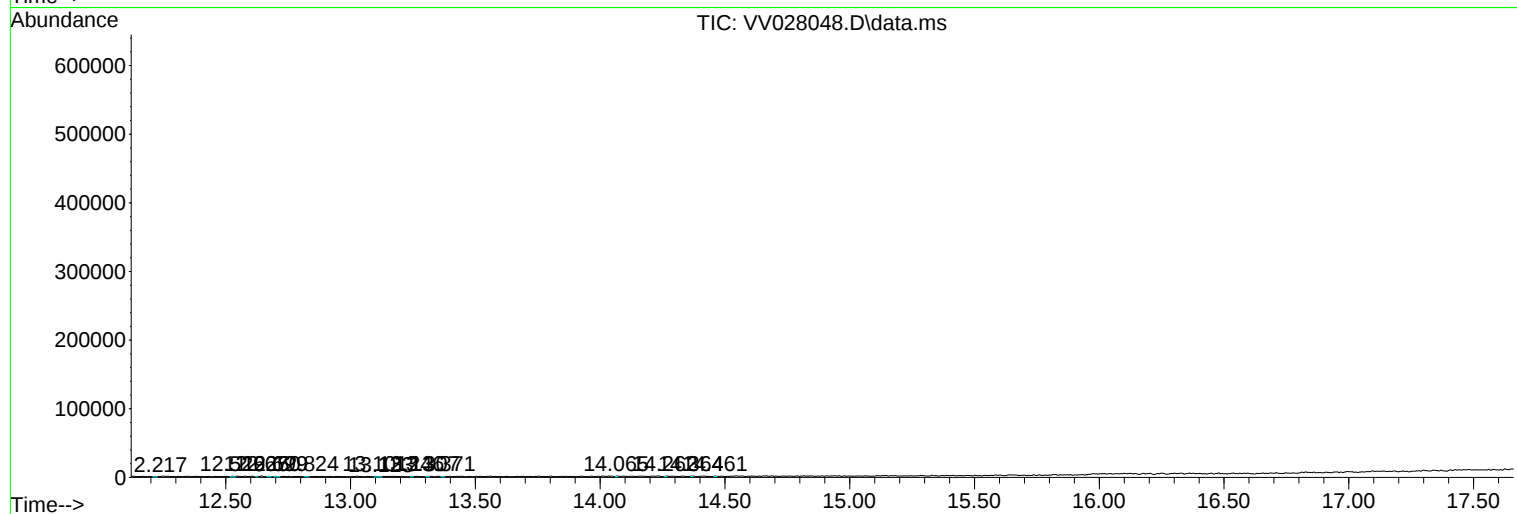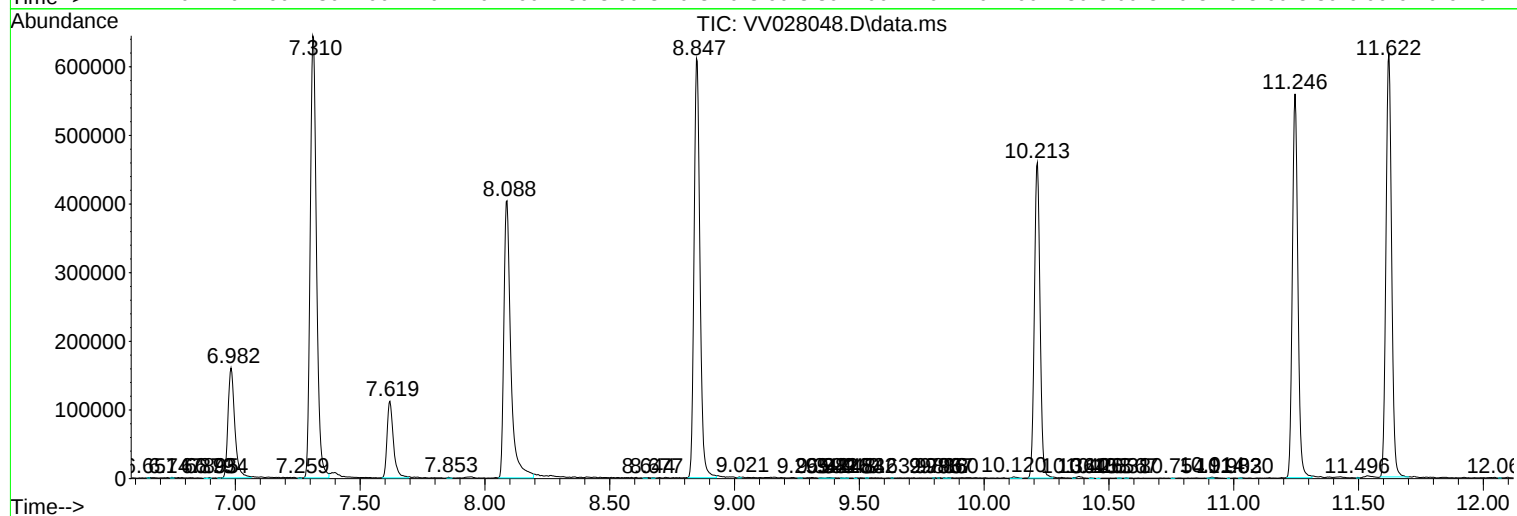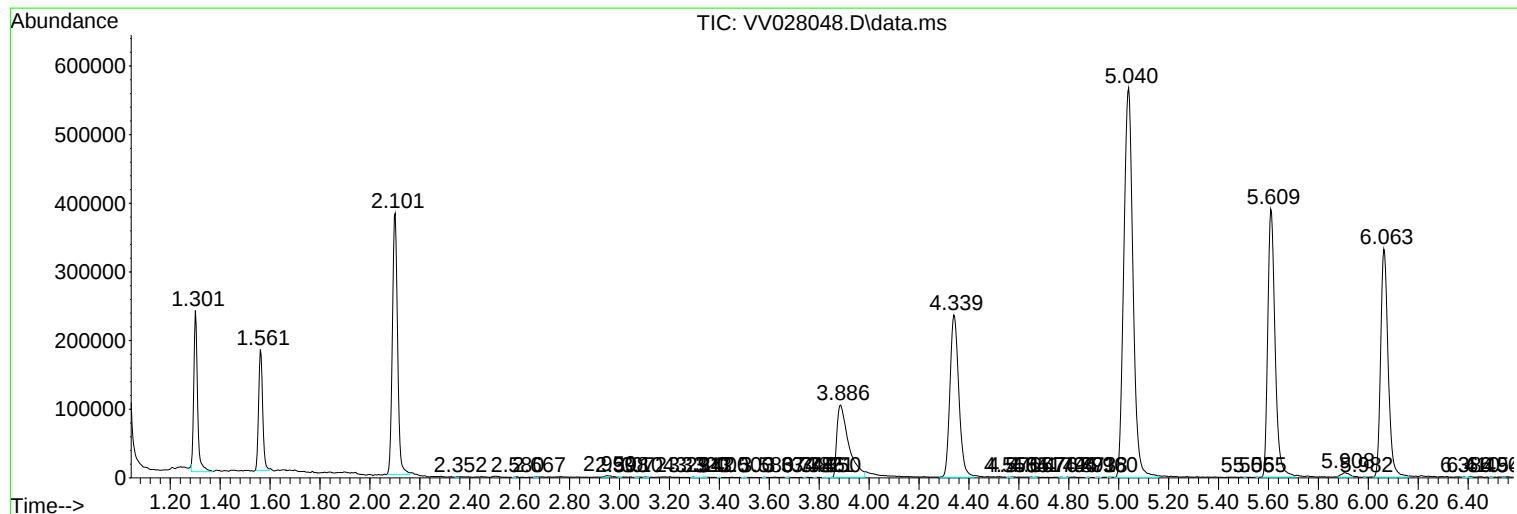

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028048.D
Acq On : 22 Sep 2022 05:11
Operator : SY/MD
Sample : N4659-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028048.D
Acq On : 22 Sep 2022 05:11
Operator : SY/MD
Sample : N4659-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc