

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028052.D
 Acq On : 22 Sep 2022 09:21
 Operator : SY/MD
 Sample : VV0921WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028052.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	101	rVB	260290	273551	16.52%	2.269%
2	1.561	156	162	175	rVB	198399	222648	13.44%	1.847%
3	2.098	320	329	351	rBV	433008	626819	37.85%	5.199%
4	2.256	376	378	382	rBV3	777	487	0.03%	0.004%
5	2.462	438	442	444	rBV2	633	488	0.03%	0.004%
6	2.584	476	480	482	rBV3	507	392	0.02%	0.003%
7	2.677	504	509	514	rBV3	693	500	0.03%	0.004%
8	2.751	528	532	534	rBV2	680	544	0.03%	0.005%
9	2.857	562	565	567	rBV2	539	290	0.02%	0.002%
10	2.902	576	579	582	rBV2	612	366	0.02%	0.003%
11	2.918	582	584	588	rBV4	632	427	0.03%	0.004%
12	3.024	614	617	620	rVB3	620	455	0.03%	0.004%
13	3.047	620	624	625	rBV2	576	456	0.03%	0.004%
14	3.130	647	650	654	rVV4	646	389	0.02%	0.003%
15	3.201	666	672	674	rBV5	844	642	0.04%	0.005%
16	3.252	685	688	692	rVB3	686	445	0.03%	0.004%
17	3.285	692	698	700	rBV3	580	641	0.04%	0.005%
18	3.317	704	708	711	rVV2	620	526	0.03%	0.004%
19	3.426	739	742	744	rVB2	499	256	0.02%	0.002%
20	3.442	744	747	749	rBV	670	354	0.02%	0.003%
21	3.461	751	753	755	rVV	935	394	0.02%	0.003%
22	3.481	755	759	761	rVB2	564	395	0.02%	0.003%
23	3.587	790	792	795	rBV3	432	297	0.02%	0.002%
24	3.616	800	801	806	rBV2	587	334	0.02%	0.003%
25	3.645	806	810	814	rBV2	641	483	0.03%	0.004%
26	3.748	838	842	845	rVB3	559	495	0.03%	0.004%
27	3.879	872	883	920	rBV	126221	409256	24.71%	3.395%
28	4.336	1008	1025	1050	rBV	258649	647060	39.07%	5.367%
29	4.709	1138	1141	1144	rVV3	578	360	0.02%	0.003%
30	4.735	1147	1149	1150	rVV	651	263	0.02%	0.002%
31	4.754	1153	1155	1157	rVB3	833	366	0.02%	0.003%
32	4.828	1175	1178	1180	rBV	579	332	0.02%	0.003%
33	4.870	1187	1191	1193	rBV3	767	544	0.03%	0.005%
34	4.892	1196	1198	1203	rBV3	618	513	0.03%	0.004%
35	4.928	1208	1209	1212	rVB	635	250	0.02%	0.002%
36	4.947	1212	1215	1216	rBV	527	308	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028052.D
 Acq On : 22 Sep 2022 09:21
 Operator : SY/MD
 Sample : VV0921WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.034	1223	1242	1270	rBV2	641846	1656132	100.00%	13.737%
38	5.365	1343	1345	1348	rBV3	713	357	0.02%	0.003%
39	5.606	1407	1420	1442	rBV	424239	866622	52.33%	7.188%
40	5.899	1501	1511	1525	rBV8	8658	20631	1.25%	0.171%
41	5.989	1536	1539	1541	rBV2	943	785	0.05%	0.007%
42	6.059	1547	1561	1593	rBV	363655	749032	45.23%	6.213%
43	6.291	1631	1633	1637	rBV4	496	409	0.02%	0.003%
44	6.320	1641	1642	1644	rBV2	694	351	0.02%	0.003%
45	6.465	1682	1687	1689	rBV3	418	458	0.03%	0.004%
46	6.548	1711	1713	1717	rVB2	975	491	0.03%	0.004%
47	6.571	1717	1720	1722	rBV	616	397	0.02%	0.003%
48	6.654	1744	1746	1750	rVB2	797	608	0.04%	0.005%
49	6.722	1765	1767	1771	rBV5	595	353	0.02%	0.003%
50	6.764	1778	1780	1783	rBV4	509	291	0.02%	0.002%
51	6.796	1788	1790	1796	rVB4	825	701	0.04%	0.006%
52	6.979	1836	1847	1874	rBV	172328	321482	19.41%	2.667%
53	7.307	1937	1949	1970	rBV	721625	1261695	76.18%	10.465%
54	7.574	2029	2032	2033	rBV2	636	278	0.02%	0.002%
55	7.616	2035	2045	2071	rVV	121745	216313	13.06%	1.794%
56	7.908	2134	2136	2138	rBV2	600	426	0.03%	0.004%
57	8.082	2180	2190	2230	rVV	433845	822394	49.66%	6.822%
58	8.529	2326	2329	2331	rBV2	783	542	0.03%	0.004%
59	8.567	2336	2341	2344	rVB5	812	741	0.04%	0.006%
60	8.680	2374	2376	2381	rBV4	500	259	0.02%	0.002%
61	8.770	2400	2404	2407	rBV3	610	545	0.03%	0.005%
62	8.847	2416	2428	2448	rBV	641533	1052157	63.53%	8.727%
63	9.114	2509	2511	2515	rVB2	711	346	0.02%	0.003%
64	9.133	2515	2517	2518	rBV2	1071	563	0.03%	0.005%
65	9.233	2547	2548	2553	rVB2	765	497	0.03%	0.004%
66	9.365	2586	2589	2594	rBV3	519	406	0.02%	0.003%
67	9.387	2594	2596	2599	rVB3	835	382	0.02%	0.003%
68	9.407	2599	2602	2605	rBV2	633	506	0.03%	0.004%
69	9.500	2629	2631	2632	rBV	658	265	0.02%	0.002%
70	9.747	2705	2708	2710	rVB2	798	426	0.03%	0.004%
71	9.783	2714	2719	2721	rBV4	494	434	0.03%	0.004%
72	9.892	2751	2753	2759	rVB3	717	642	0.04%	0.005%
73	9.969	2775	2777	2780	rBV3	599	328	0.02%	0.003%
74	10.053	2801	2803	2804	rBV2	872	314	0.02%	0.003%
75	10.095	2814	2816	2818	rBV2	622	372	0.02%	0.003%
76	10.210	2838	2852	2872	rBV	522439	808276	48.81%	6.704%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028052.D
 Acq On : 22 Sep 2022 09:21
 Operator : SY/MD
 Sample : VV0921WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.365	2898	2900	2903	rBV4	1304	864	0.05%	0.007%
78	10.445	2923	2925	2927	rVV3	629	324	0.02%	0.003%
79	10.548	2951	2957	2960	rBV4	1305	1419	0.09%	0.012%
80	10.728	3007	3013	3015	rBV3	681	606	0.04%	0.005%
81	11.053	3112	3114	3117	rVB3	559	326	0.02%	0.003%
82	11.246	3163	3174	3192	rBV	616638	955158	57.67%	7.923%
83	11.516	3256	3258	3262	rBV3	559	458	0.03%	0.004%
84	11.619	3278	3290	3308	rBV	710349	1109101	66.97%	9.200%
85	11.927	3383	3386	3387	rBV3	813	418	0.03%	0.003%
86	11.953	3391	3394	3397	rBV4	1067	623	0.04%	0.005%
87	12.197	3467	3470	3473	rBV4	410	335	0.02%	0.003%
88	12.281	3494	3496	3497	rBV	588	300	0.02%	0.002%
89	12.525	3570	3572	3574	rBV2	1085	507	0.03%	0.004%
90	12.574	3584	3587	3590	rBV4	675	584	0.04%	0.005%
91	12.754	3641	3643	3644	rBV	904	425	0.03%	0.004%
92	12.815	3660	3662	3665	rBV3	660	316	0.02%	0.003%
93	13.004	3717	3721	3724	rBV4	713	687	0.04%	0.006%
94	13.156	3766	3768	3769	rBV2	824	256	0.02%	0.002%
95	13.255	3797	3799	3802	rBV2	748	476	0.03%	0.004%
96	13.329	3819	3822	3827	rBV4	471	430	0.03%	0.004%
97	13.664	3922	3926	3930	rBV3	582	429	0.03%	0.004%
98	13.722	3941	3944	3947	rBV2	596	335	0.02%	0.003%
99	13.744	3947	3951	3952	rBV2	824	532	0.03%	0.004%
100	14.008	4029	4033	4038	rVB3	578	452	0.03%	0.004%




Sum of corrected areas: 12055894

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028052.D
Acq On : 22 Sep 2022 09:21
Operator : SY/MD
Sample : VV0921WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

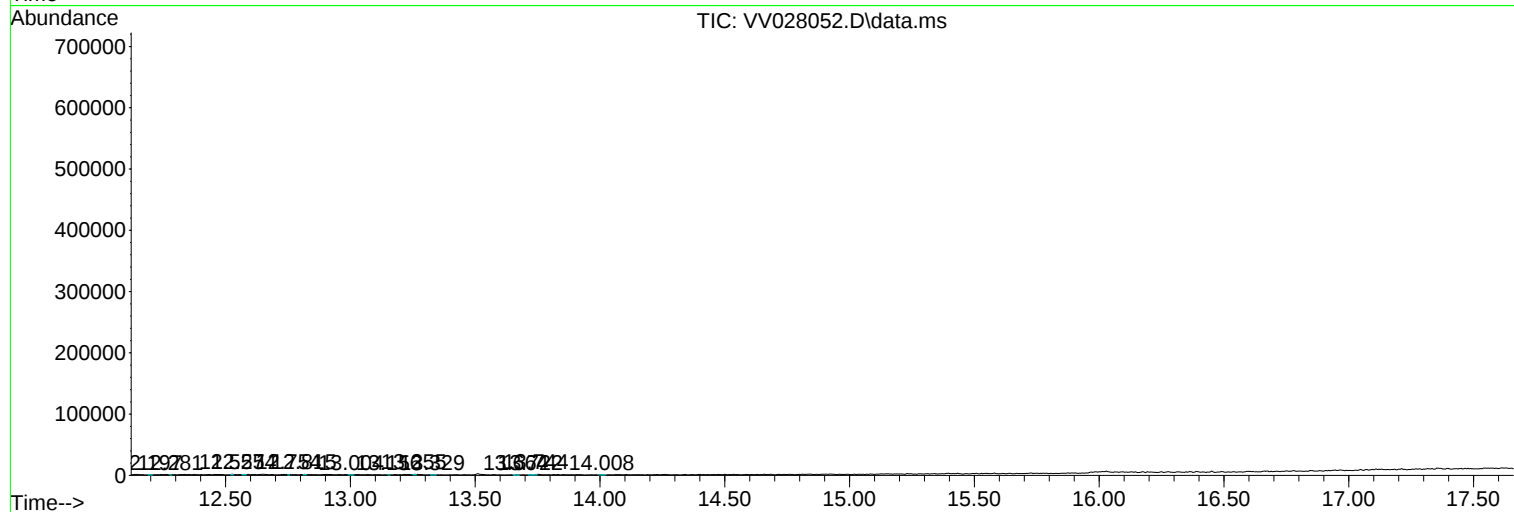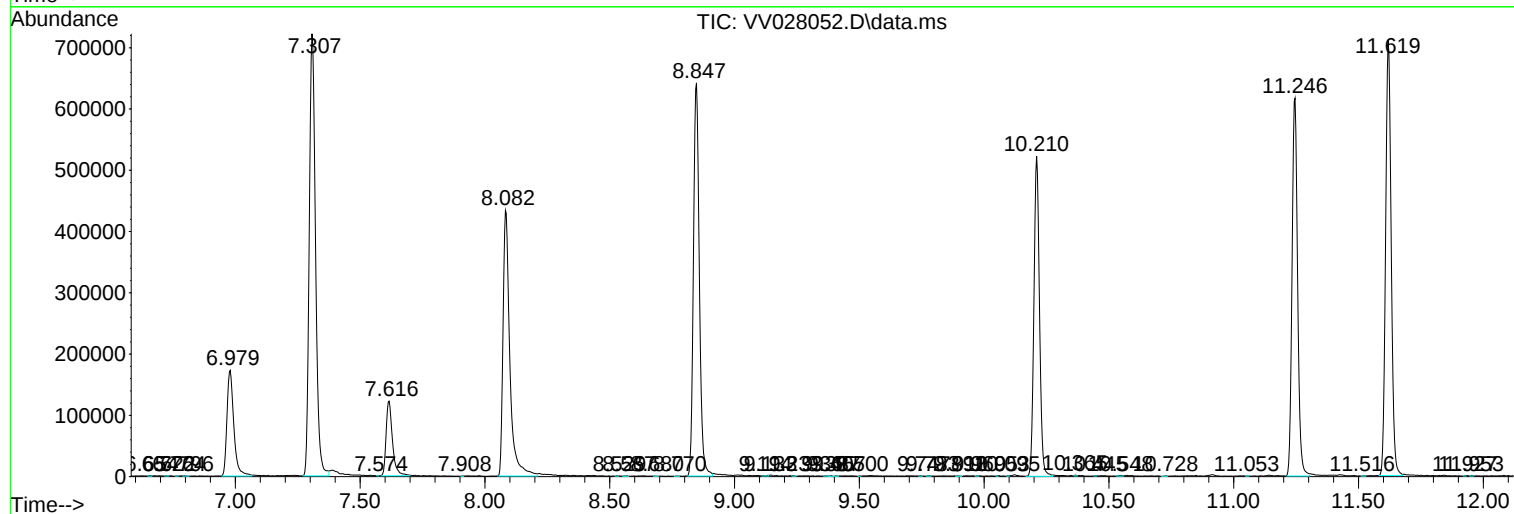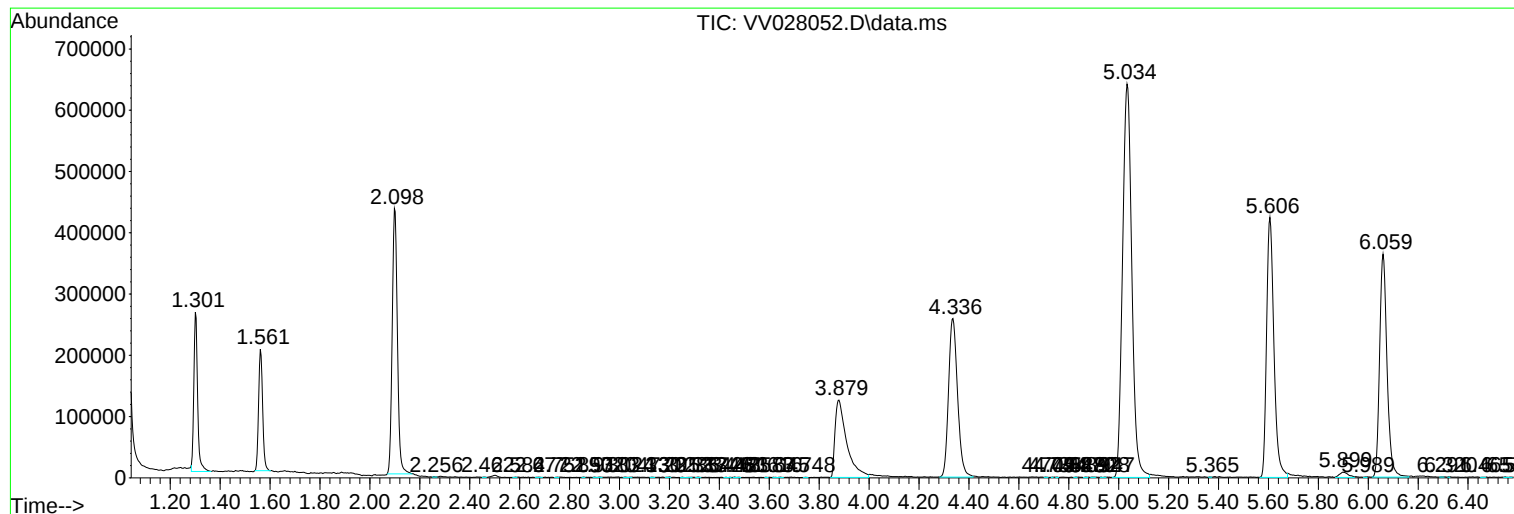

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028052.D
Acq On : 22 Sep 2022 09:21
Operator : SY/MD
Sample : VV0921WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028052.D
Acq On : 22 Sep 2022 09:21
Operator : SY/MD
Sample : VV0921WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc