

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028053.D
 Acq On : 22 Sep 2022 09:46
 Operator : SY/MD
 Sample : N4677-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	95	rVB	231170	234584	14.99%	2.052%
2	1.561	156	162	179	rVB	186974	212757	13.59%	1.861%
3	2.098	320	329	363	rVB	401438	608300	38.86%	5.321%
4	2.426	426	431	433	rBV3	974	962	0.06%	0.008%
5	2.606	483	487	491	rBV5	713	698	0.04%	0.006%
6	2.671	505	507	508	rBV	438	181	0.01%	0.002%
7	2.716	518	521	523	rBV2	389	212	0.01%	0.002%
8	2.754	527	533	538	rBV5	897	1121	0.07%	0.010%
9	2.773	538	539	544	rVB2	502	274	0.02%	0.002%
10	2.937	587	590	592	rBV2	407	294	0.02%	0.003%
11	2.995	606	608	609	rVB2	681	199	0.01%	0.002%
12	3.082	630	635	639	rBV3	517	424	0.03%	0.004%
13	3.185	662	667	669	rBV2	602	499	0.03%	0.004%
14	3.220	676	678	681	rVB3	530	251	0.02%	0.002%
15	3.240	682	684	689	rVB4	535	380	0.02%	0.003%
16	3.301	699	703	706	rBV3	605	502	0.03%	0.004%
17	3.394	730	732	734	rBV	425	222	0.01%	0.002%
18	3.442	745	747	751	rBV2	356	263	0.02%	0.002%
19	3.478	754	758	760	rBV2	532	414	0.03%	0.004%
20	3.535	772	776	779	rBV4	604	485	0.03%	0.004%
21	3.577	787	789	792	rVB2	536	287	0.02%	0.003%
22	3.597	792	795	798	rBV3	696	583	0.04%	0.005%
23	3.642	807	809	811	rBV	451	261	0.02%	0.002%
24	3.728	831	836	840	rVB3	747	551	0.04%	0.005%
25	3.754	841	844	846	rBV2	401	248	0.02%	0.002%
26	3.777	849	851	855	rBV2	528	290	0.02%	0.003%
27	3.802	855	859	866	rVB5	653	848	0.05%	0.007%
28	3.831	866	868	871	rBV3	606	306	0.02%	0.003%
29	3.883	874	884	925	rBV2	127313	418924	26.76%	3.664%
30	4.179	975	976	977	rBV	834	278	0.02%	0.002%
31	4.339	1010	1026	1051	rBV	247696	608028	38.85%	5.318%
32	4.738	1147	1150	1153	rBV3	438	351	0.02%	0.003%
33	4.780	1160	1163	1164	rBV	485	242	0.02%	0.002%
34	4.818	1169	1175	1176	rVB3	496	351	0.02%	0.003%
35	4.851	1181	1185	1189	rBV3	795	692	0.04%	0.006%
36	4.937	1210	1212	1214	rBV4	589	308	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028053.D
 Acq On : 22 Sep 2022 09:46
 Operator : SY/MD
 Sample : N4677-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.040	1226	1244	1269	rBV2	609533	1565199	100.00%	13.690%
38	5.481	1377	1381	1383	rBV4	675	483	0.03%	0.004%
39	5.542	1396	1400	1401	rBV4	983	646	0.04%	0.006%
40	5.609	1409	1421	1449	rBV	401114	820012	52.39%	7.172%
41	5.969	1530	1533	1535	rVB2	793	378	0.02%	0.003%
42	6.005	1542	1544	1546	rBV3	635	239	0.02%	0.002%
43	6.063	1550	1562	1592	rVV	347821	710182	45.37%	6.212%
44	6.445	1678	1681	1682	rBV	796	448	0.03%	0.004%
45	6.477	1689	1691	1693	rVB2	718	318	0.02%	0.003%
46	6.494	1693	1696	1698	rBV3	440	288	0.02%	0.003%
47	6.580	1721	1723	1724	rBV	464	202	0.01%	0.002%
48	6.670	1749	1751	1755	rVB3	894	692	0.04%	0.006%
49	6.703	1759	1761	1764	rVB3	732	467	0.03%	0.004%
50	6.828	1796	1800	1801	rBV3	496	369	0.02%	0.003%
51	6.902	1821	1823	1825	rBV2	436	209	0.01%	0.002%
52	6.982	1835	1848	1873	rBV	158176	299605	19.14%	2.621%
53	7.185	1908	1911	1912	rBV	455	244	0.02%	0.002%
54	7.310	1938	1950	1969	rBV	667319	1151808	73.59%	10.075%
55	7.619	2033	2046	2068	rBV	113411	207460	13.25%	1.815%
56	7.883	2127	2128	2131	rVB2	489	226	0.01%	0.002%
57	7.973	2153	2156	2158	rBV2	723	467	0.03%	0.004%
58	8.085	2177	2191	2222	rBV	443449	811746	51.86%	7.100%
59	8.674	2373	2374	2380	rVB5	976	608	0.04%	0.005%
60	8.847	2417	2428	2451	rBV	616909	1013365	64.74%	8.864%
61	9.230	2545	2547	2552	rVB2	838	581	0.04%	0.005%
62	9.252	2552	2554	2556	rBV3	742	473	0.03%	0.004%
63	9.410	2600	2603	2604	rBV2	698	375	0.02%	0.003%
64	9.622	2667	2669	2671	rBV2	631	435	0.03%	0.004%
65	9.735	2702	2704	2707	rBV2	604	251	0.02%	0.002%
66	9.770	2712	2715	2717	rBV2	585	357	0.02%	0.003%
67	9.818	2728	2730	2731	rVV	624	192	0.01%	0.002%
68	9.828	2731	2733	2738	rVV3	373	249	0.02%	0.002%
69	9.982	2780	2781	2785	rBV3	283	225	0.01%	0.002%
70	9.998	2785	2786	2790	rVV2	919	484	0.03%	0.004%
71	10.040	2797	2799	2800	rBV	624	268	0.02%	0.002%
72	10.063	2804	2806	2811	rVB4	810	484	0.03%	0.004%
73	10.091	2812	2815	2817	rBV3	761	497	0.03%	0.004%
74	10.210	2841	2852	2877	rBV	499912	789342	50.43%	6.904%
75	10.423	2916	2918	2923	rBV5	642	565	0.04%	0.005%
76	10.493	2938	2940	2943	rVB3	761	352	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028053.D
 Acq On : 22 Sep 2022 09:46
 Operator : SY/MD
 Sample : N4677-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.538	2950	2954	2955	rBV2	704	559	0.04%	0.005%
78	10.651	2986	2989	2991	rBV2	496	280	0.02%	0.002%
79	10.673	2994	2996	3000	rBV3	409	294	0.02%	0.003%
80	10.702	3000	3005	3006	rBV3	524	468	0.03%	0.004%
81	10.763	3022	3024	3028	rVB2	714	463	0.03%	0.004%
82	10.911	3064	3070	3072	rBV5	1793	1973	0.13%	0.017%
83	10.992	3089	3095	3096	rBV2	588	543	0.03%	0.005%
84	11.133	3132	3139	3140	rBV4	1127	1189	0.08%	0.010%
85	11.181	3151	3154	3156	rBV2	1039	631	0.04%	0.006%
86	11.246	3162	3174	3197	rBV	579155	893355	57.08%	7.814%
87	11.619	3278	3290	3314	rBV	664597	1051720	67.19%	9.199%
88	11.850	3360	3362	3363	rBV2	734	219	0.01%	0.002%
89	12.069	3428	3430	3433	rVB3	696	271	0.02%	0.002%
90	12.271	3491	3493	3495	rVB2	821	318	0.02%	0.003%
91	12.307	3503	3504	3507	rBV2	453	200	0.01%	0.002%
92	12.599	3589	3595	3597	rBV3	778	902	0.06%	0.008%
93	13.024	3724	3727	3730	rBV2	738	441	0.03%	0.004%
94	13.368	3832	3834	3836	rBV2	602	268	0.02%	0.002%
95	13.468	3863	3865	3868	rVB2	666	298	0.02%	0.003%
96	13.644	3917	3920	3924	rBV	551	420	0.03%	0.004%
97	13.924	4004	4007	4009	rBV2	647	385	0.02%	0.003%
98	14.059	4047	4049	4050	rBV2	490	219	0.01%	0.002%
99	14.172	4082	4084	4085	rBV	565	253	0.02%	0.002%
100	14.545	4196	4200	4203	rBV2	968	802	0.05%	0.007%




Sum of corrected areas: 11432832

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028053.D
Acq On : 22 Sep 2022 09:46
Operator : SY/MD
Sample : N4677-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

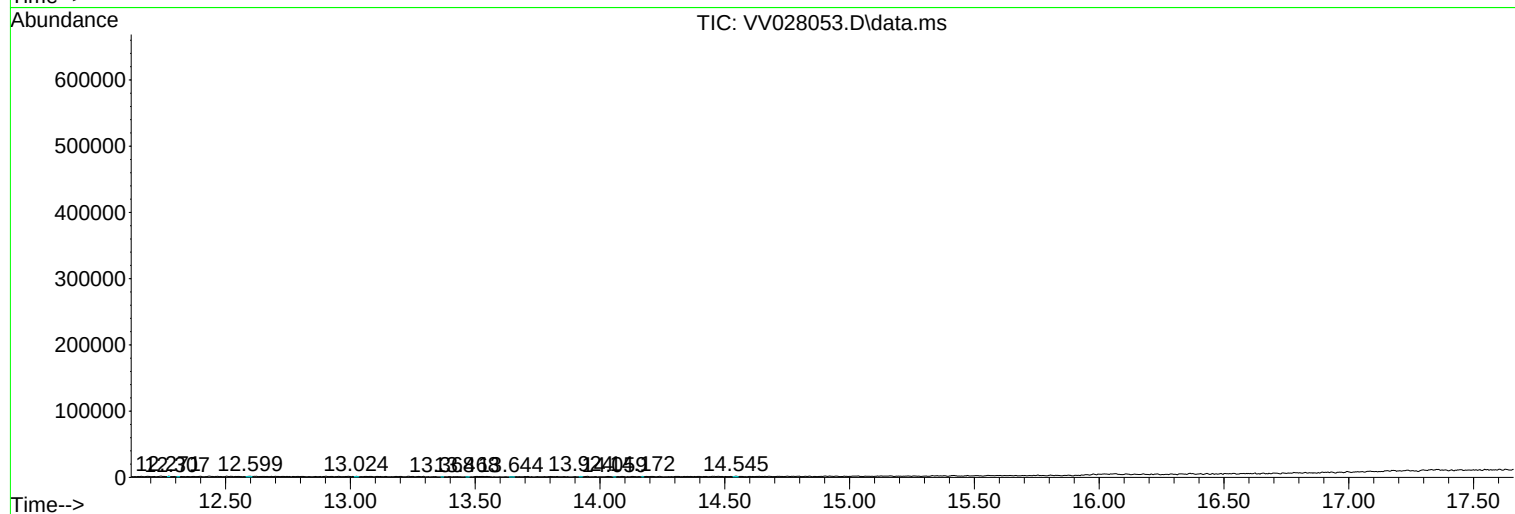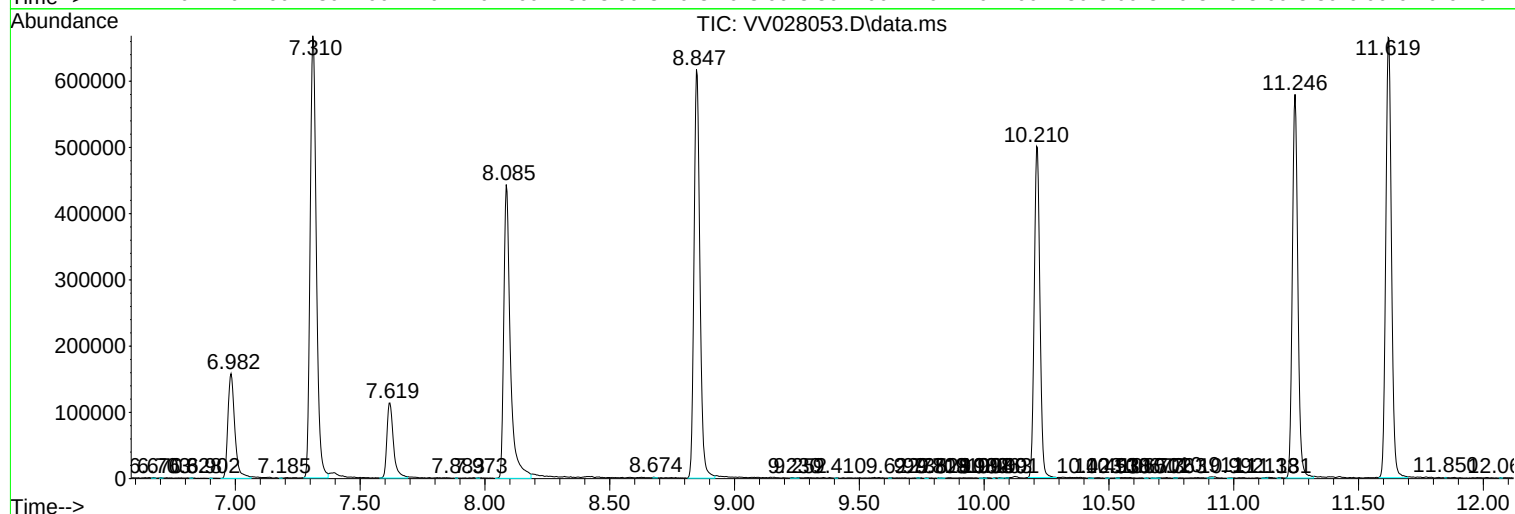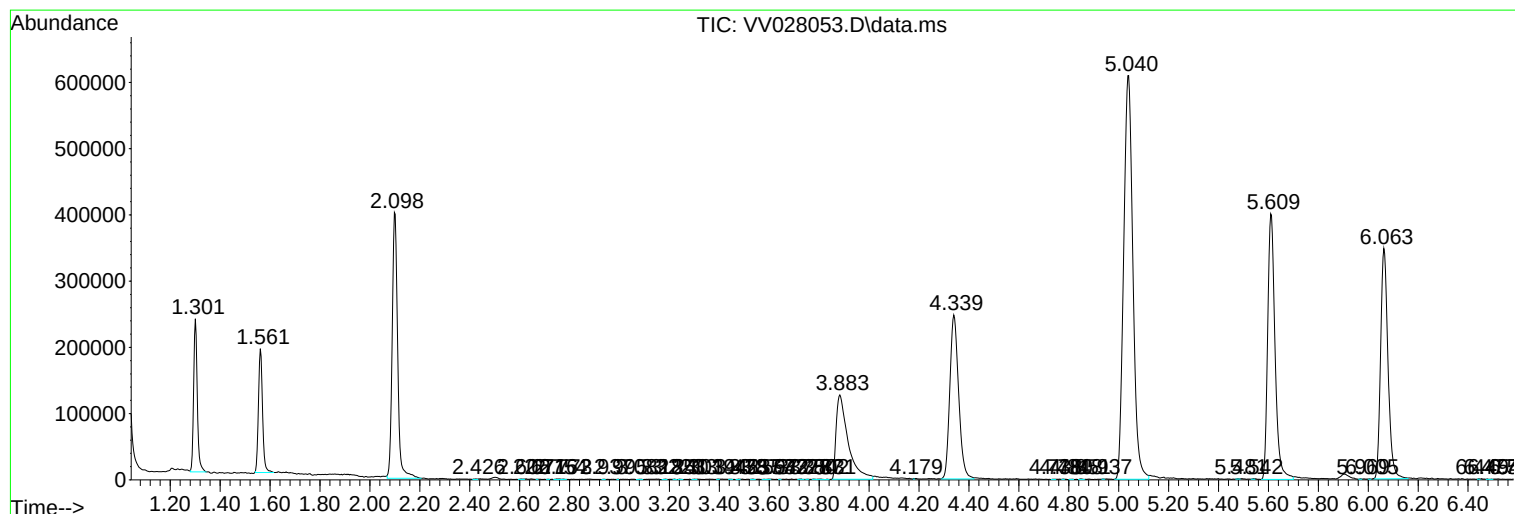

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028053.D
Acq On : 22 Sep 2022 09:46
Operator : SY/MD
Sample : N4677-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028053.D
Acq On : 22 Sep 2022 09:46
Operator : SY/MD
Sample : N4677-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------