

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028056.D
 Acq On : 22 Sep 2022 11:00
 Operator : SY/MD
 Sample : N4659-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	98	rVB	219591	227824	14.98%	1.978%
2	1.561	156	162	179	rVB	176540	197414	12.98%	1.714%
3	2.098	320	329	359	rVB2	386694	583327	38.35%	5.065%
4	2.500	447	454	457	rBV7	1900	2215	0.15%	0.019%
5	2.571	468	476	477	rBV2	577	576	0.04%	0.005%
6	2.635	493	496	498	rBV2	724	459	0.03%	0.004%
7	2.838	555	559	562	rVV	408	291	0.02%	0.003%
8	2.921	581	585	589	rBV2	630	635	0.04%	0.006%
9	2.960	589	597	601	rBV6	1534	2515	0.17%	0.022%
10	3.027	615	618	620	rVV3	363	279	0.02%	0.002%
11	3.043	621	623	625	rVB3	714	280	0.02%	0.002%
12	3.072	630	632	636	rVB3	385	266	0.02%	0.002%
13	3.101	636	641	643	rBV2	481	386	0.03%	0.003%
14	3.146	652	655	656	rBV2	542	315	0.02%	0.003%
15	3.333	711	713	717	rBV2	410	281	0.02%	0.002%
16	3.387	726	730	733	rBV2	555	500	0.03%	0.004%
17	3.484	757	760	761	rBV2	549	269	0.02%	0.002%
18	3.529	772	774	776	rBV	546	353	0.02%	0.003%
19	3.645	808	810	813	rBV	546	322	0.02%	0.003%
20	3.712	828	831	833	rBV3	538	393	0.03%	0.003%
21	3.757	842	845	847	rBV4	519	280	0.02%	0.002%
22	3.789	852	855	857	rBV3	545	323	0.02%	0.003%
23	3.847	868	873	874	rBV4	421	345	0.02%	0.003%
24	3.886	874	885	926	rBV	121646	401761	26.41%	3.488%
25	4.339	1011	1026	1052	rBV	235567	583923	38.39%	5.070%
26	4.815	1171	1174	1176	rBV2	480	264	0.02%	0.002%
27	4.850	1184	1185	1190	rBV3	420	307	0.02%	0.003%
28	4.908	1199	1203	1207	rBV4	550	543	0.04%	0.005%
29	4.931	1207	1210	1212	rVV2	845	447	0.03%	0.004%
30	5.037	1226	1243	1275	rBV2	591314	1521036	100.00%	13.207%
31	5.403	1354	1357	1366	rBV7	984	1522	0.10%	0.013%
32	5.448	1369	1371	1375	rVB3	987	588	0.04%	0.005%
33	5.468	1375	1377	1378	rBV	766	302	0.02%	0.003%
34	5.516	1390	1392	1396	rBV3	446	337	0.02%	0.003%
35	5.561	1402	1406	1409	rBV4	891	897	0.06%	0.008%
36	5.609	1409	1421	1445	rBV	399653	814122	53.52%	7.069%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028056.D
 Acq On : 22 Sep 2022 11:00
 Operator : SY/MD
 Sample : N4659-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.908	1502	1514	1538	rBV2	177844	366973	24.13%	3.186%
38	6.063	1551	1562	1588	rVB	321169	656211	43.14%	5.698%
39	6.326	1640	1644	1648	rBV5	1005	839	0.06%	0.007%
40	6.352	1648	1652	1655	rVV4	584	489	0.03%	0.004%
41	6.391	1662	1664	1667	rVB3	584	335	0.02%	0.003%
42	6.429	1672	1676	1679	rVB3	480	379	0.02%	0.003%
43	6.445	1679	1681	1684	rBV3	454	338	0.02%	0.003%
44	6.590	1723	1726	1730	rBV2	785	484	0.03%	0.004%
45	6.702	1760	1761	1764	rBV3	636	395	0.03%	0.003%
46	6.776	1782	1784	1787	rBV3	665	274	0.02%	0.002%
47	6.873	1810	1814	1816	rBV3	575	451	0.03%	0.004%
48	6.895	1819	1821	1824	rVB2	1079	452	0.03%	0.004%
49	6.928	1829	1831	1833	rBV2	611	311	0.02%	0.003%
50	6.982	1836	1848	1872	rBV	174123	326150	21.44%	2.832%
51	7.182	1908	1910	1912	rBV2	690	325	0.02%	0.003%
52	7.310	1939	1950	1971	rBV	652222	1149826	75.59%	9.984%
53	7.619	2036	2046	2063	rBV	127324	223886	14.72%	1.944%
54	7.731	2079	2081	2085	rVB4	1359	824	0.05%	0.007%
55	7.841	2113	2115	2118	rBV3	985	537	0.04%	0.005%
56	7.857	2118	2120	2122	rVB3	885	332	0.02%	0.003%
57	8.085	2181	2191	2229	rBV	436072	830705	54.61%	7.213%
58	8.532	2328	2330	2332	rBV2	729	293	0.02%	0.003%
59	8.564	2338	2340	2342	rBV2	882	500	0.03%	0.004%
60	8.670	2371	2373	2377	rBV3	667	413	0.03%	0.004%
61	8.850	2417	2429	2451	rBV	597845	988400	64.98%	8.582%
62	9.127	2511	2515	2516	rBV2	694	319	0.02%	0.003%
63	9.143	2518	2520	2523	rBV3	931	530	0.03%	0.005%
64	9.223	2542	2545	2549	rBV3	555	424	0.03%	0.004%
65	9.329	2575	2578	2581	rBV	427	386	0.03%	0.003%
66	9.345	2581	2583	2586	rVB2	568	330	0.02%	0.003%
67	9.365	2586	2589	2590	rBV2	790	432	0.03%	0.004%
68	9.509	2630	2634	2636	rBV3	414	331	0.02%	0.003%
69	9.770	2712	2715	2716	rBV2	505	259	0.02%	0.002%
70	9.789	2716	2721	2724	rVV2	513	429	0.03%	0.004%
71	9.812	2724	2728	2732	rBV2	877	681	0.04%	0.006%
72	9.982	2779	2781	2784	rVB	797	337	0.02%	0.003%
73	10.085	2811	2813	2816	rBV2	735	408	0.03%	0.004%
74	10.214	2841	2853	2873	rBV	486929	756077	49.71%	6.565%
75	10.471	2930	2933	2940	rVB7	721	678	0.04%	0.006%
76	10.654	2987	2990	2992	rBV2	569	397	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028056.D
 Acq On : 22 Sep 2022 11:00
 Operator : SY/MD
 Sample : N4659-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.718	3006	3010	3011	rBV2	473	284	0.02%	0.002%
78	10.763	3021	3024	3026	rBV2	901	511	0.03%	0.004%
79	10.824	3037	3043	3044	rBV3	998	771	0.05%	0.007%
80	11.027	3102	3106	3108	rBV3	818	556	0.04%	0.005%
81	11.120	3132	3135	3137	rBV2	860	567	0.04%	0.005%
82	11.246	3163	3174	3194	rBV	551652	858160	56.42%	7.451%
83	11.538	3255	3265	3267	rBV5	4861	6791	0.45%	0.059%
84	11.622	3279	3291	3314	rBV	631882	984350	64.72%	8.547%
85	12.011	3409	3412	3415	rBV	648	495	0.03%	0.004%
86	12.078	3431	3433	3435	rBV3	804	421	0.03%	0.004%
87	12.136	3449	3451	3454	rBV3	477	285	0.02%	0.002%
88	12.326	3508	3510	3512	rBV2	618	306	0.02%	0.003%
89	12.574	3585	3587	3590	rBV2	659	440	0.03%	0.004%
90	12.744	3637	3640	3643	rBV4	630	397	0.03%	0.003%
91	12.895	3685	3687	3689	rBV2	653	317	0.02%	0.003%
92	12.937	3698	3700	3702	rBV2	545	266	0.02%	0.002%
93	13.027	3726	3728	3731	rBV3	631	488	0.03%	0.004%
94	13.136	3758	3762	3766	rBV3	648	689	0.05%	0.006%
95	13.239	3792	3794	3797	rVB3	709	294	0.02%	0.003%
96	13.455	3858	3861	3866	rBV4	1159	874	0.06%	0.008%
97	13.564	3893	3895	3900	rBV4	583	423	0.03%	0.004%
98	13.779	3959	3962	3964	rBV3	816	550	0.04%	0.005%
99	13.860	3984	3987	3989	rBV2	742	484	0.03%	0.004%
100	14.554	4200	4203	4205	rBV3	838	446	0.03%	0.004%




Sum of corrected areas: 11517202

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028056.D
Acq On : 22 Sep 2022 11:00
Operator : SY/MD
Sample : N4659-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

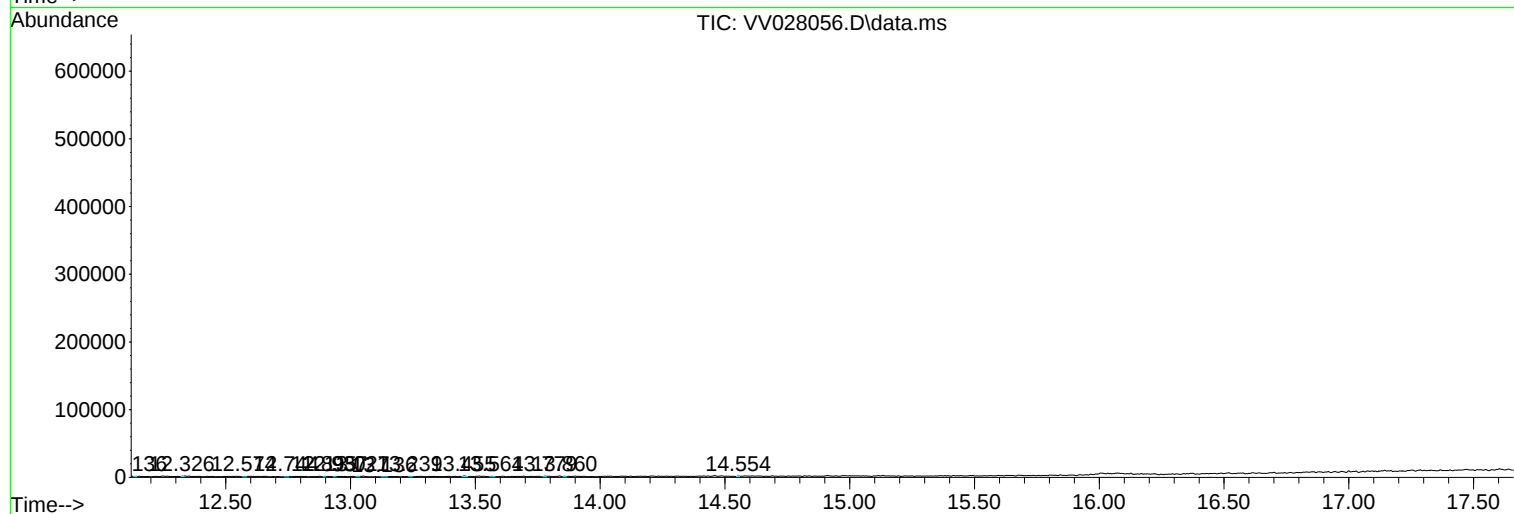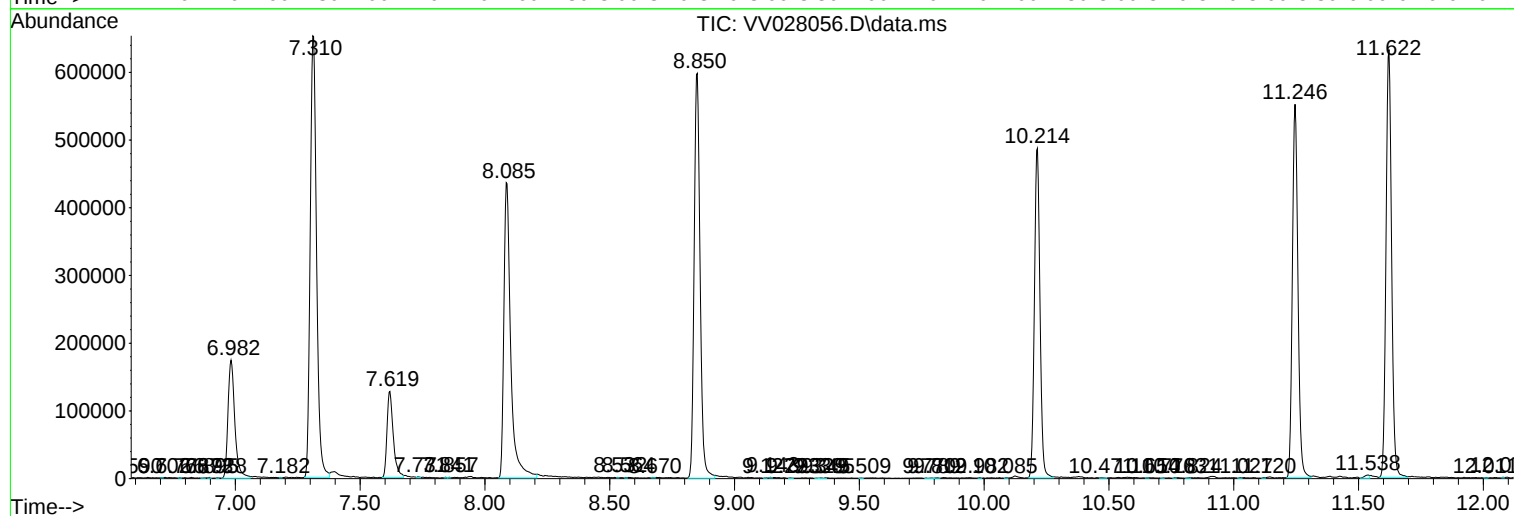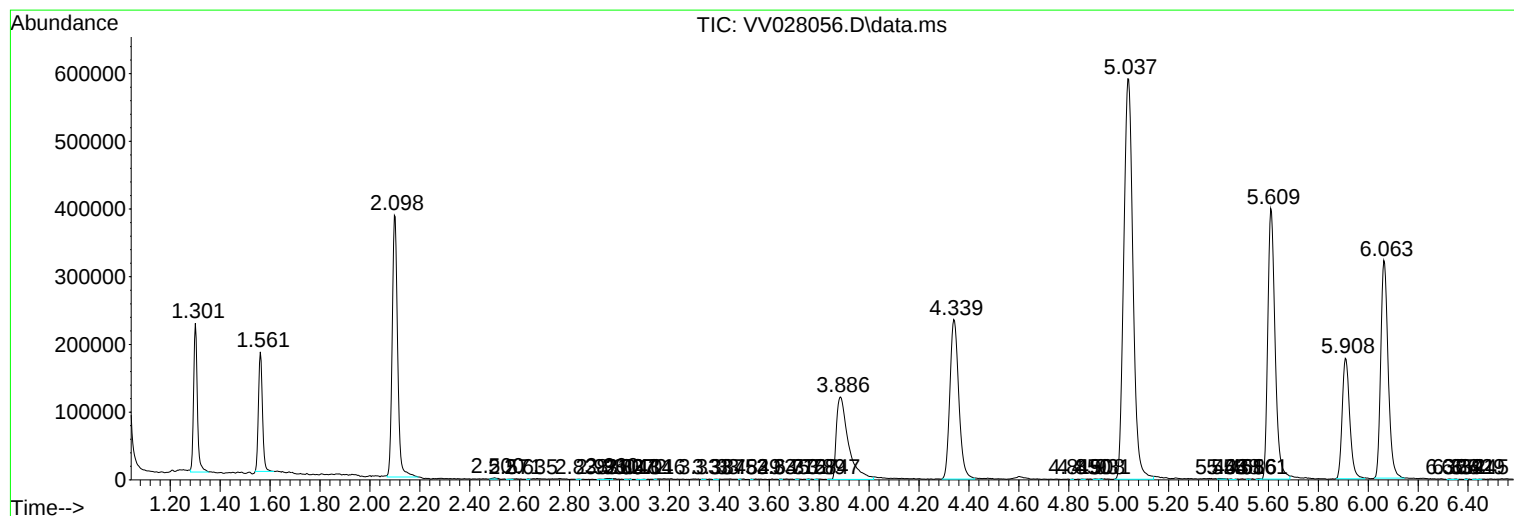

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028056.D
Acq On : 22 Sep 2022 11:00
Operator : SY/MD
Sample : N4659-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028056.D
Acq On : 22 Sep 2022 11:00
Operator : SY/MD
Sample : N4659-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
