

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028057.D
 Acq On : 22 Sep 2022 11:25
 Operator : SY/MD
 Sample : N4674-19DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	101	rVB	232207	240091	14.82%	1.991%
2	1.561	155	162	175	rBV	199157	218354	13.47%	1.811%
3	2.098	320	329	342	rBV	416890	594498	36.68%	4.930%
4	2.172	344	352	383	rVB	183141	421113	25.99%	3.492%
5	2.854	560	564	572	rBV4	805	1053	0.06%	0.009%
6	3.066	626	630	634	rBV4	423	412	0.03%	0.003%
7	3.108	641	643	647	rVB2	459	223	0.01%	0.002%
8	3.169	660	662	663	rBV3	674	231	0.01%	0.002%
9	3.230	677	681	688	rBV6	1111	1389	0.09%	0.012%
10	3.375	724	726	729	rBV3	538	368	0.02%	0.003%
11	3.458	750	752	755	rBV2	560	312	0.02%	0.003%
12	3.516	765	770	776	rVV4	627	546	0.03%	0.005%
13	3.642	805	809	812	rVB4	727	598	0.04%	0.005%
14	3.806	858	860	865	rVB3	767	482	0.03%	0.004%
15	3.883	874	884	931	rBV	130718	448768	27.69%	3.722%
16	4.224	987	990	991	rBV	759	466	0.03%	0.004%
17	4.339	1011	1026	1049	rBV	255324	624088	38.51%	5.176%
18	4.600	1105	1107	1109	rBV2	735	334	0.02%	0.003%
19	4.632	1115	1117	1122	rBV5	936	635	0.04%	0.005%
20	4.722	1141	1145	1147	rBV4	1060	656	0.04%	0.005%
21	4.761	1153	1157	1160	rBV3	891	807	0.05%	0.007%
22	4.896	1198	1199	1202	rBV2	382	212	0.01%	0.002%
23	4.912	1202	1204	1207	rVB3	541	296	0.02%	0.002%
24	4.941	1210	1213	1216	rBV3	625	509	0.03%	0.004%
25	5.037	1225	1243	1277	rBV2	631829	1620576	100.00%	13.440%
26	5.452	1369	1372	1374	rBV3	932	480	0.03%	0.004%
27	5.548	1399	1402	1404	rBV3	1220	591	0.04%	0.005%
28	5.609	1408	1421	1446	rBV	397992	810328	50.00%	6.720%
29	5.902	1502	1512	1528	rBV	11019	27669	1.71%	0.229%
30	6.063	1548	1562	1587	rBV	357962	733517	45.26%	6.083%
31	6.365	1655	1656	1659	rBV	530	233	0.01%	0.002%
32	6.452	1680	1683	1685	rBV3	617	365	0.02%	0.003%
33	6.497	1693	1697	1699	rBV	539	346	0.02%	0.003%
34	6.510	1699	1701	1704	rVB2	630	293	0.02%	0.002%
35	6.526	1704	1706	1709	rVB	445	292	0.02%	0.002%
36	6.545	1709	1712	1715	rBV2	715	441	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028057.D
 Acq On : 22 Sep 2022 11:25
 Operator : SY/MD
 Sample : N4674-19DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.561	1715	1717	1719	rBV3	366	242	0.01%	0.002%
38	6.574	1719	1721	1723	rBV3	698	298	0.02%	0.002%
39	6.625	1734	1737	1739	rVB4	488	282	0.02%	0.002%
40	6.645	1740	1743	1744	rBV2	647	284	0.02%	0.002%
41	6.658	1744	1747	1749	rVV2	618	351	0.02%	0.003%
42	6.732	1768	1770	1775	rVB4	787	501	0.03%	0.004%
43	6.777	1782	1784	1786	rBV	416	216	0.01%	0.002%
44	6.805	1791	1793	1796	rBV2	677	338	0.02%	0.003%
45	6.825	1796	1799	1802	rBV3	557	356	0.02%	0.003%
46	6.847	1802	1806	1810	rBV3	558	555	0.03%	0.005%
47	6.915	1824	1827	1828	rBV2	281	189	0.01%	0.002%
48	6.982	1836	1848	1874	rBV	177561	333648	20.59%	2.767%
49	7.233	1924	1926	1928	rBV2	478	200	0.01%	0.002%
50	7.310	1939	1950	1968	rBV	699709	1213588	74.89%	10.065%
51	7.616	2036	2045	2066	rBV	135845	237041	14.63%	1.966%
52	7.802	2098	2103	2106	rBV5	1179	1116	0.07%	0.009%
53	7.902	2129	2134	2139	rBV5	759	829	0.05%	0.007%
54	7.934	2139	2144	2147	rBV4	2266	2345	0.14%	0.019%
55	8.085	2182	2191	2225	rBV	467590	864034	53.32%	7.166%
56	8.648	2364	2366	2368	rBV3	555	334	0.02%	0.003%
57	8.735	2392	2393	2396	rVB2	755	351	0.02%	0.003%
58	8.776	2404	2406	2408	rBV2	513	274	0.02%	0.002%
59	8.847	2418	2428	2456	rBV	593118	969163	59.80%	8.038%
60	9.490	2623	2628	2632	rBV2	710	909	0.06%	0.008%
61	9.538	2641	2643	2646	rBV4	591	272	0.02%	0.002%
62	9.693	2689	2691	2692	rBV	453	228	0.01%	0.002%
63	9.719	2698	2699	2704	rVB5	1148	675	0.04%	0.006%
64	9.818	2728	2730	2733	rBV2	868	528	0.03%	0.004%
65	9.870	2744	2746	2750	rVB4	423	340	0.02%	0.003%
66	9.928	2762	2764	2765	rBV	716	286	0.02%	0.002%
67	10.005	2784	2788	2790	rBV3	737	700	0.04%	0.006%
68	10.075	2807	2810	2811	rBV2	677	364	0.02%	0.003%
69	10.124	2815	2825	2832	rBV7	3396	5167	0.32%	0.043%
70	10.214	2840	2853	2871	rBV	504525	799737	49.35%	6.633%
71	10.445	2922	2925	2927	rVB2	684	406	0.03%	0.003%
72	10.487	2936	2938	2941	rBV2	538	207	0.01%	0.002%
73	10.535	2949	2953	2954	rBV3	754	476	0.03%	0.004%
74	10.680	2996	2998	3004	rVB4	1154	905	0.06%	0.008%
75	10.719	3004	3010	3014	rVB5	859	723	0.04%	0.006%
76	10.747	3014	3019	3021	rBV3	657	617	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028057.D
 Acq On : 22 Sep 2022 11:25
 Operator : SY/MD
 Sample : N4674-19DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.812	3037	3039	3041	rBV2	510	218	0.01%	0.002%
78	10.825	3041	3043	3047	rVV4	512	253	0.02%	0.002%
79	10.911	3061	3070	3072	rBV5	2411	2497	0.15%	0.021%
80	10.960	3083	3085	3088	rBV2	568	361	0.02%	0.003%
81	11.034	3105	3108	3110	rVV3	793	532	0.03%	0.004%
82	11.098	3125	3128	3130	rBV2	579	305	0.02%	0.003%
83	11.140	3136	3141	3148	rVB6	1200	1541	0.10%	0.013%
84	11.175	3149	3152	3155	rVB2	677	358	0.02%	0.003%
85	11.194	3155	3158	3162	rVB3	557	428	0.03%	0.004%
86	11.246	3162	3174	3193	rBV	539095	831855	51.33%	6.899%
87	11.519	3254	3259	3260	rBV3	1067	747	0.05%	0.006%
88	11.622	3278	3291	3311	rBV	643245	1021465	63.03%	8.471%
89	11.918	3379	3383	3389	rBV6	1068	1107	0.07%	0.009%
90	11.995	3405	3407	3410	rBV4	923	571	0.04%	0.005%
91	12.059	3425	3427	3431	rVB3	893	441	0.03%	0.004%
92	12.149	3453	3455	3457	rBV2	549	244	0.02%	0.002%
93	12.403	3531	3534	3537	rBV3	598	425	0.03%	0.004%
94	12.802	3651	3658	3661	rBV5	809	943	0.06%	0.008%
95	13.329	3820	3822	3828	rBV5	673	617	0.04%	0.005%
96	13.358	3828	3831	3834	rVV2	662	400	0.02%	0.003%
97	13.371	3834	3835	3843	rVB3	748	589	0.04%	0.005%
98	13.432	3852	3854	3856	rBV2	584	194	0.01%	0.002%
99	13.670	3926	3928	3929	rBV	612	318	0.02%	0.003%
100	14.654	4232	4234	4237	rBV4	1075	621	0.04%	0.005%




Sum of corrected areas: 12057677

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028057.D
Acq On : 22 Sep 2022 11:25
Operator : SY/MD
Sample : N4674-19DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

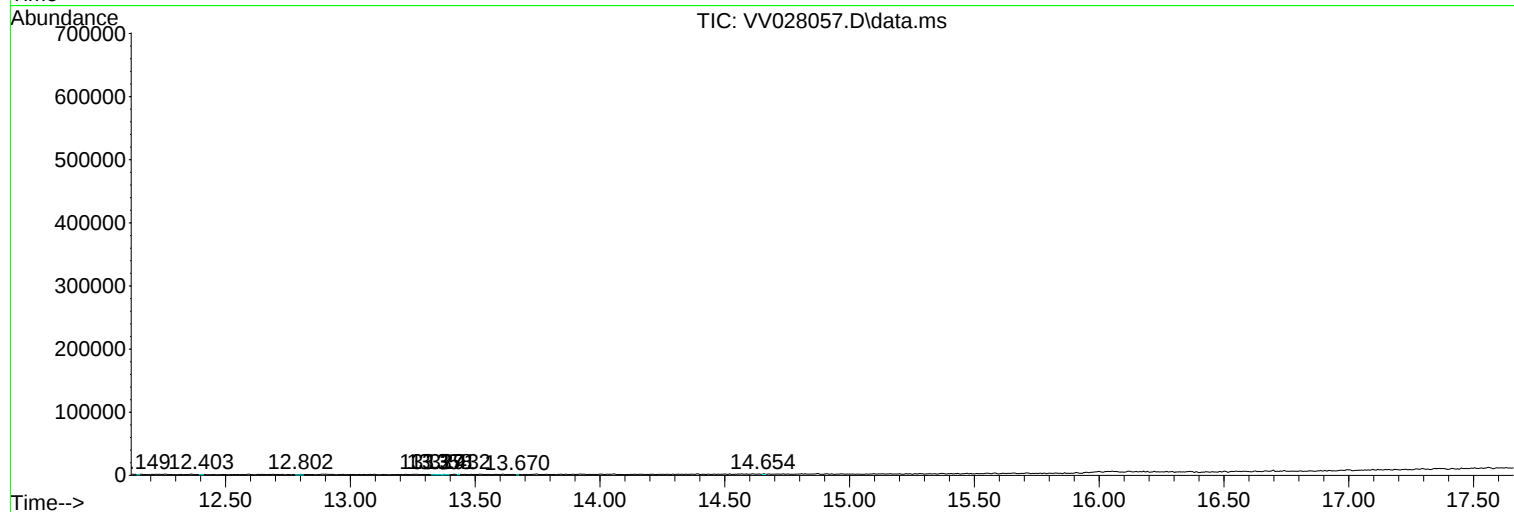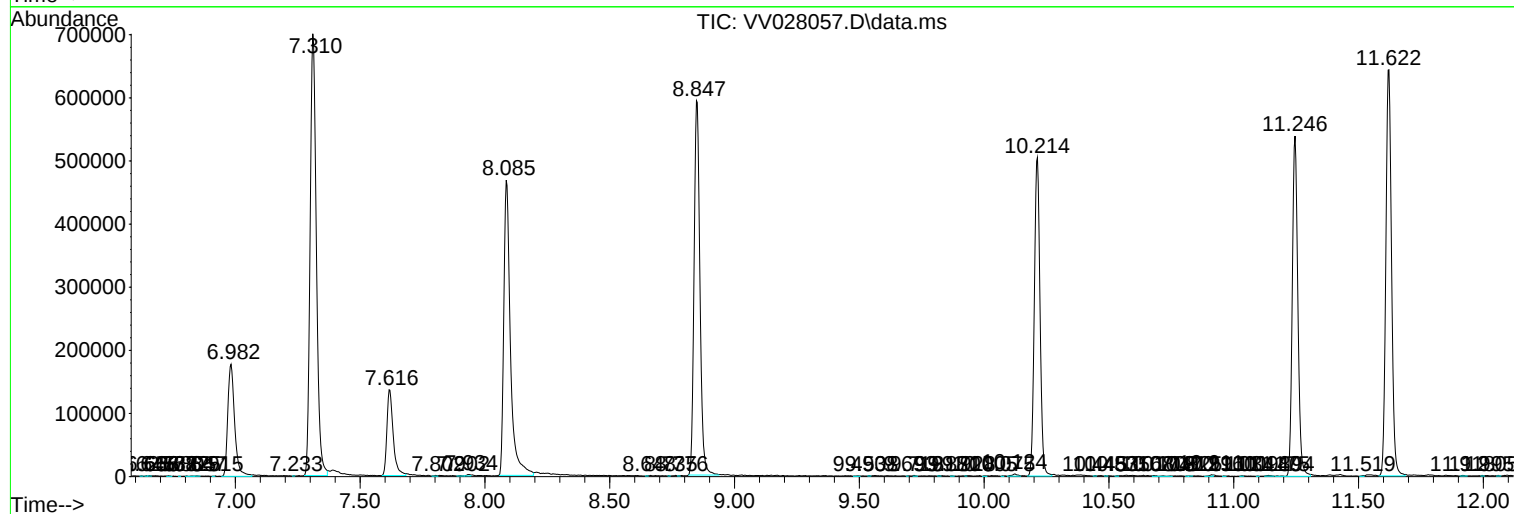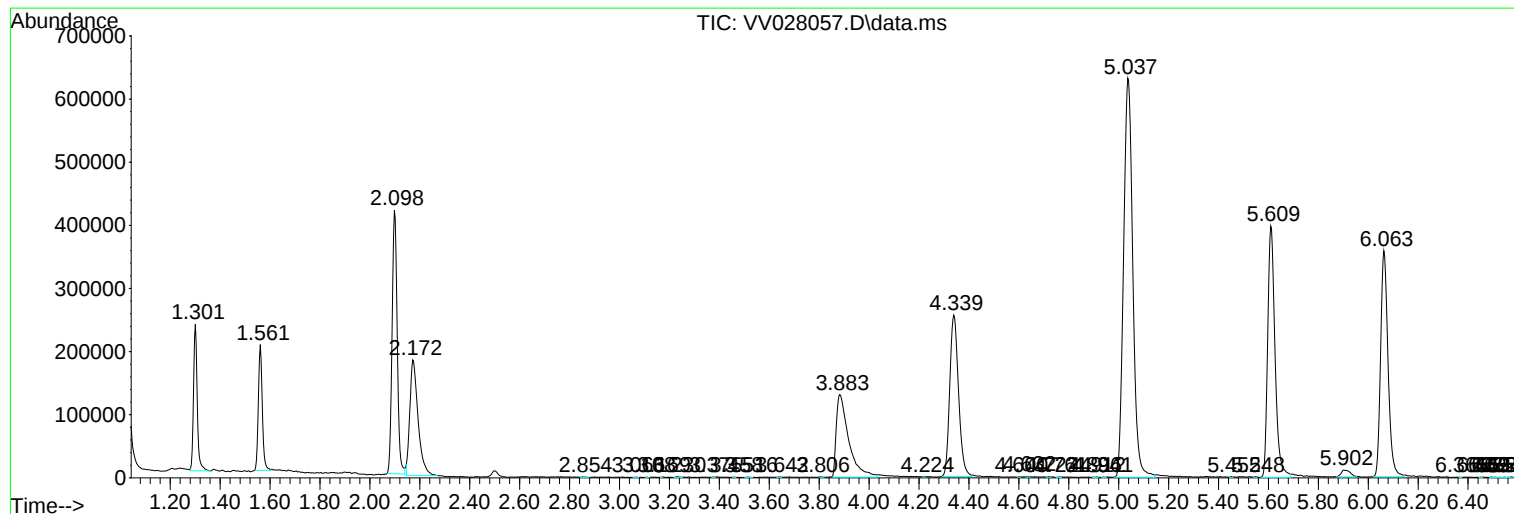

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028057.D
Acq On : 22 Sep 2022 11:25
Operator : SY/MD
Sample : N4674-19DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028057.D
Acq On : 22 Sep 2022 11:25
Operator : SY/MD
Sample : N4674-19DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------