

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028058.D
 Acq On : 22 Sep 2022 11:50
 Operator : SY/MD
 Sample : N4659-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV028058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	245981	254916	15.90%	2.188%
2	1.561	155	162	177	rVB	194060	224622	14.01%	1.928%
3	2.098	320	329	358	rVB	425715	628421	39.21%	5.394%
4	2.433	430	433	436	rBV5	992	948	0.06%	0.008%
5	2.561	469	473	474	rBV3	548	315	0.02%	0.003%
6	2.606	482	487	488	rBV3	1201	931	0.06%	0.008%
7	2.658	500	503	507	rBV4	737	649	0.04%	0.006%
8	2.757	526	534	535	rBV4	1869	1790	0.11%	0.015%
9	2.806	547	549	552	rVB2	773	416	0.03%	0.004%
10	2.896	573	577	578	rBV2	486	255	0.02%	0.002%
11	2.905	578	580	583	rVV2	426	333	0.02%	0.003%
12	2.947	588	593	595	rBV4	699	685	0.04%	0.006%
13	3.024	614	617	621	rVB3	779	530	0.03%	0.005%
14	3.040	621	622	625	rBV2	946	505	0.03%	0.004%
15	3.114	642	645	648	rBV4	745	709	0.04%	0.006%
16	3.179	662	665	667	rBV2	729	468	0.03%	0.004%
17	3.317	705	708	710	rBV3	834	492	0.03%	0.004%
18	3.378	722	727	728	rBV2	677	424	0.03%	0.004%
19	3.400	732	734	738	rBV3	369	349	0.02%	0.003%
20	3.452	745	750	752	rBV3	500	369	0.02%	0.003%
21	3.465	752	754	760	rVV3	483	248	0.02%	0.002%
22	3.548	776	780	785	rBV5	648	659	0.04%	0.006%
23	3.680	818	821	825	rVB2	613	422	0.03%	0.004%
24	3.880	872	883	913	rBV2	147058	457098	28.52%	3.923%
25	4.339	1012	1026	1054	rVB	247735	616204	38.44%	5.289%
26	4.587	1099	1103	1109	rBV7	1178	1544	0.10%	0.013%
27	4.741	1149	1151	1155	rVB3	1023	490	0.03%	0.004%
28	4.780	1160	1163	1166	rVB2	808	469	0.03%	0.004%
29	4.896	1195	1199	1201	rBV2	879	643	0.04%	0.006%
30	5.037	1227	1243	1273	rBV2	622035	1602867	100.00%	13.757%
31	5.474	1376	1379	1381	rVV2	430	281	0.02%	0.002%
32	5.609	1409	1421	1456	rBV	396484	812466	50.69%	6.973%
33	5.799	1478	1480	1482	rBV2	825	360	0.02%	0.003%
34	5.828	1485	1489	1496	rVB5	1235	1193	0.07%	0.010%
35	5.860	1496	1499	1502	rVB3	707	397	0.02%	0.003%
36	5.905	1503	1513	1528	rBV7	7750	17474	1.09%	0.150%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028058.D
 Acq On : 22 Sep 2022 11:50
 Operator : SY/MD
 Sample : N4659-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.063	1547	1562	1584	rBV	329520	685053	42.74%	5.880%
38	6.262	1621	1624	1629	rVB3	804	521	0.03%	0.004%
39	6.339	1646	1648	1650	rBV2	504	210	0.01%	0.002%
40	6.375	1654	1659	1661	rBV3	883	881	0.05%	0.008%
41	6.497	1695	1697	1698	rBV2	682	325	0.02%	0.003%
42	6.523	1703	1705	1707	rVV2	834	274	0.02%	0.002%
43	6.603	1726	1730	1733	rVB4	944	687	0.04%	0.006%
44	6.619	1733	1735	1738	rBV3	620	469	0.03%	0.004%
45	6.741	1771	1773	1776	rVB	475	222	0.01%	0.002%
46	6.867	1808	1812	1813	rVV2	583	353	0.02%	0.003%
47	6.908	1823	1825	1827	rBV	516	211	0.01%	0.002%
48	6.931	1830	1832	1833	rBV2	792	258	0.02%	0.002%
49	6.982	1837	1848	1874	rBV	172868	322456	20.12%	2.768%
50	7.310	1939	1950	1970	rBV	686710	1205245	75.19%	10.345%
51	7.619	2036	2046	2066	rBV	123470	221322	13.81%	1.900%
52	7.789	2095	2099	2102	rBV5	901	865	0.05%	0.007%
53	8.040	2172	2177	2178	rBV3	717	537	0.03%	0.005%
54	8.085	2181	2191	2231	rBV	478855	898369	56.05%	7.711%
55	8.641	2362	2364	2366	rBV2	687	289	0.02%	0.002%
56	8.702	2381	2383	2386	rVB2	634	303	0.02%	0.003%
57	8.847	2417	2428	2458	rBV	613589	1007245	62.84%	8.645%
58	9.297	2566	2568	2569	rBV	542	219	0.01%	0.002%
59	9.368	2588	2590	2594	rBV	433	356	0.02%	0.003%
60	9.468	2619	2621	2624	rVB4	926	472	0.03%	0.004%
61	9.702	2692	2694	2698	rBV2	1007	841	0.05%	0.007%
62	9.722	2698	2700	2702	rVV3	556	281	0.02%	0.002%
63	9.773	2714	2716	2718	rBV	879	355	0.02%	0.003%
64	9.812	2723	2728	2729	rBV2	550	444	0.03%	0.004%
65	9.886	2749	2751	2756	rBV2	379	278	0.02%	0.002%
66	10.001	2786	2787	2791	rBV3	463	274	0.02%	0.002%
67	10.127	2819	2826	2830	rBV5	2030	2261	0.14%	0.019%
68	10.210	2840	2852	2869	rBV	482772	764307	47.68%	6.560%
69	10.384	2905	2906	2909	rVB2	1066	448	0.03%	0.004%
70	10.432	2916	2921	2922	rBV2	559	358	0.02%	0.003%
71	10.657	2986	2991	2995	rVV2	405	405	0.03%	0.003%
72	10.722	3005	3011	3015	rBV3	894	840	0.05%	0.007%
73	10.757	3020	3022	3025	rBV2	415	253	0.02%	0.002%
74	10.780	3027	3029	3031	rVB2	619	286	0.02%	0.002%
75	10.799	3031	3035	3038	rBV2	620	403	0.03%	0.003%
76	10.815	3038	3040	3042	rBV2	476	262	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028058.D
 Acq On : 22 Sep 2022 11:50
 Operator : SY/MD
 Sample : N4659-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.828	3042	3044	3046	rVV3	783	336	0.02%	0.003%
78	10.844	3046	3049	3052	rVV3	403	304	0.02%	0.003%
79	10.860	3052	3054	3058	rVB4	825	474	0.03%	0.004%
80	11.011	3098	3101	3102	rBV	552	245	0.02%	0.002%
81	11.104	3125	3130	3132	rBV3	559	530	0.03%	0.005%
82	11.140	3138	3141	3144	rBV3	1443	1186	0.07%	0.010%
83	11.185	3151	3155	3163	rVB7	1403	1723	0.11%	0.015%
84	11.246	3163	3174	3192	rBV	549552	848595	52.94%	7.283%
85	11.538	3260	3265	3267	rBV3	1038	934	0.06%	0.008%
86	11.622	3279	3291	3310	rBV	653396	1036370	64.66%	8.895%
87	11.873	3366	3369	3370	rBV2	878	406	0.03%	0.003%
88	12.030	3415	3418	3421	rBV2	734	561	0.03%	0.005%
89	12.156	3455	3457	3460	rBV2	442	295	0.02%	0.003%
90	12.323	3507	3509	3510	rBV	513	226	0.01%	0.002%
91	12.480	3556	3558	3560	rBV2	536	276	0.02%	0.002%
92	12.542	3575	3577	3583	rBV5	948	604	0.04%	0.005%
93	12.693	3621	3624	3629	rBV3	557	578	0.04%	0.005%
94	13.124	3754	3758	3760	rBV2	821	658	0.04%	0.006%
95	13.268	3799	3803	3806	rBV4	1275	974	0.06%	0.008%
96	13.333	3821	3823	3827	rBV2	752	608	0.04%	0.005%
97	13.516	3869	3880	3884	rBV7	1591	3161	0.20%	0.027%
98	13.747	3949	3952	3954	rBV3	1069	627	0.04%	0.005%
99	14.091	4057	4059	4064	rBV2	842	732	0.05%	0.006%
100	14.230	4100	4102	4105	rBV2	619	257	0.02%	0.002%




Sum of corrected areas: 11651040

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028058.D
Acq On : 22 Sep 2022 11:50
Operator : SY/MD
Sample : N4659-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

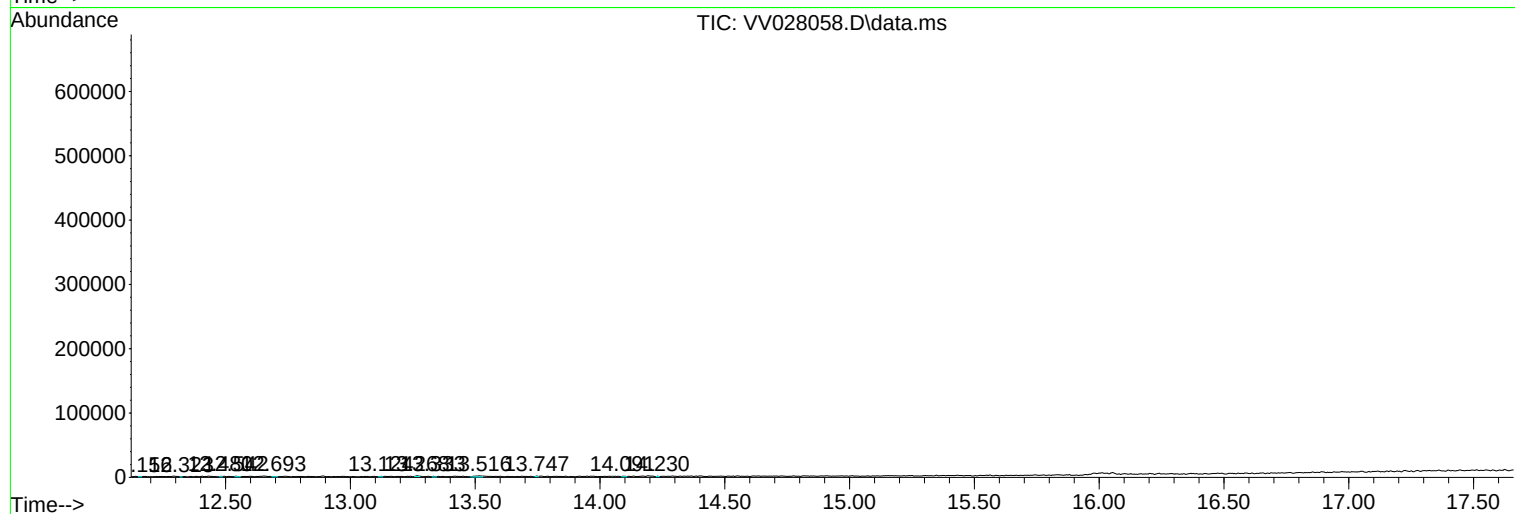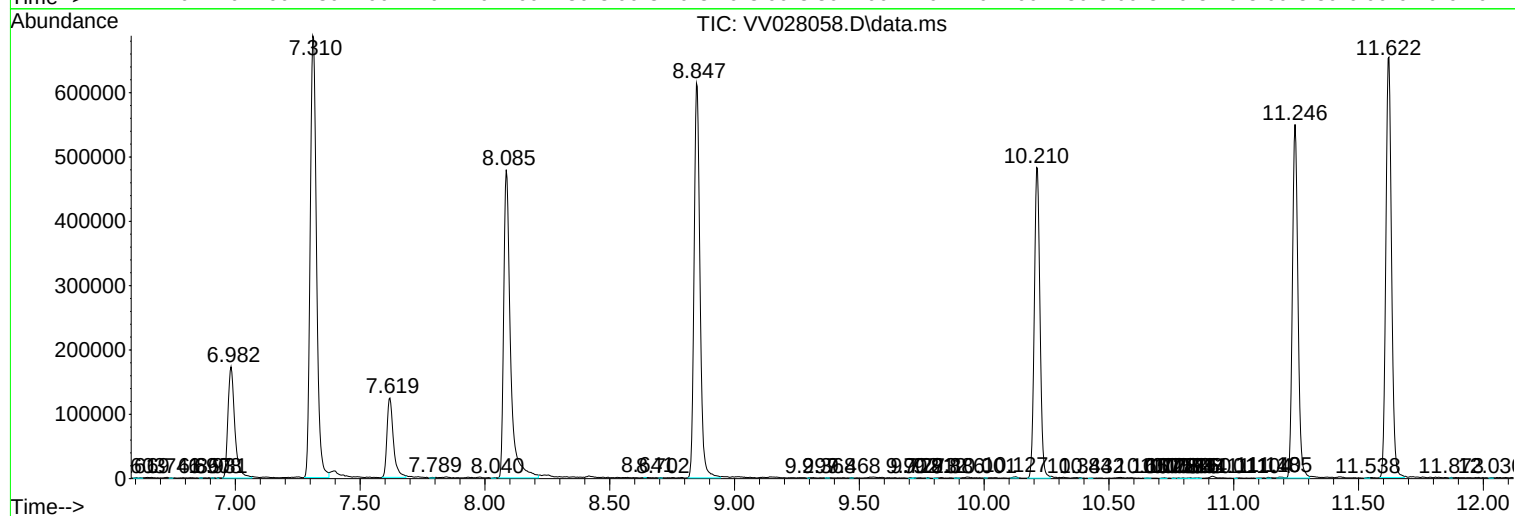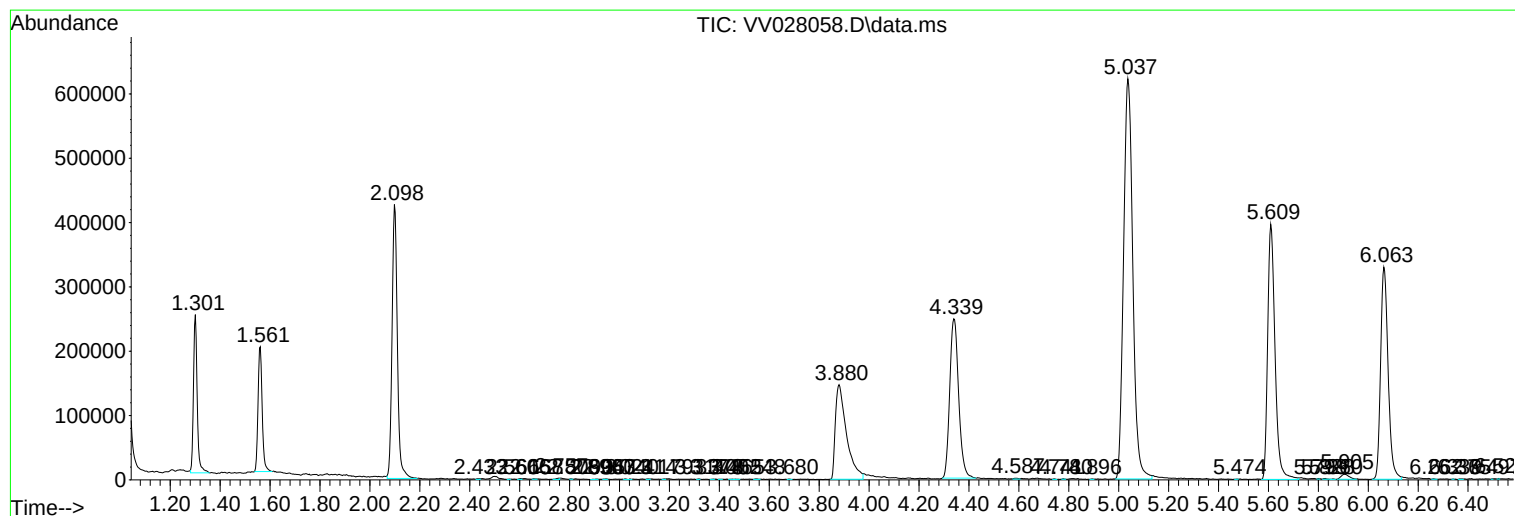

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028058.D
Acq On : 22 Sep 2022 11:50
Operator : SY/MD
Sample : N4659-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028058.D
Acq On : 22 Sep 2022 11:50
Operator : SY/MD
Sample : N4659-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
